


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
 Data File : BF129081.D
 Acq On : 01 Jul 2022 09:11
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 29 17:05:31 2022

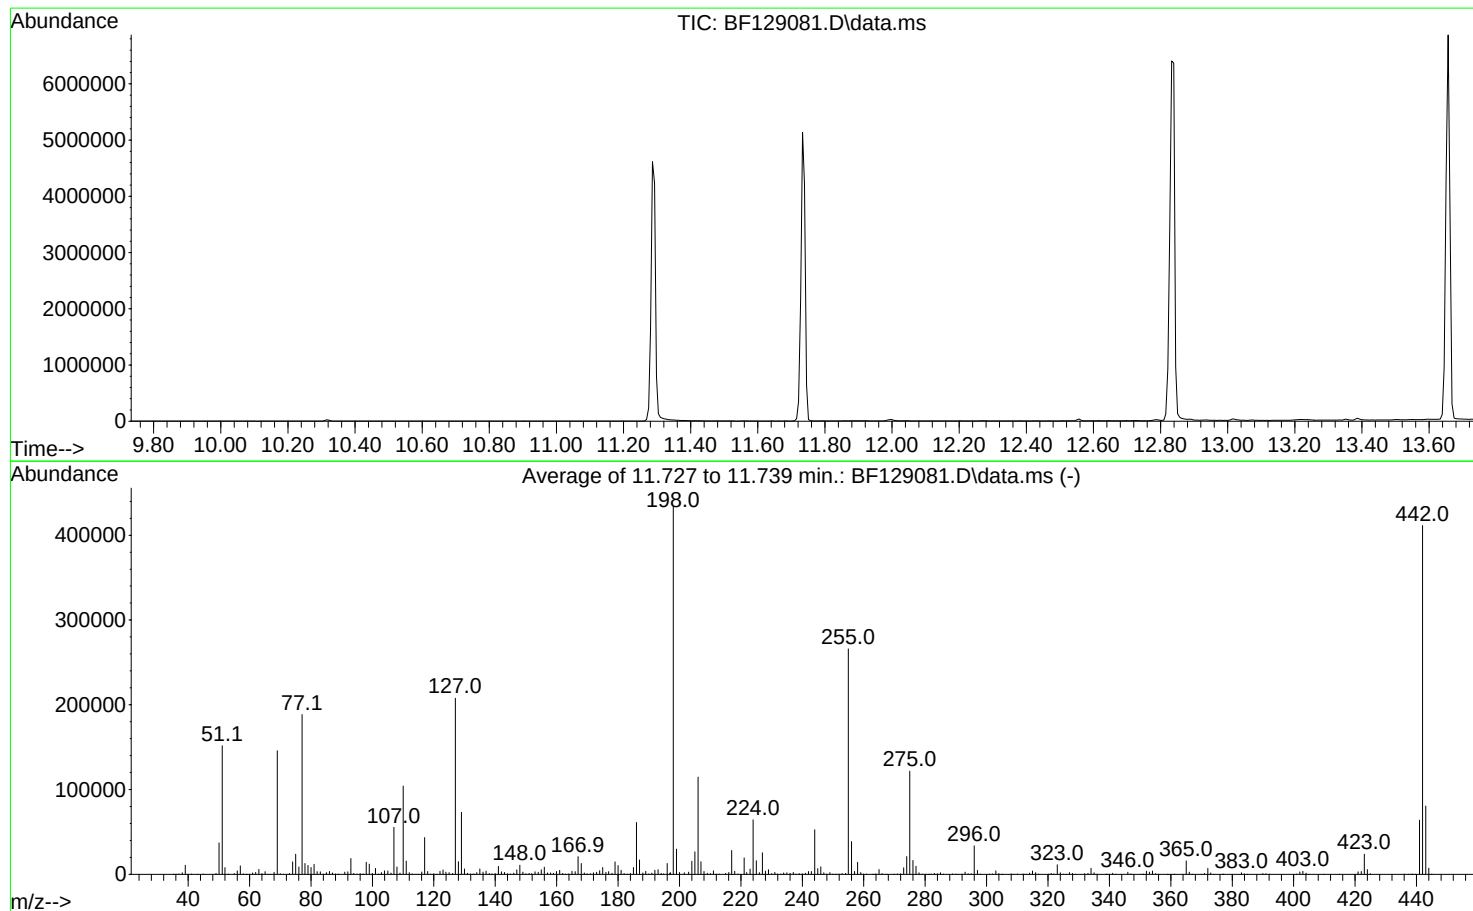




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	151744	PASS
68	69	0.00	2	1.6	2372	PASS
69	198	0.00	100	33.6	145997	PASS
70	69	0.00	2	0.6	823	PASS
127	198	10	80	47.9	207787	PASS
197	198	0.00	2	0.5	2160	PASS
198	198	100	100	100.0	433899	PASS
199	198	5	9	6.9	29861	PASS
275	198	10	60	28.1	121811	PASS
365	198	1	100	3.6	15787	PASS
441	198	0.01	100	14.7	63927	PASS
442	442	50	100	100.0	411475	PASS
443	442	15	24	19.6	80595	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
Data File : BF129081.D
Acq On : 01 Jul 2022 09:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 02 03:59:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

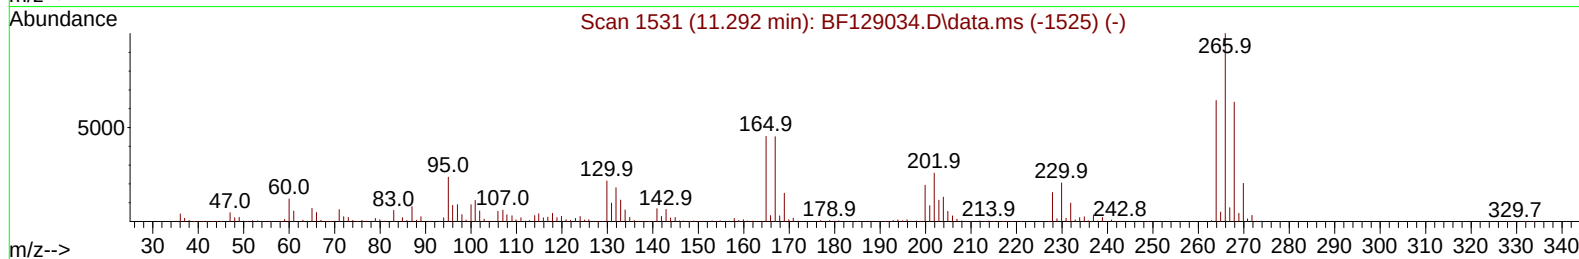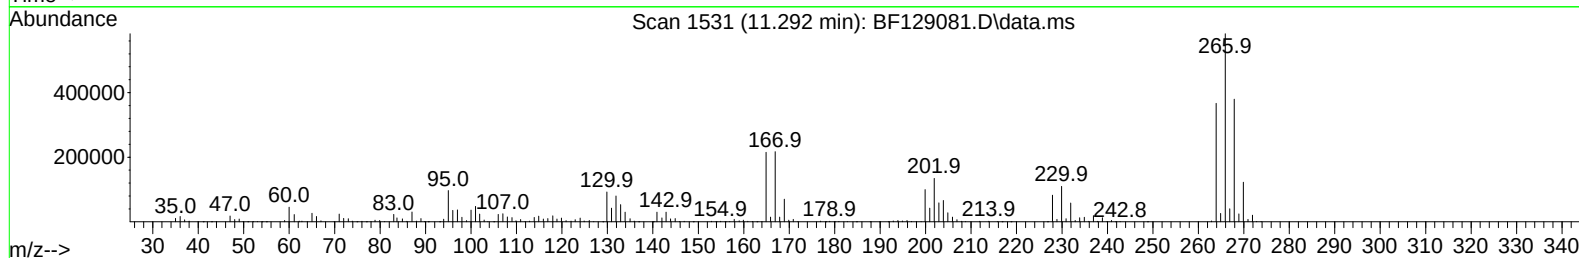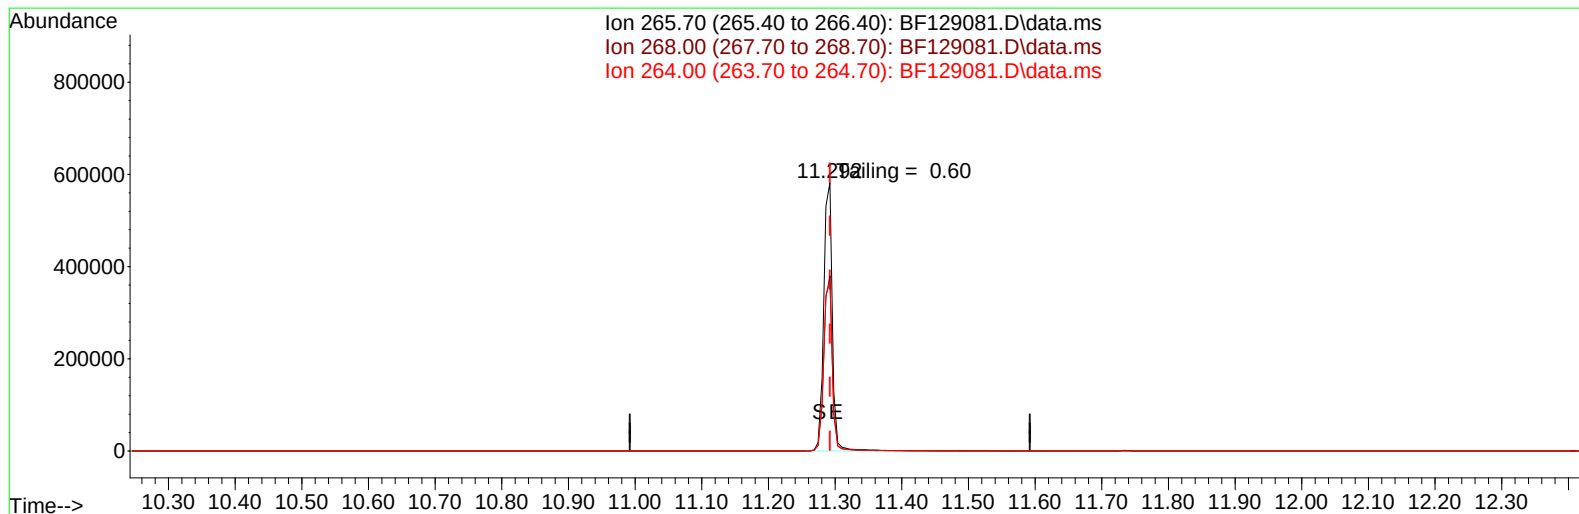

TIC: BF129081.D\data.ms

(70) Pentachlorophenol (C)

11.292min (-0.000) 183959.80 ng




response 524329

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	65.18
264.00	61.80	62.97
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\  
Data File : BF129081.D  
Acq On    : 01 Jul 2022  09:11  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 02 03:59:12 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jun 29 17:05:31 2022
Response via : Initial Calibration

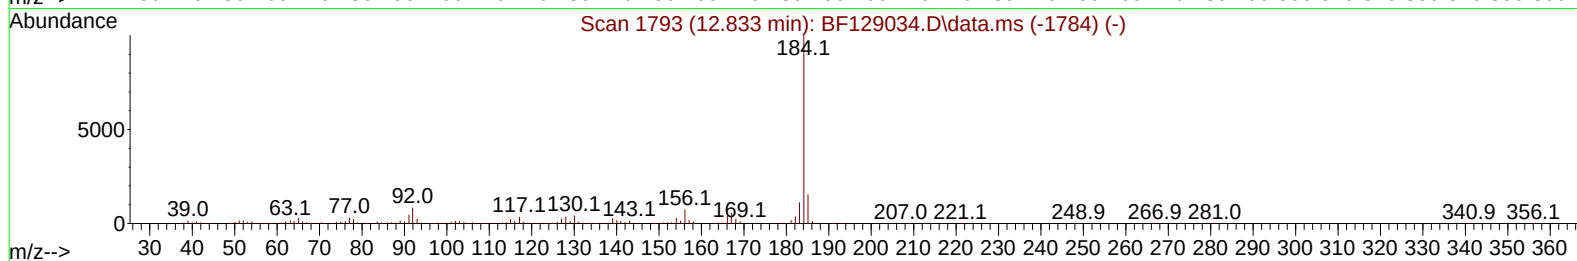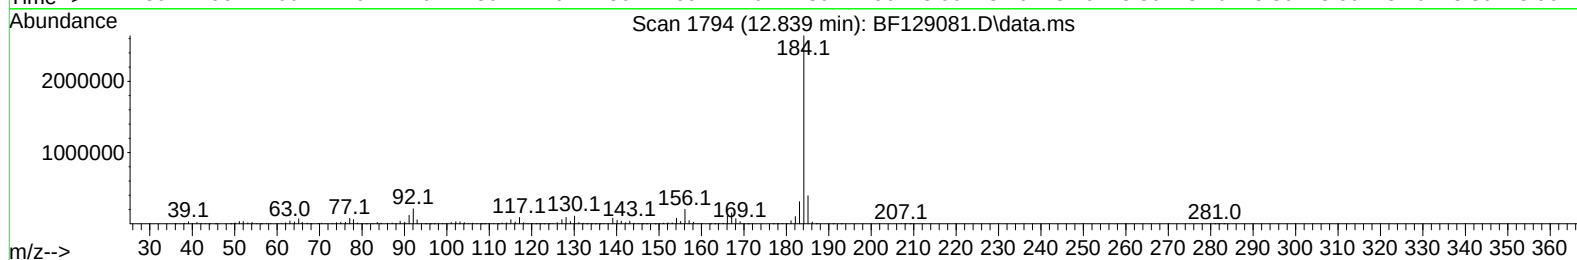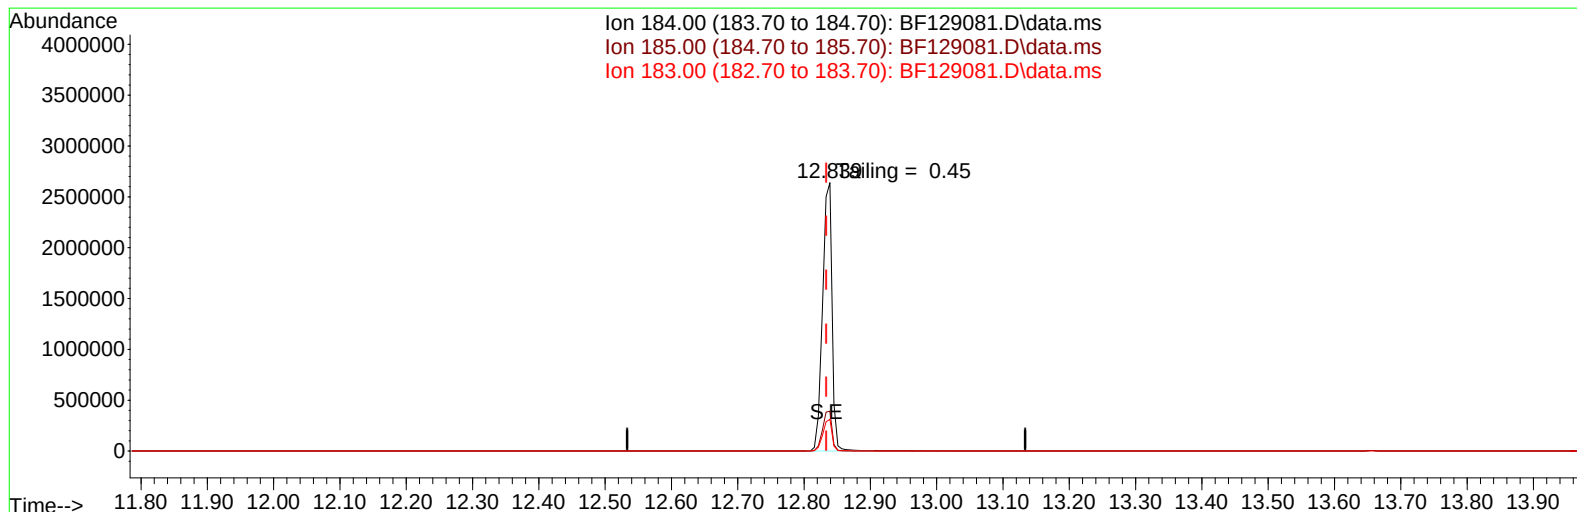

TIC: BF129081.D\data.ms

(77) Benzidine

12.839min (+ 0.006) 238953.64 ng

response **2646541**

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00	14.90	14.89
--------	-------	-------

183.00	11.60	11.79
--------	-------	-------

0.00 0.00 0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/1/2022	BNA_F	<u>BF129081.D</u>
Compound Name	Response	Retention Time
DDT	1099615	13.657
DDD	6494	13.386
DDE	4488	13.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10982	1110597	0.99

Instrument :
BNA_F
ClientSampleId :
DFTPP