


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
 Data File : BF129091.D
 Acq On : 01 Jul 2022 14:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jun 29 17:05:31 2022

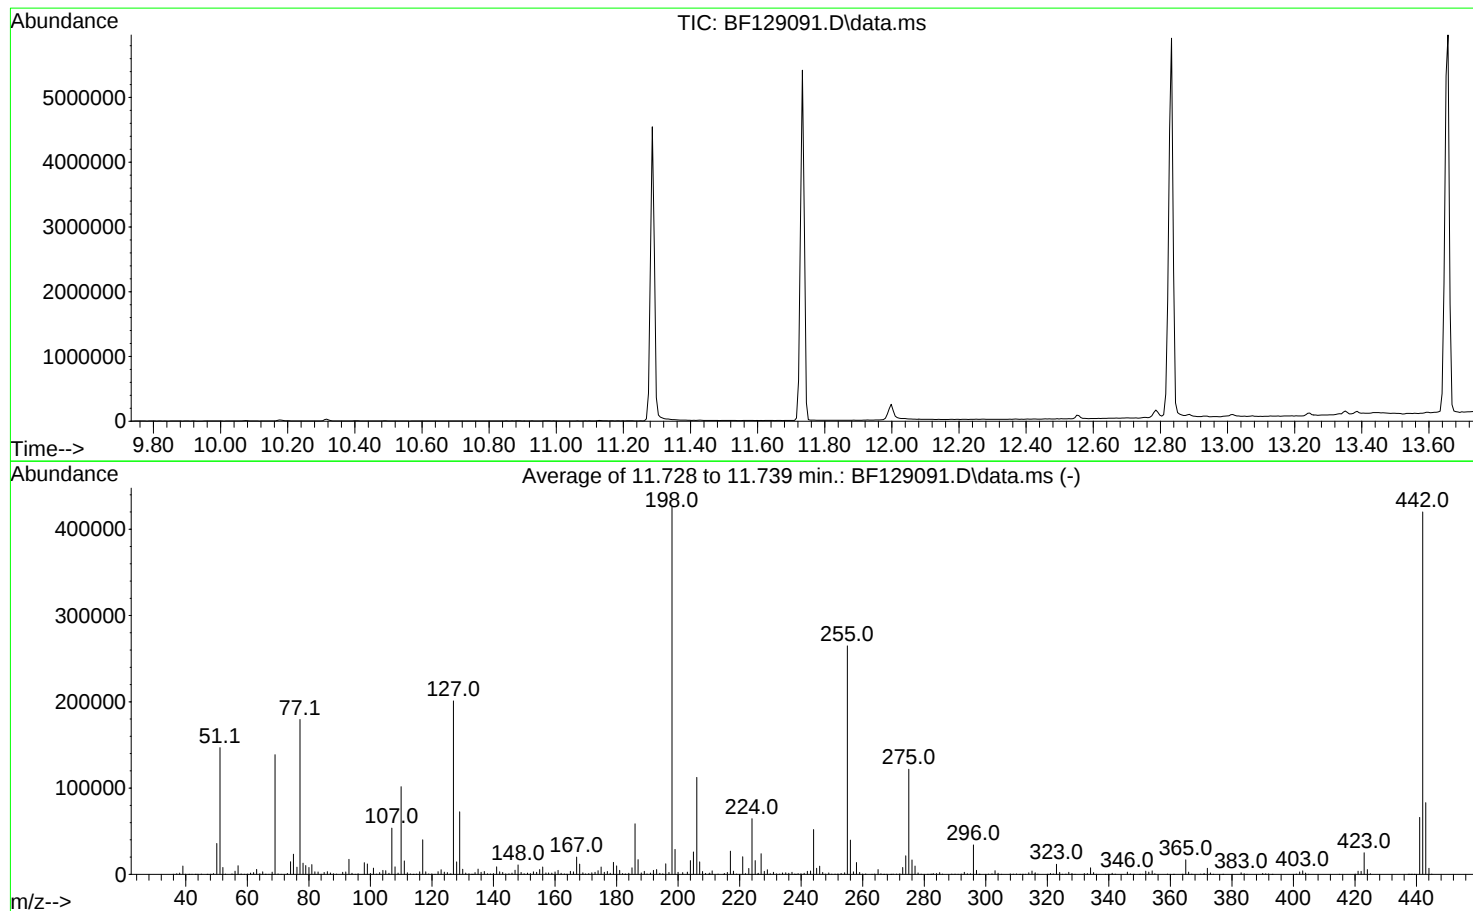




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	146835	PASS
68	69	0.00	2	1.8	2531	PASS
69	198	0.00	100	32.5	138676	PASS
70	69	0.00	2	0.4	581	PASS
127	198	10	80	47.1	200968	PASS
197	198	0.00	2	0.5	2197	PASS
198	198	100	100	100.0	426389	PASS
199	198	5	9	6.8	28877	PASS
275	198	10	60	28.6	121872	PASS
365	198	1	100	4.0	16931	PASS
441	198	0.01	100	15.5	66064	PASS
442	442	50	100	100.0	420117	PASS
443	442	15	24	19.8	83032	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
 Data File : BF129091.D
 Acq On : 01 Jul 2022 14:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 02 04:02:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:05:31 2022
 Response via : Initial Calibration

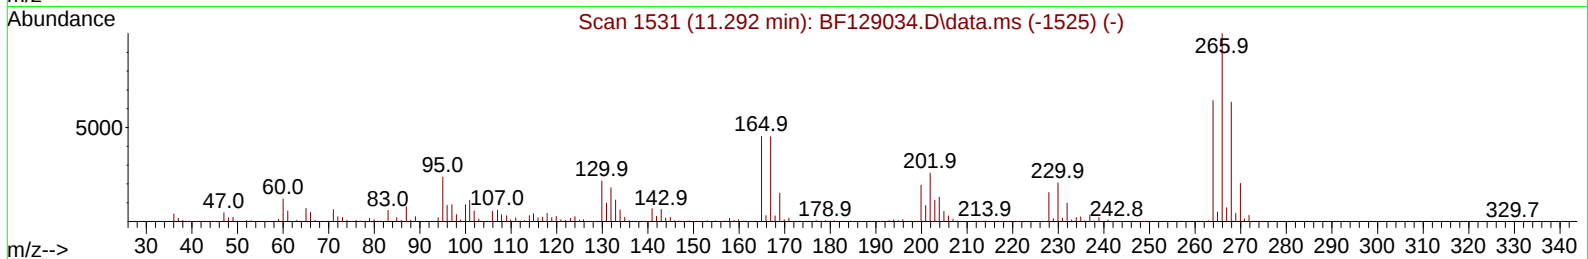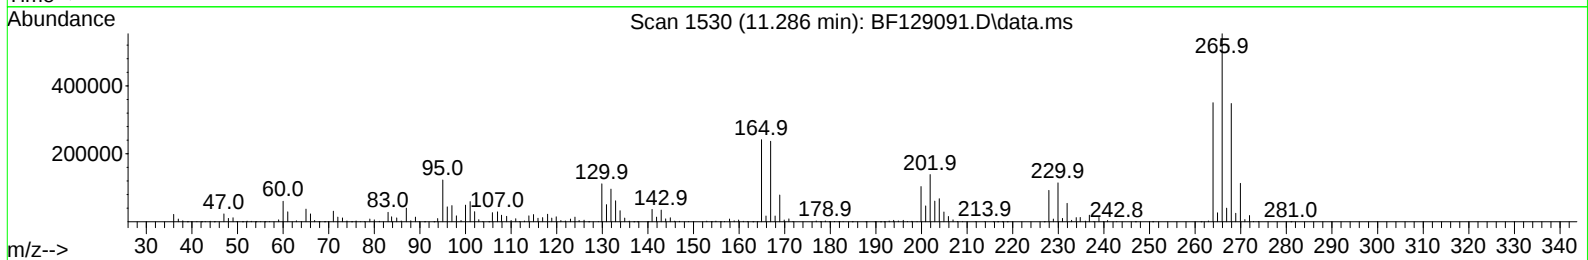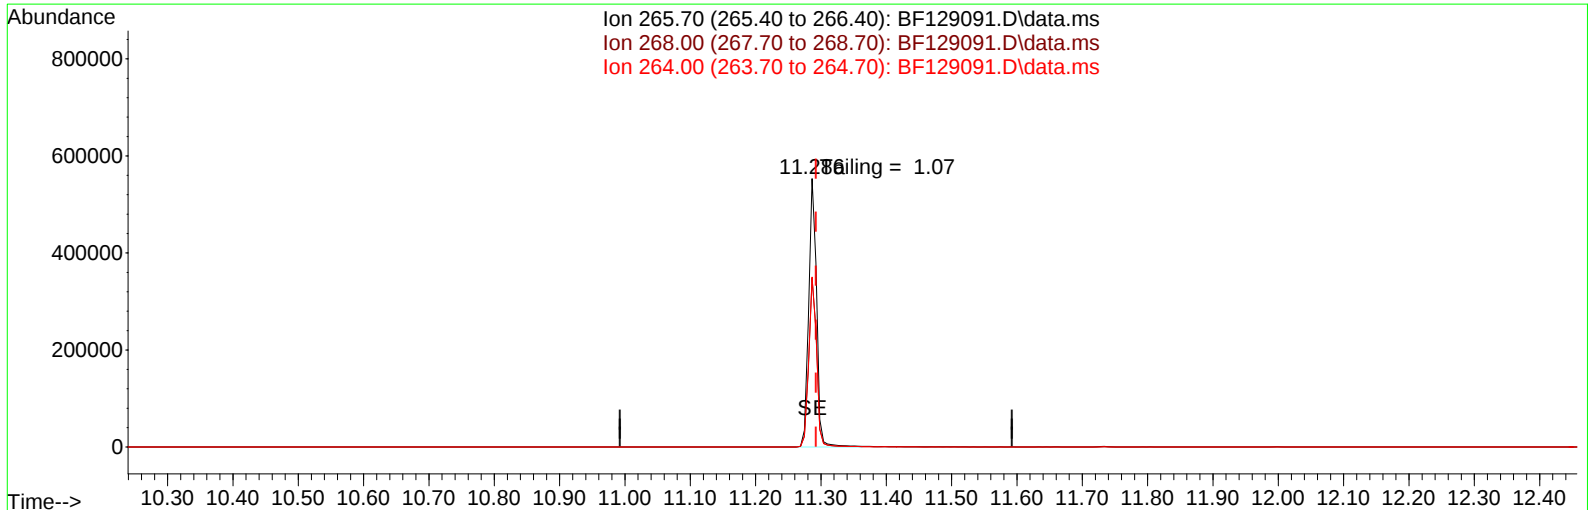

TIC: BF129091.D\data.ms

(70) Pentachlorophenol (C)

11.286min (-0.006) 145792.17 ng




response 471085

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.89
264.00	61.80	63.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070122\
 Data File : BF129091.D
 Acq On : 01 Jul 2022 14:30
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 02 04:02:35 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jun 29 17:05:31 2022
 Response via : Initial Calibration

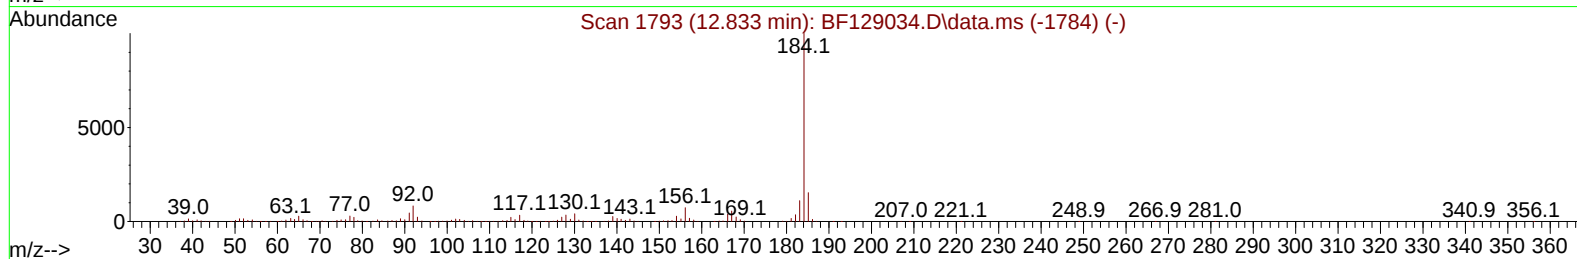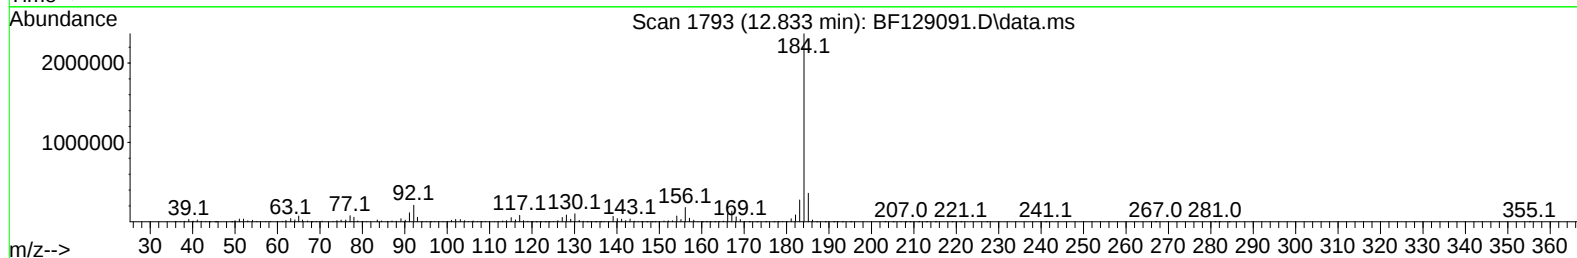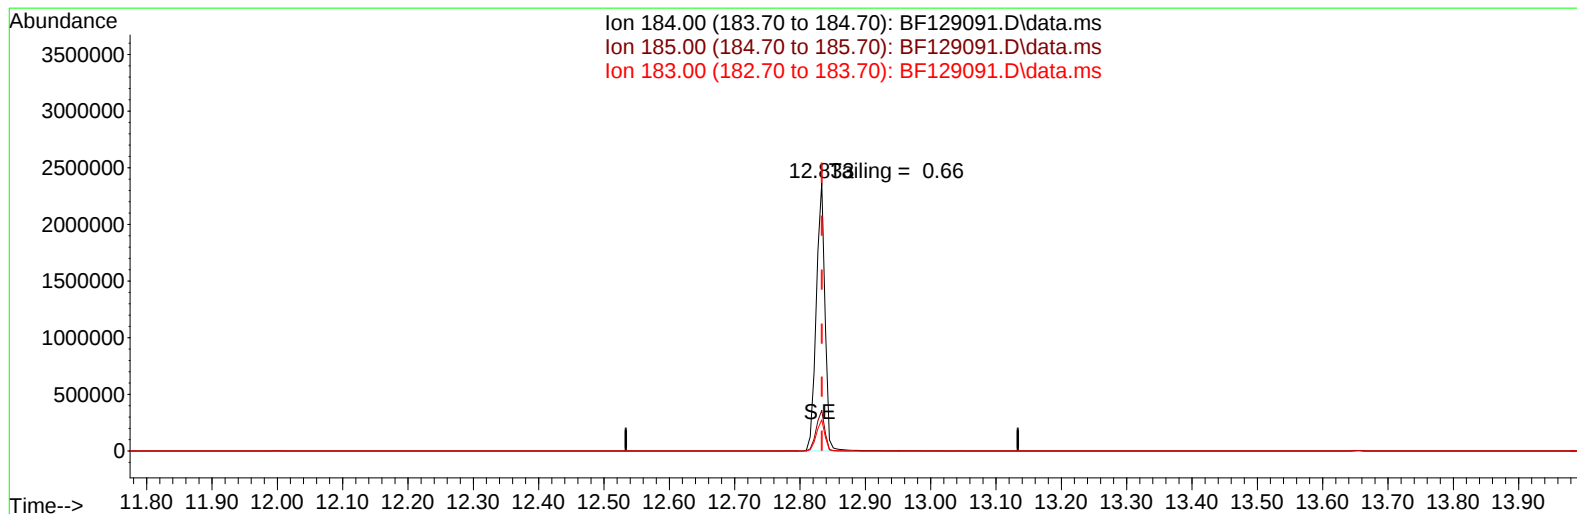

TIC: BF129091.D\data.ms

(77) Benzidine

12.833min (0.000) 124218.79 ng

response 2205246

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	15.18
183.00	11.60	11.63
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/1/2022	BNA_F	<u>BF129091.D</u>
Compound Name	Response	Retention Time
DDT	1056195	13.657
DDD	13288	13.351
DDE	4549	13.016
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17837	1074032	1.66

Instrument :
BNA_F
ClientSampleId :
DFTPP