
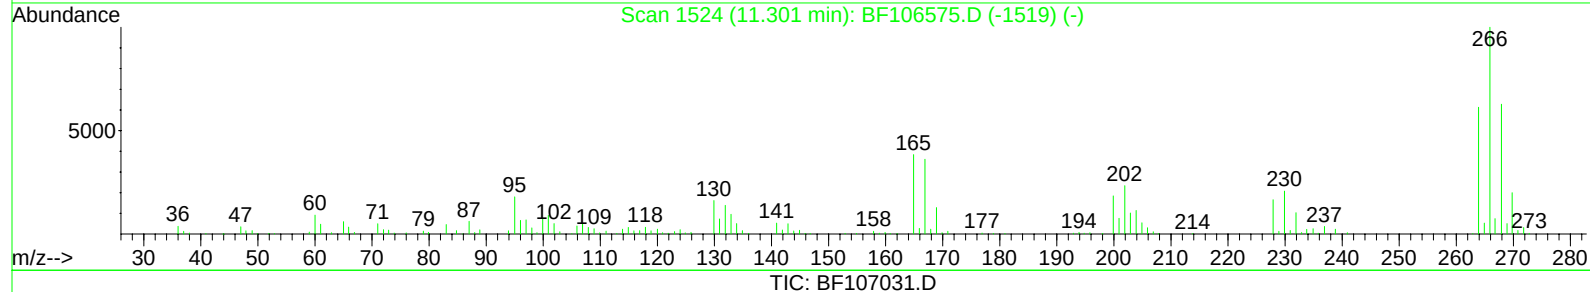
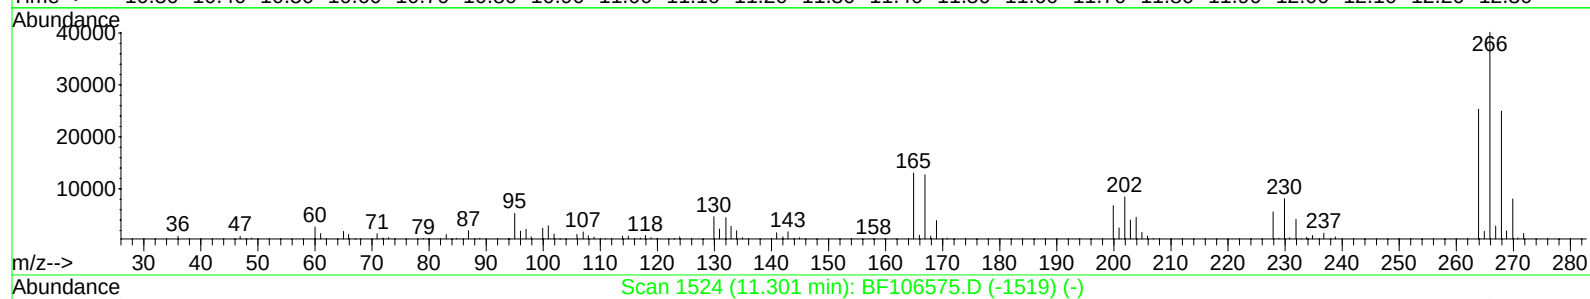


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF070218\
Data File : BF107031.D
Acq On : 2 Jul 2018 8:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 16:02:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

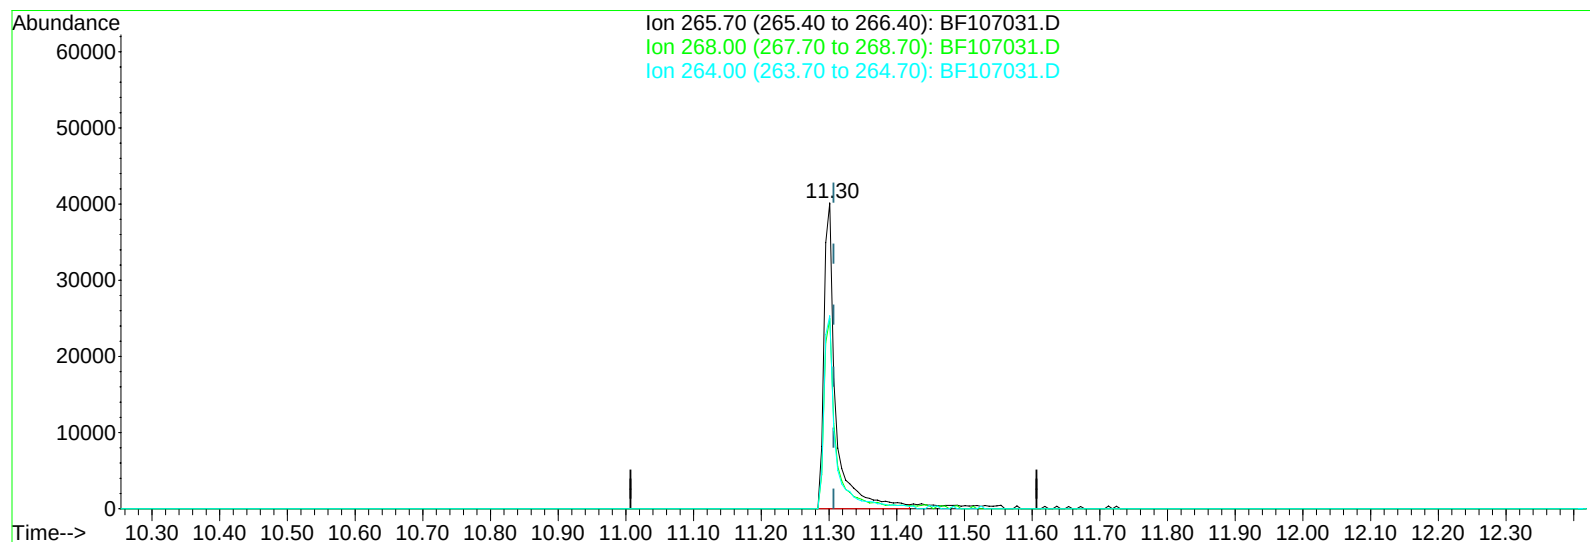

(69) Pentachlorophenol (C)




11.301min (-0.006) 29605.91ng

response 48898

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.22
264.00	61.90	63.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF070218\
Data File : BF107031.D
Acq On : 2 Jul 2018 8:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 16:02:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

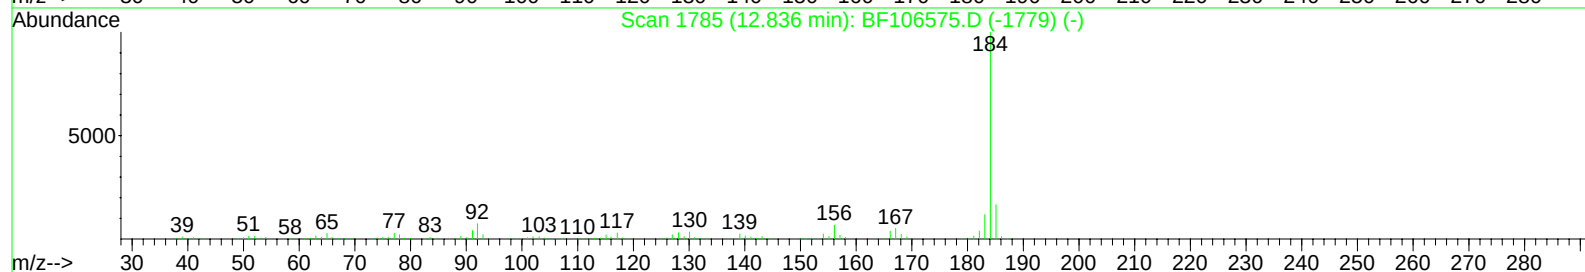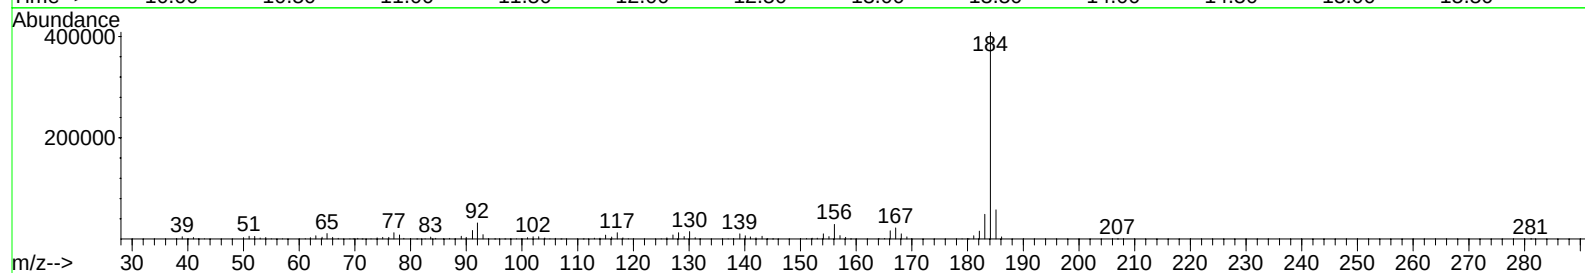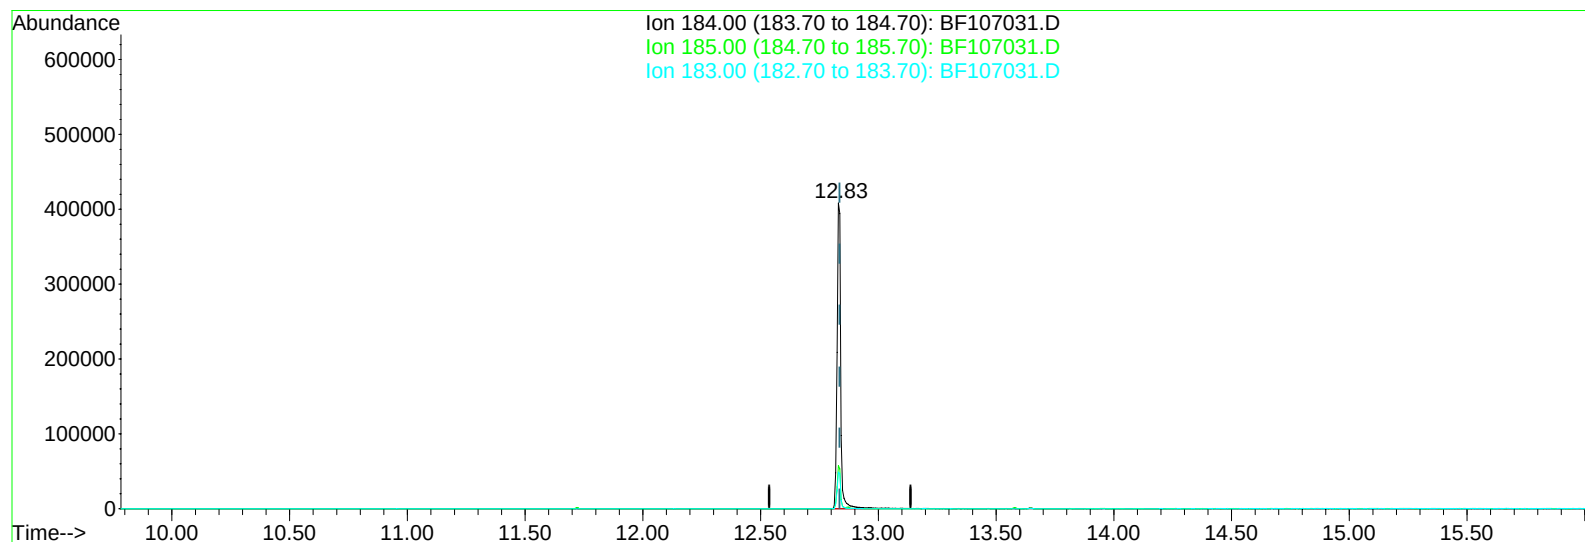

TIC: BF107031.D

(76) Benzidine

12.830min (-0.006) 0.00ng

response 445260

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.14
183.00	11.60	11.98
0.00	0.00	0.00