
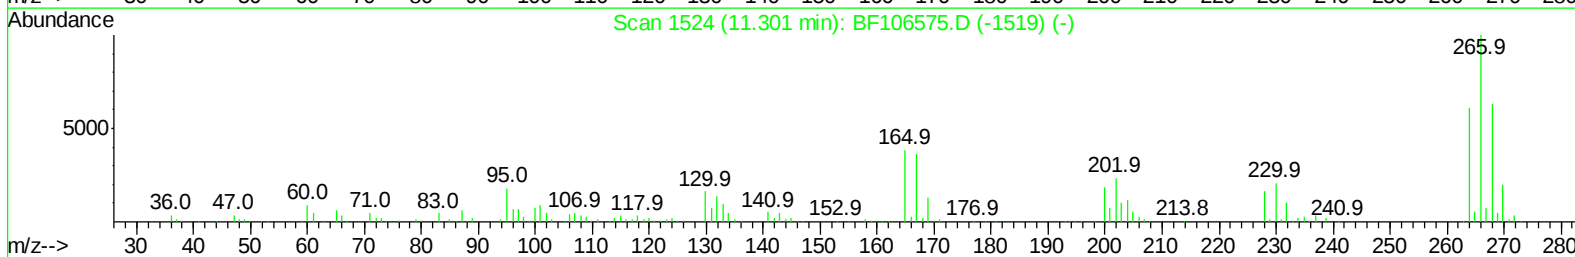
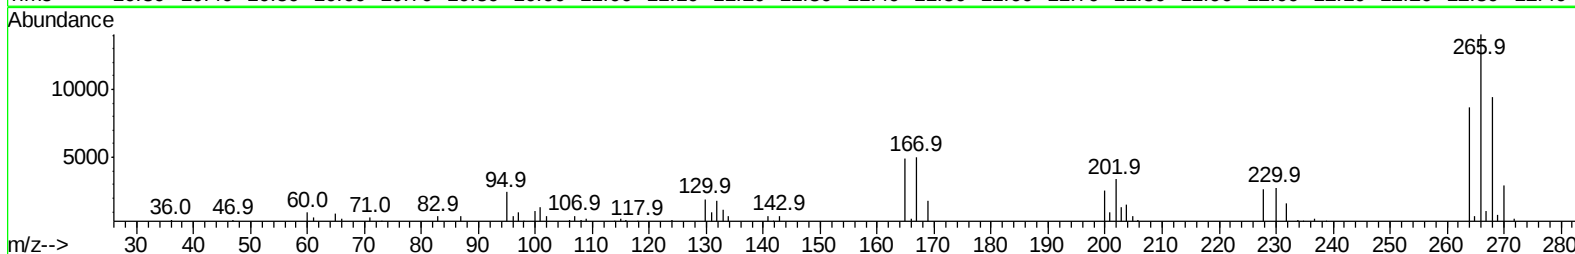


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF070218\
Data File : BF107057.D
Acq On : 2 Jul 2018 21:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 07:48:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

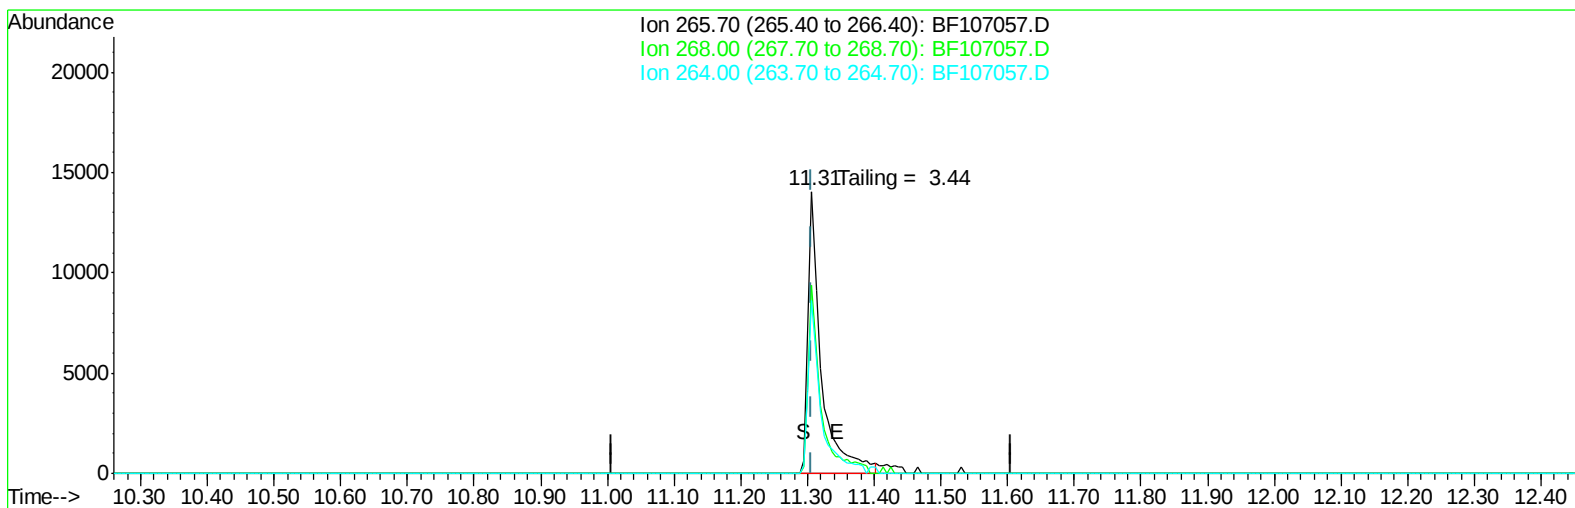

TIC: BF107057.D

(69) Pentachlorophenol (C)




11.307min (-0.000) 24214.01ng

response 19619

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.85
264.00	61.90	61.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF070218\
Data File : BF107057.D
Acq On : 2 Jul 2018 21:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 07:48:48 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

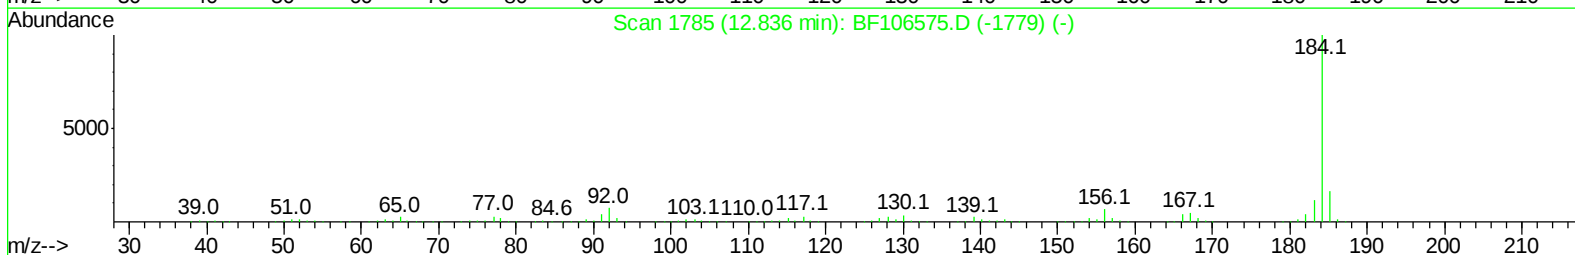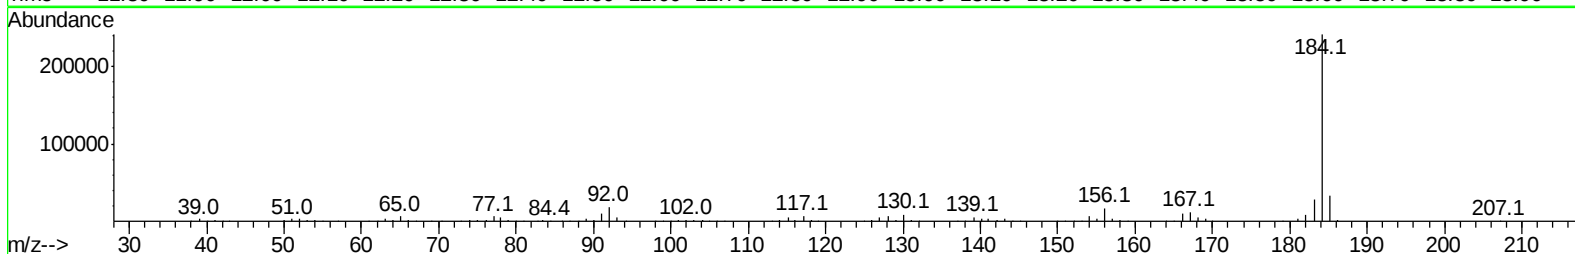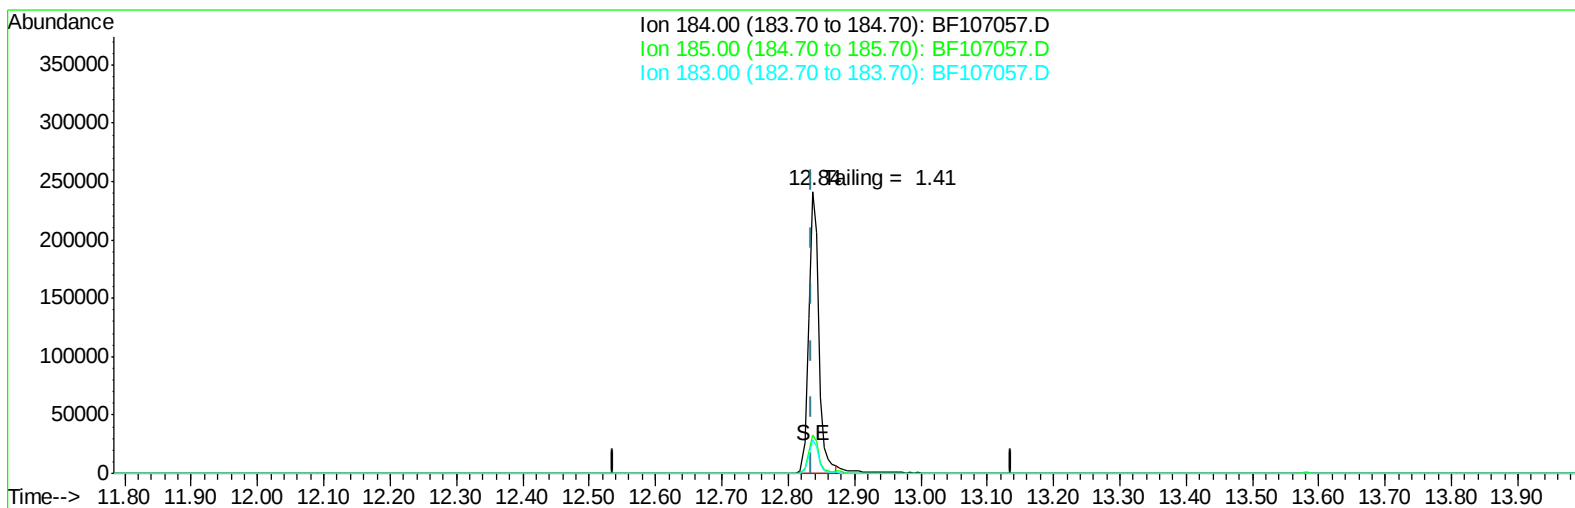

TIC: BF107057.D

(76) Benzidine

12.836min (-0.000) 0.00ng

response 265431

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.56
183.00	11.60	11.74
0.00	0.00	0.00