

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070218\
 Data File : BF107048.D
 Acq On : 2 Jul 2018 17:00
 Operator : JU/SJ
 Sample : J3629-08
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 A0C10-03

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.178	480	483	491	rBV	21581	25250	5.10%	0.545%
2	5.595	551	554	567	rBV	265542	282681	57.10%	6.104%
3	6.601	722	725	730	rBV	257132	262324	52.99%	5.665%
4	6.731	744	747	752	rBV	355830	299461	60.49%	6.466%
5	6.954	782	785	789	rBV	474993	375670	75.89%	8.112%
6	7.107	808	811	818	rBV	265183	247539	50.00%	5.345%
7	7.519	877	881	890	rBV	170354	167938	33.92%	3.626%
8	8.236	1000	1003	1009	rBV	465611	457650	92.45%	9.882%
9	9.307	1182	1185	1194	rBV	323989	348126	70.32%	7.517%
10	9.707	1248	1253	1257	rBV	22244	29454	5.95%	0.636%
11	9.901	1284	1286	1289	rVB2	12728	11270	2.28%	0.243%
12	10.001	1299	1303	1315	rVB	501142	489847	98.95%	10.578%
13	10.401	1369	1371	1375	rVB3	16723	14060	2.84%	0.304%
14	10.795	1434	1438	1445	rBV	180375	168621	34.06%	3.641%
15	10.878	1449	1452	1456	rBV2	12751	17937	3.62%	0.387%
16	10.960	1463	1466	1469	rBV	17823	19121	3.86%	0.413%
17	10.989	1469	1471	1475	rVB2	20291	24169	4.88%	0.522%
18	11.025	1475	1477	1480	rBV	19512	15296	3.09%	0.330%
19	11.142	1493	1497	1500	rBV3	16010	18137	3.66%	0.392%
20	11.177	1500	1503	1505	rVV	18450	14924	3.01%	0.322%
21	11.219	1508	1510	1514	rVB	12552	9742	1.97%	0.210%
22	11.354	1530	1533	1536	rBV3	10332	11128	2.25%	0.240%
23	11.495	1553	1557	1565	rBV	544051	495042	100.00%	10.690%
24	11.830	1611	1614	1616	rVB4	9610	9822	1.98%	0.212%
25	12.713	1762	1764	1767	rBV	29053	28923	5.84%	0.625%
26	13.077	1822	1826	1829	rBV	394183	355313	71.77%	7.672%
27	13.254	1854	1856	1860	rBV4	36459	52311	10.57%	1.130%
28	14.154	2006	2009	2013	rBV	413778	379259	76.61%	8.190%


Sum of corrected areas: 4631015

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070218\
Data File : BF107048.D
Acq On : 2 Jul 2018 17:00
Operator : JU/SJ
Sample : J3629-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A0C10-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

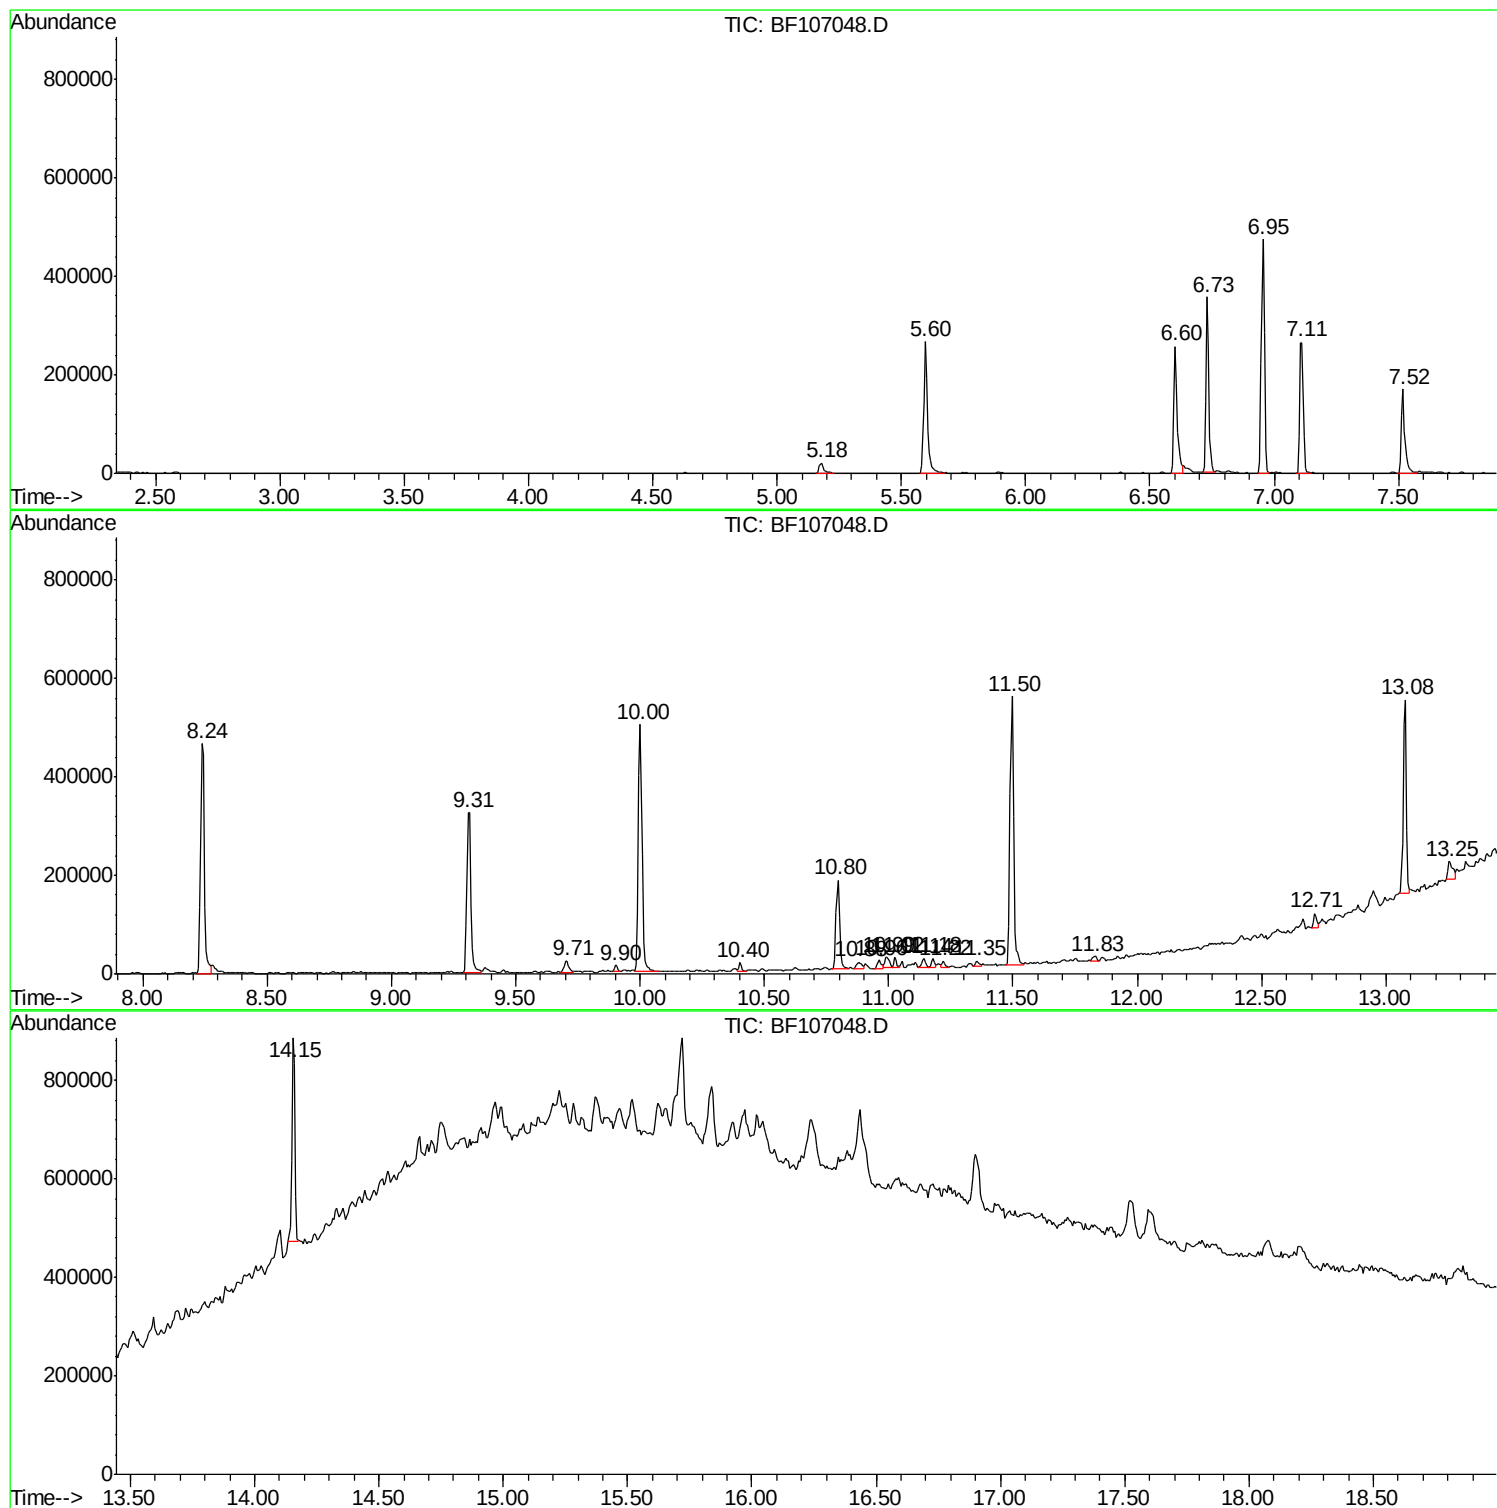

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070218\
Data File : BF107048.D
Acq On : 2 Jul 2018 17:00
Operator : JU/SJ
Sample : J3629-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A0C10-03










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.73 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.73	15.94 ng	299461	1,4-Dichlorobenzene-d4	6.95

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		Imidazole, 4,5-dicyano-1-methyl-	132	C6H4N4	019485-35-9	9

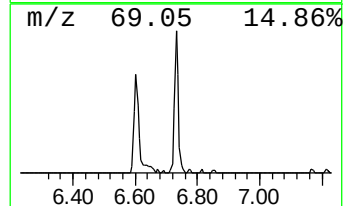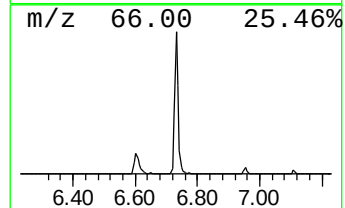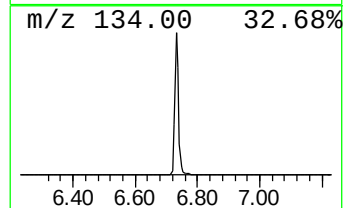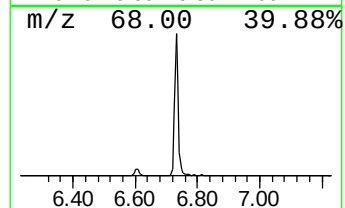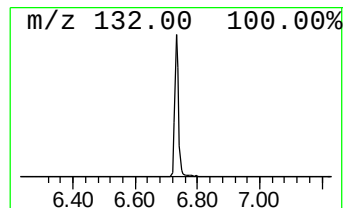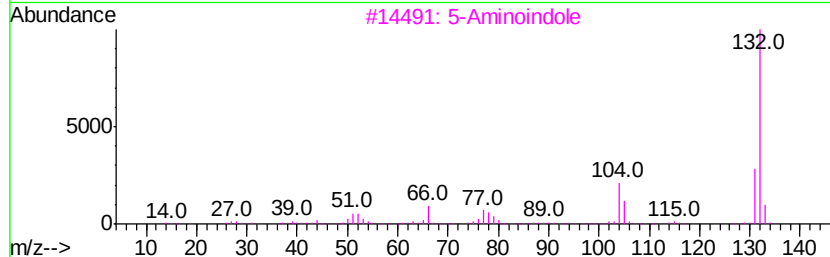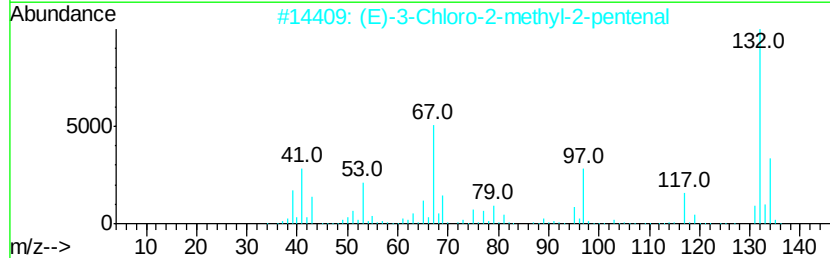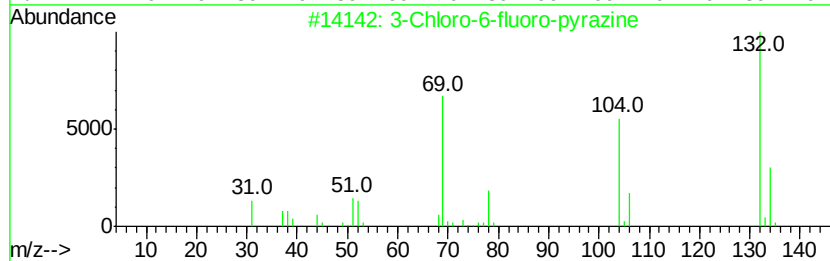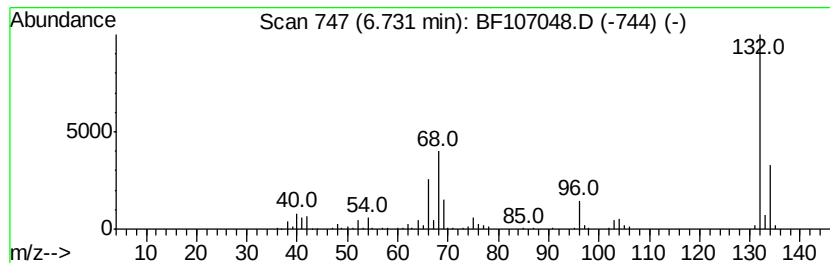

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070218\
Data File : BF107048.D
Acq On : 2 Jul 2018 17:00
Operator : JU/SJ
Sample : J3629-08
Misc :
ALS Vial : 18 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
A0C10-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Pregnane Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.25	2.76 ng	52311	Chrysene-d12	14.15
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	Pregnane	288 C21H36	000481-26-5	50
2	Allopregnane	288 C21H36	000641-85-0	43
3	7b-Phenyl-2a,7b-dihydro-3H-cyclo...	218 C17H14	138089-70-0	35
4	Butanoic acid, 3-oxo-2-(phenylme...	218 C13H14O3	000620-80-4	30
5	Naphthalene, 1-(phenylmethyl)-	218 C17H14	000611-45-0	27

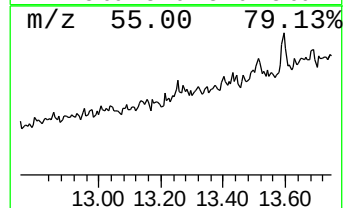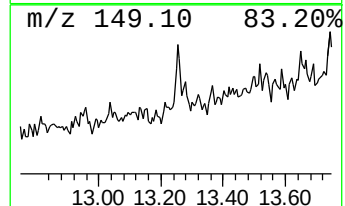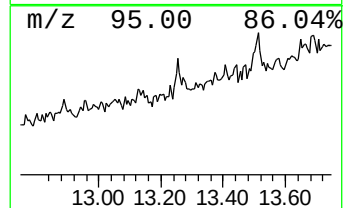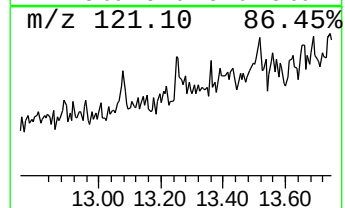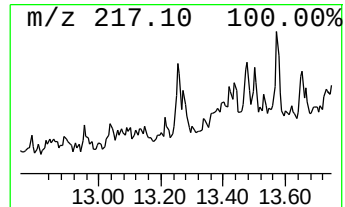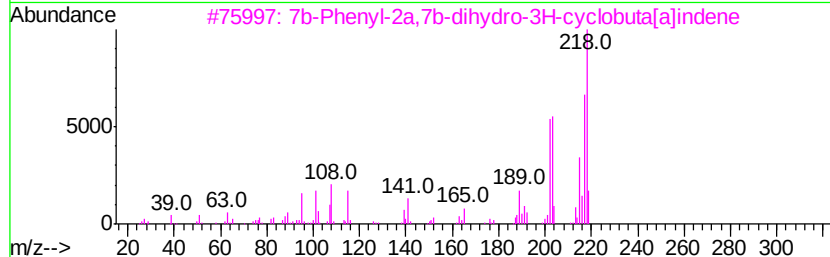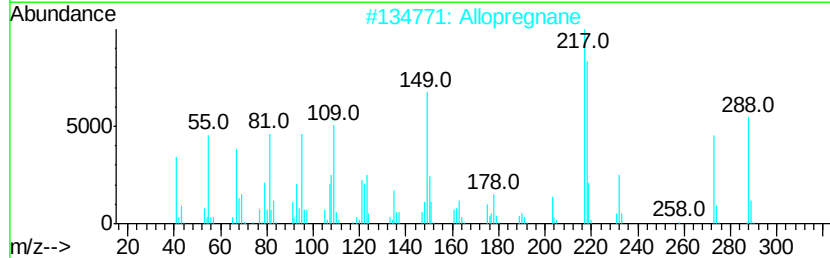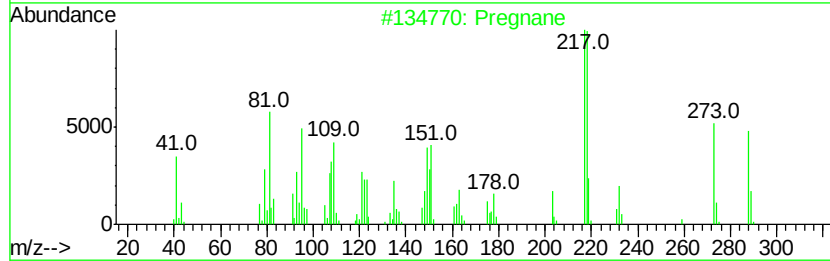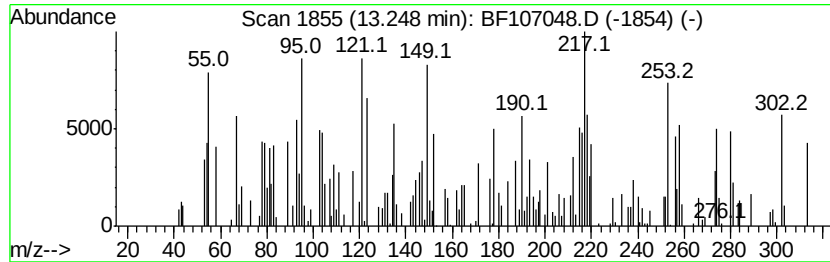

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070218\
Data File : BF107048.D
Acq On : 2 Jul 2018 17:00
Operator : JU/SJ
Sample : J3629-08
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A0C10-03

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.73	6.73	15.9	ng	299461	1	6.95	375670	20.0
Pregnane	13.25	2.8	ng	52311	5	14.15	379259	20.0