

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070218\
 Data File : BF107051.D
 Acq On : 2 Jul 2018 18:23
 Operator : JU/SJ
 Sample : J3629-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 A0C14-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.178	480	483	493	rBB	15293	17363	4.15%	0.428%
2	5.601	551	555	569	rBV	219370	237371	56.74%	5.845%
3	6.607	723	726	740	rBV	215474	252946	60.46%	6.229%
4	6.737	744	748	758	rVV	289629	252340	60.32%	6.214%
5	6.960	782	786	793	rBV	388761	338046	80.81%	8.324%
6	7.113	809	812	822	rVB	239756	203909	48.74%	5.021%
7	7.519	878	881	890	rBV	104307	113518	27.14%	2.795%
8	8.242	1000	1004	1010	rBV	440012	384235	91.85%	9.462%
9	9.313	1183	1186	1196	rBV	261192	260442	62.26%	6.413%
10	9.707	1248	1253	1260	rBV	21959	22555	5.39%	0.555%
11	9.866	1277	1280	1285	rBV	7612	7613	1.82%	0.187%
12	10.001	1300	1303	1317	rVB	416780	395283	94.49%	9.734%
13	10.801	1436	1439	1444	rBV	132697	130726	31.25%	3.219%
14	10.878	1450	1452	1457	rBV2	5735	6617	1.58%	0.163%
15	11.501	1554	1558	1561	rBV	451444	418342	100.00%	10.302%
16	11.577	1568	1571	1574	rBV	7641	7618	1.82%	0.188%
17	12.001	1641	1643	1647	rBV5	5870	9626	2.30%	0.237%
18	12.189	1673	1675	1677	rBV2	7206	8326	1.99%	0.205%
19	12.630	1749	1750	1752	rBV2	11490	11327	2.71%	0.279%
20	12.719	1762	1765	1769	rVB	59813	49189	11.76%	1.211%
21	12.954	1802	1805	1807	rVB	48114	40525	9.69%	0.998%
22	13.077	1823	1826	1830	rBV	354697	310978	74.34%	7.658%
23	14.160	2006	2010	2013	rBV	393604	380240	90.89%	9.364%
24	15.713	2271	2274	2279	rVB	162037	201736	48.22%	4.968%


Sum of corrected areas: 4060871

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070218\
Data File : BF107051.D
Acq On : 2 Jul 2018 18:23
Operator : JU/SJ
Sample : J3629-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A0C14-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

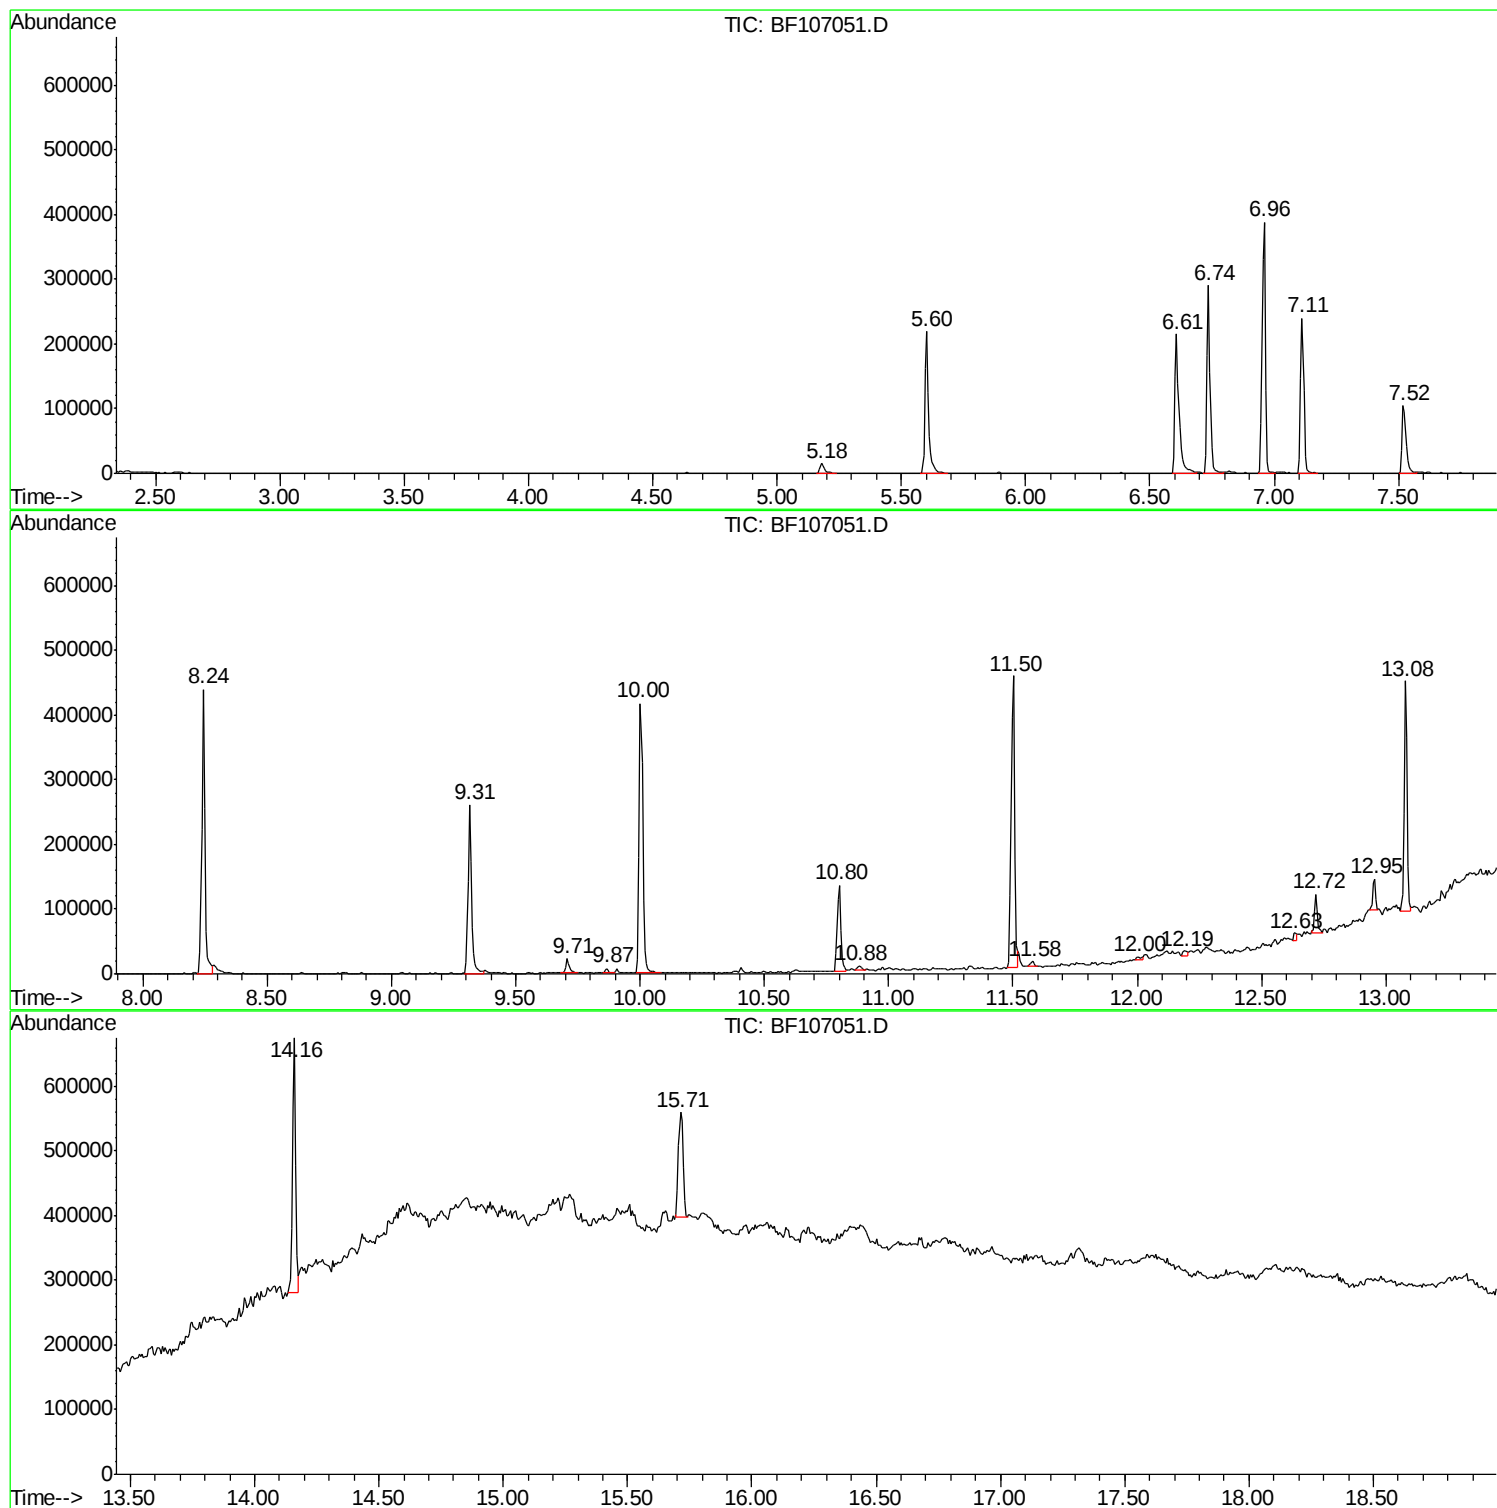

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070218\
Data File : BF107051.D
Acq On : 2 Jul 2018 18:23
Operator : JU/SJ
Sample : J3629-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A0C14-01










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.74 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.74	14.93 ng	252340	1,4-Dichlorobenzene-d4	6.96

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	10
3		5-Aminoindole	132	C8H8N2	005192-03-0	10
4		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

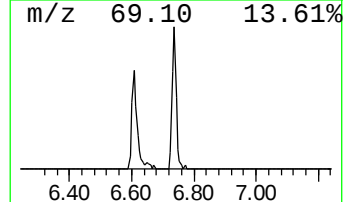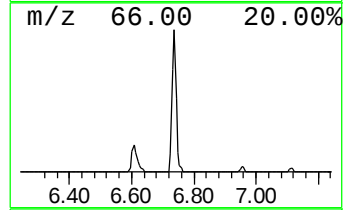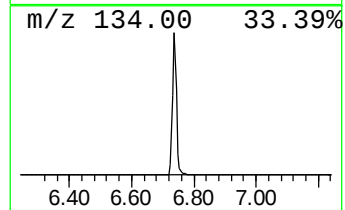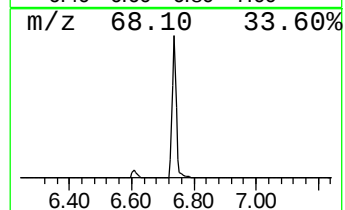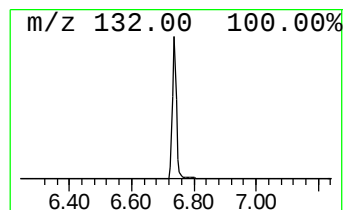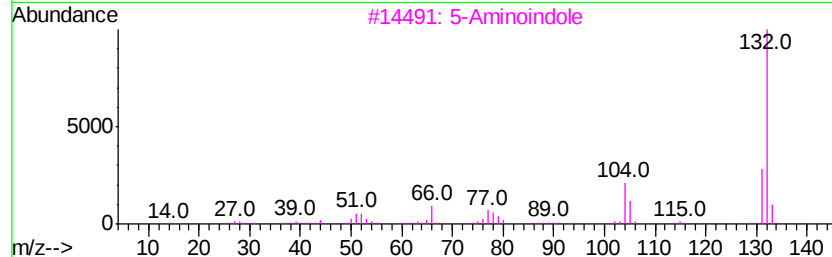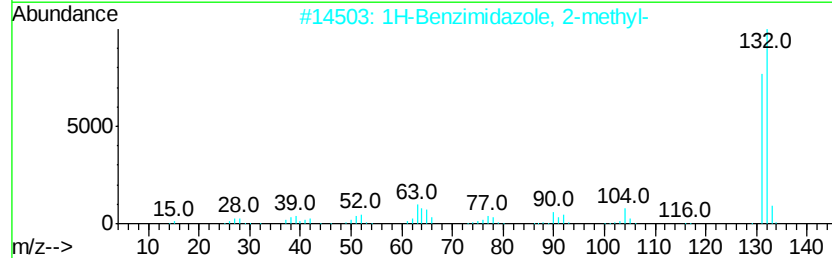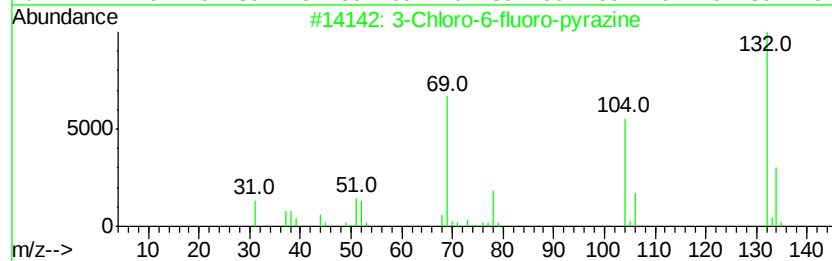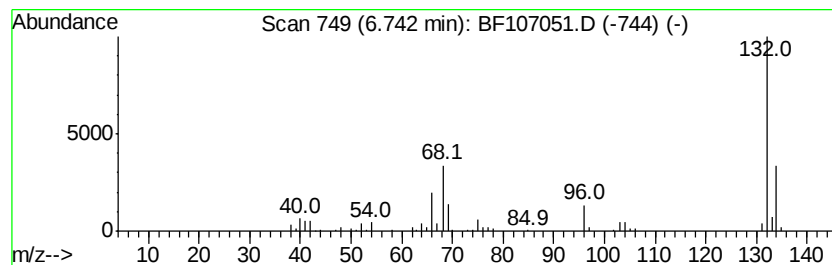

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070218\
Data File : BF107051.D
Acq On : 2 Jul 2018 18:23
Operator : JU/SJ
Sample : J3629-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A0C14-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.74	6.74	14.9	ng	252340	1	6.96	338046	20.0