


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070218\
 Data File : BF107031.D
 Acq On : 2 Jul 2018 8:41
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 29 14:38:29 2018

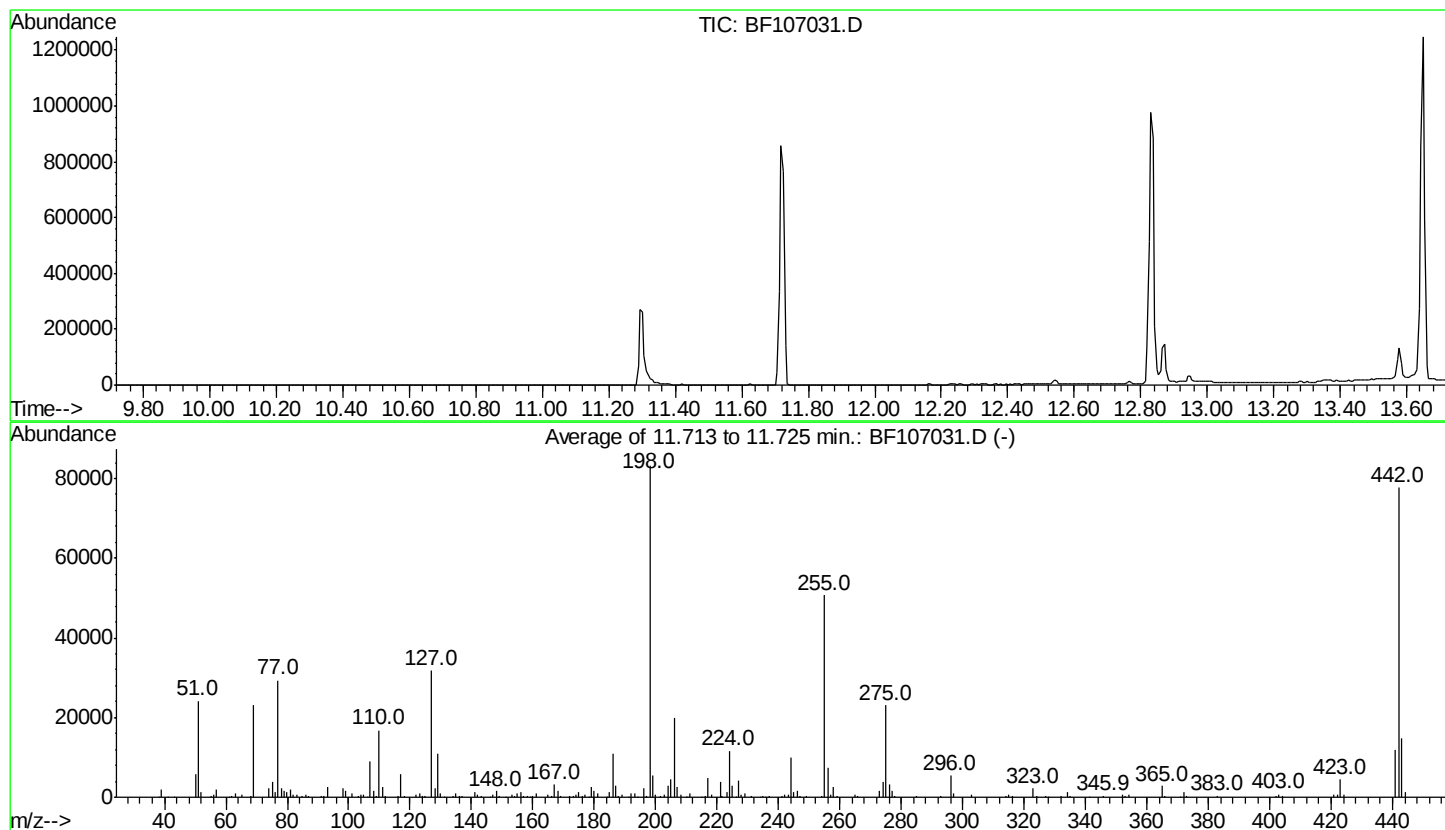

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	24248	PASS
68	69	0.00	2	2.0	472	PASS
69	198	0.00	100	27.9	23202	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.1	31712	PASS
197	198	0.00	2	0.6	484	PASS
198	198	100	100	100.0	83216	PASS
199	198	5	9	6.6	5495	PASS
275	198	10	60	27.7	23091	PASS
365	198	1	100	3.3	2786	PASS
441	443	0.01	100	81.8	11987	PASS
442	198	50	100	93.3	77642	PASS
443	442	15	24	18.9	14651	PASS