

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070219\
 Data File : BF115355.D
 Acq On : 2 Jul 2019 11:16
 Operator : HP/JU
 Sample : PB121082BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB121082BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.207	551	556	559	rBV	3987088	4438245	72.69%	9.609%
2	6.248	726	733	735	rBV	3819511	4534338	74.27%	9.817%
3	6.372	749	754	757	rBV	4703331	4825969	79.05%	10.449%
4	6.601	789	793	796	rBV	1393623	1159634	18.99%	2.511%
5	6.760	815	820	823	rBV	4289581	4023871	65.91%	8.712%
6	7.166	883	889	892	rBV	2703173	3120003	51.10%	6.755%
7	7.884	1006	1011	1027	rBV	1436240	1491516	24.43%	3.229%
8	8.960	1188	1194	1197	rBV	5743306	5843795	95.72%	12.652%
9	9.625	1302	1307	1322	rBV	1540687	1690120	27.68%	3.659%
10	10.413	1436	1441	1471	rBV	3401330	3680290	60.28%	7.968%
11	11.101	1554	1558	1572	rBV	1946299	1790100	29.32%	3.876%
12	12.689	1823	1828	1831	rBV	6040979	6105311	100.00%	13.219%
13	13.724	2000	2004	2020	rBV	1659127	1663084	27.24%	3.601%
14	15.107	2233	2239	2247	rBV	1134407	1657862	27.15%	3.589%
15	15.166	2247	2249	2257	rVB	61541	91513	1.50%	0.198%
16	15.554	2310	2315	2321	rBV	46569	71673	1.17%	0.155%


Sum of corrected areas: 46187324

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070219\
Data File : BF115355.D
Acq On : 2 Jul 2019 11:16
Operator : HP/JU
Sample : PB121082BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121082BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

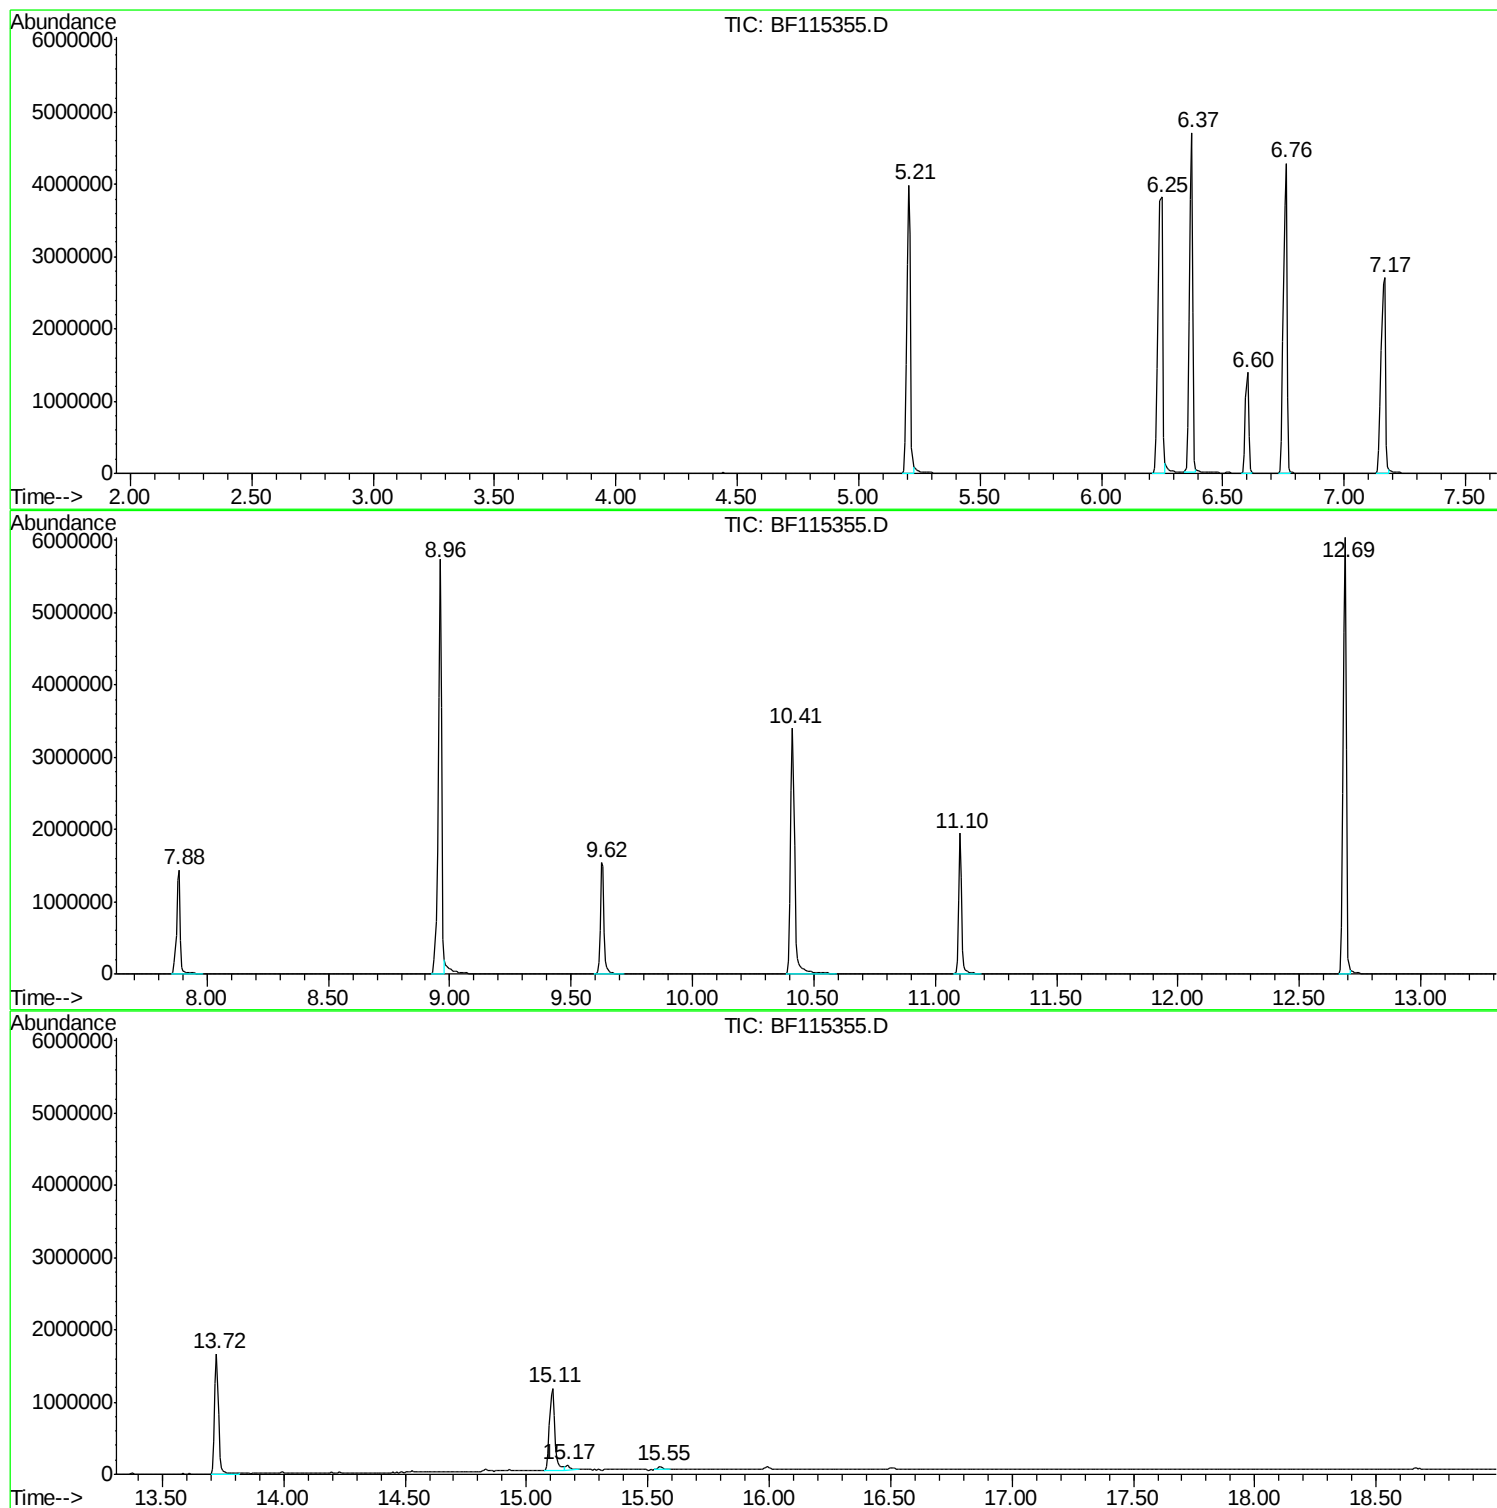

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070219\
Data File : BF115355.D
Acq On : 2 Jul 2019 11:16
Operator : HP/JU
Sample : PB121082BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121082BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.37 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.37	83.23 ng	4825970	1,4-Dichlorobenzene-d4	6.60

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	16
4		5-Aminoindole	132	C8H8N2	005192-03-0	16
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

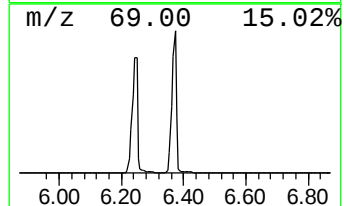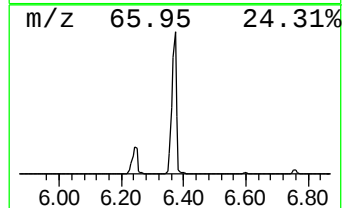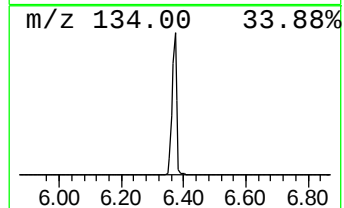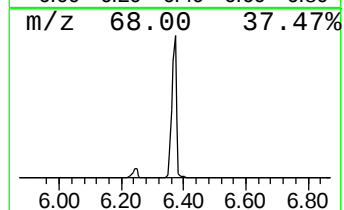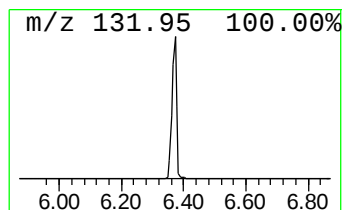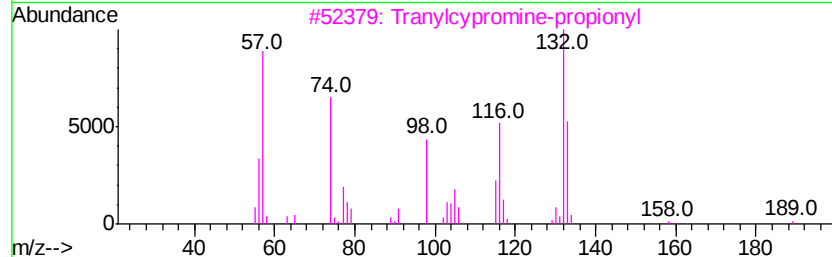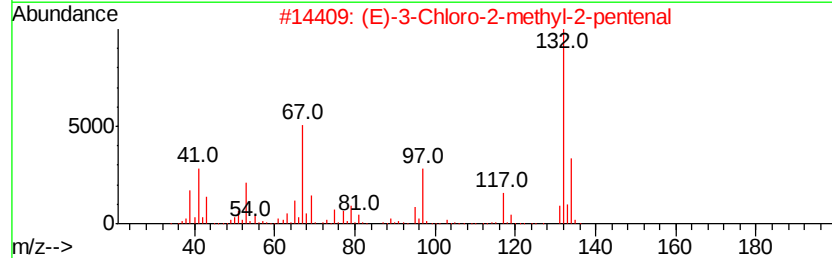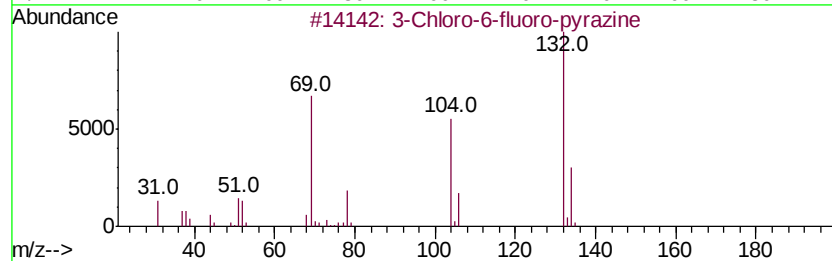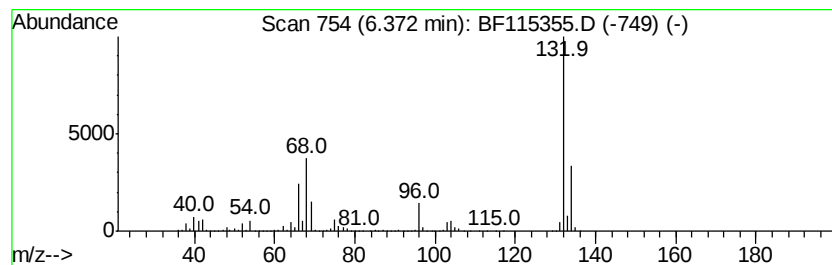

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070219\
Data File : BF115355.D
Acq On : 2 Jul 2019 11:16
Operator : HP/JU
Sample : PB121082BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121082BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.37	6.37	83.2	ng	4825970	1	6.60	1159630	20.0