

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070219\
 Data File : BF115364.D
 Acq On : 2 Jul 2019 17:20
 Operator : HP/JU
 Sample : K3632-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OIL-WATER-SEPERATOR-4-(OWS)-

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.419	78	82	88	rVB	99569	133789	2.02%	0.236%
2	3.243	216	222	232	rVB	56466	99370	1.50%	0.175%
3	3.507	260	267	276	rVB2	47450	98831	1.49%	0.174%
4	4.348	405	410	416	rVB	233026	253619	3.83%	0.447%
5	4.795	482	486	488	rBV	152879	190637	2.88%	0.336%
6	4.825	488	491	498	rVB	268575	291265	4.40%	0.513%
7	5.025	521	525	528	rVB	139971	132021	1.99%	0.233%
8	5.219	553	558	561	rBV	3954358	4184386	63.19%	7.376%
9	6.254	729	734	739	rBV	3589740	3874407	58.51%	6.830%
10	6.295	739	741	750	rVB2	57998	77454	1.17%	0.137%
11	6.378	750	755	758	rBV	4815728	5045680	76.19%	8.895%
12	6.436	762	765	768	rVB	144639	112672	1.70%	0.199%
13	6.607	790	794	797	rBV	1803752	1421889	21.47%	2.507%
14	6.766	816	821	824	rBV	5133223	4568485	68.99%	8.054%
15	7.013	860	863	871	rVB	110055	105719	1.60%	0.186%
16	7.172	883	890	893	rBV	3481292	3708184	56.00%	6.537%
17	7.413	928	931	932	rBV2	84928	84158	1.27%	0.148%
18	7.431	932	934	938	rVB	119695	109162	1.65%	0.192%
19	7.566	952	957	964	rVB5	59463	95947	1.45%	0.169%
20	7.631	964	968	972	rBV2	176462	206901	3.12%	0.365%
21	7.731	982	985	988	rVB	111563	102728	1.55%	0.181%
22	7.889	1007	1012	1015	rBV	1970556	1774675	26.80%	3.128%
23	8.142	1051	1055	1058	rBV2	51829	71438	1.08%	0.126%
24	8.395	1094	1098	1104	rVB	131739	122622	1.85%	0.216%
25	8.554	1121	1125	1128	rVB	89695	88332	1.33%	0.156%
26	8.601	1128	1133	1137	rVB2	87731	81459	1.23%	0.144%
27	8.972	1191	1196	1199	rBV	6426215	6622068	100.00%	11.674%
28	9.225	1234	1239	1246	rBV5	41944	66491	1.00%	0.117%
29	9.301	1246	1252	1254	rBV2	106480	131879	1.99%	0.232%
30	9.360	1259	1262	1270	rBV	361455	375978	5.68%	0.663%
31	9.636	1304	1309	1313	rBV2	2215127	2174603	32.84%	3.834%
32	9.789	1331	1335	1342	rBV	571083	565729	8.54%	0.997%
33	10.013	1369	1373	1380	rBV	394517	469445	7.09%	0.828%
34	10.424	1438	1443	1457	rBV	3680158	3852761	58.18%	6.792%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070219\
 Data File : BF115364.D
 Acq On : 2 Jul 2019 17:20
 Operator : HP/JU
 Sample : K3632-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OIL-WATER-SEPERATOR-4-(OWS)-

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.524	1457	1460	1465	rVV	230846	258222	3.90%	0.455%
36	10.577	1465	1469	1474	rVV2	131070	200291	3.02%	0.353%
37	10.624	1474	1477	1480	rVV	204559	253984	3.84%	0.448%
38	10.660	1480	1483	1486	rVV2	207125	306617	4.63%	0.541%
39	10.695	1486	1489	1491	rVV2	215384	276038	4.17%	0.487%
40	10.719	1491	1493	1496	rVV	148306	169426	2.56%	0.299%
41	10.760	1496	1500	1505	rVV2	150924	319117	4.82%	0.563%
42	10.807	1505	1508	1512	rVV3	257130	388006	5.86%	0.684%
43	10.842	1512	1514	1519	rVV	262276	379752	5.73%	0.669%
44	10.883	1519	1521	1530	rVB	153533	198030	2.99%	0.349%
45	11.013	1537	1543	1545	rBV3	67034	75695	1.14%	0.133%
46	11.113	1556	1560	1564	rBV	2308981	2013264	30.40%	3.549%
47	11.466	1618	1620	1635	rVB	50676	95540	1.44%	0.168%
48	11.666	1648	1654	1666	rBV2	169045	272165	4.11%	0.480%
49	12.448	1784	1787	1791	rBV2	55969	66993	1.01%	0.118%
50	12.624	1811	1817	1826	rBV	34452	77961	1.18%	0.137%
51	12.707	1826	1831	1834	rBV	5688693	5776044	87.22%	10.182%
52	13.218	1915	1918	1922	rVB	233171	205071	3.10%	0.362%
53	13.560	1971	1976	1981	rBV	56676	91658	1.38%	0.162%
54	13.742	2001	2007	2021	rVB	1644163	1776350	26.82%	3.131%
55	14.248	2090	2093	2099	rVB	73386	88485	1.34%	0.156%
56	14.542	2140	2143	2146	rVB	107570	96856	1.46%	0.171%
57	14.607	2151	2154	2159	rBV	64799	66300	1.00%	0.117%
58	14.842	2191	2194	2198	rBV	113467	121686	1.84%	0.215%
59	15.118	2236	2241	2247	rBV	1231092	1468477	22.18%	2.589%
60	15.183	2249	2252	2257	rVB	111852	129908	1.96%	0.229%
61	15.565	2313	2317	2322	rBV	91204	129558	1.96%	0.228%
62	16.006	2389	2392	2404	rVB2	59263	129978	1.96%	0.229%


Sum of corrected areas: 56726256

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070219\
Data File : BF115364.D
Acq On : 2 Jul 2019 17:20
Operator : HP/JU
Sample : K3632-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OIL-WATER-SEPARATOR-4-(OWS)-

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF062119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

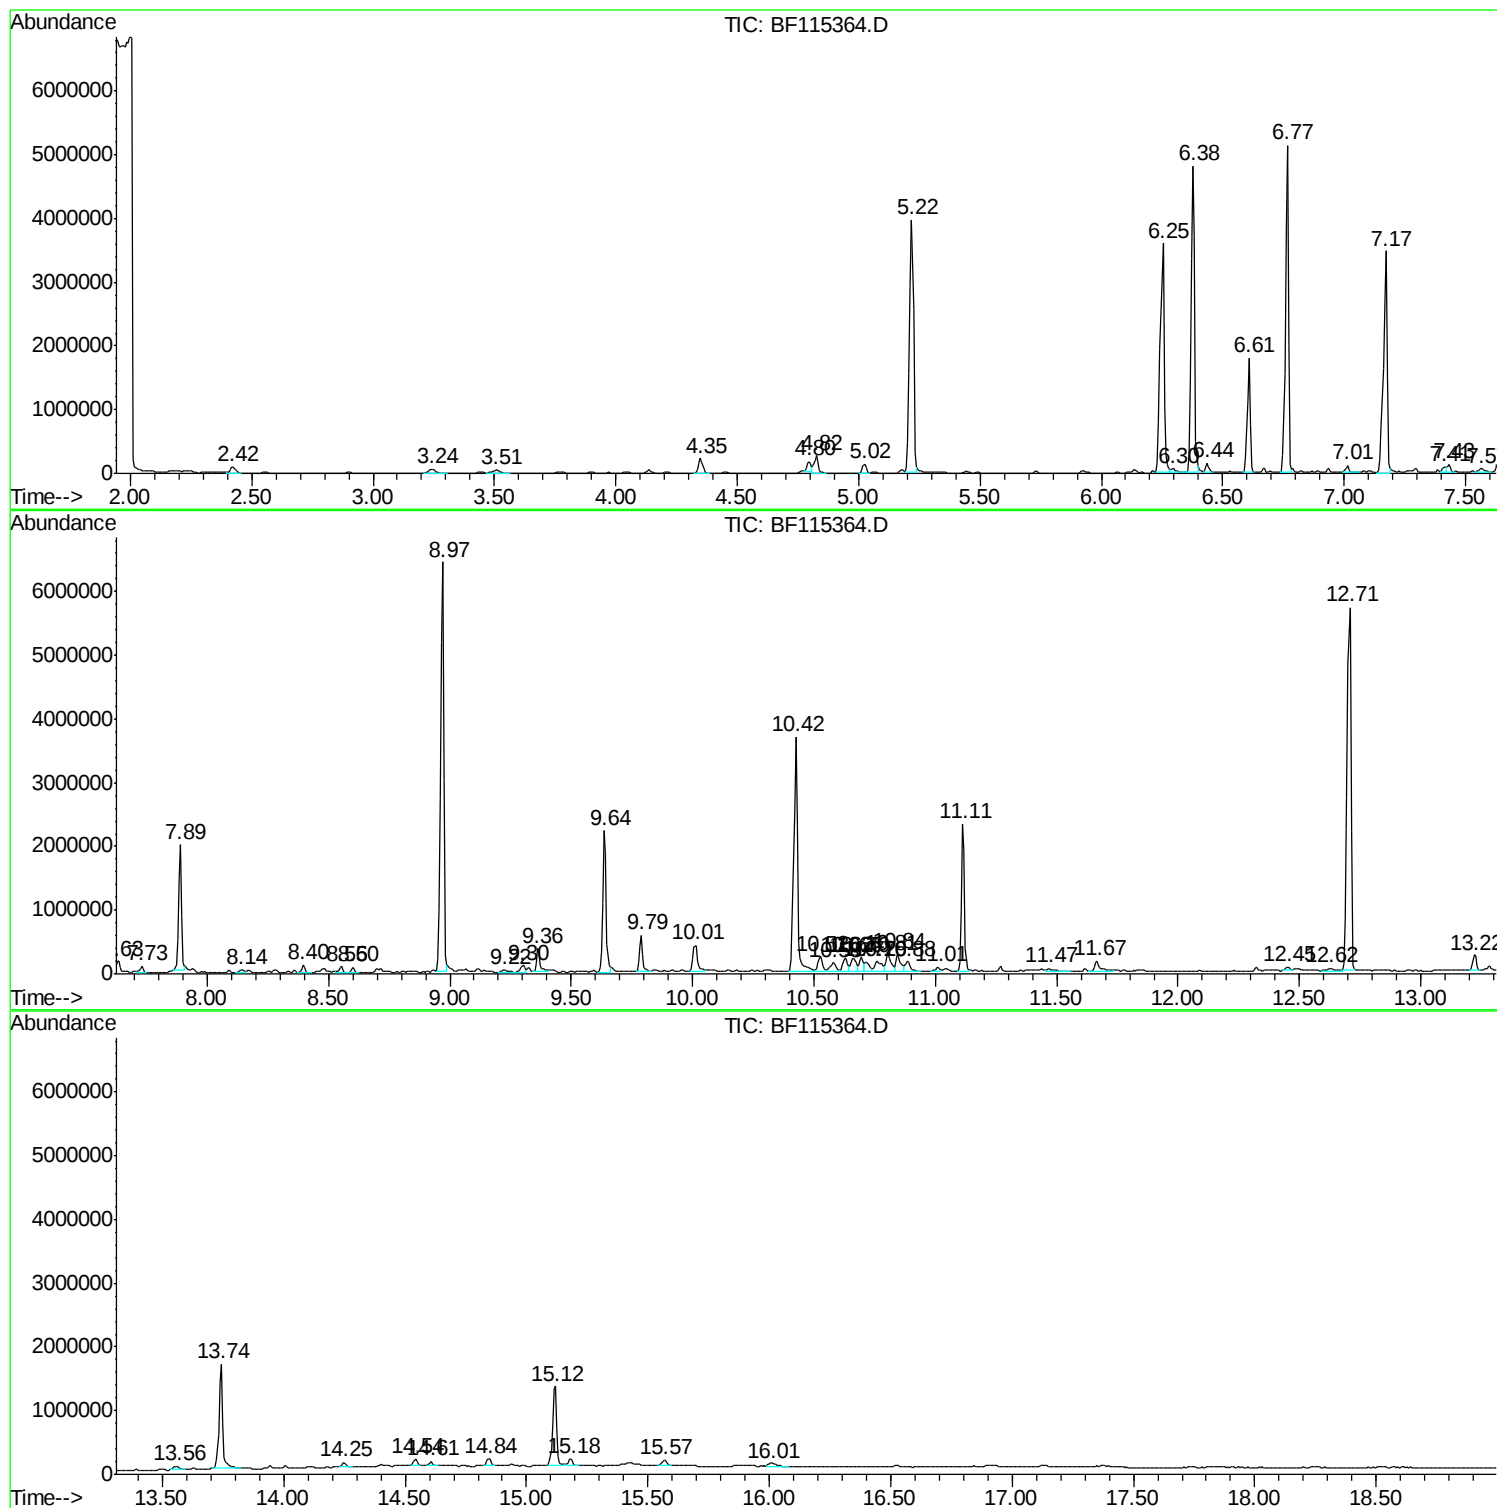

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070219\
Data_File : BF115364.D
Acq_On : 2_Jul_2019_ 17:200
Operator : HP/JUU
Sample : K3632-011
Misc :
ALS_Vial : 6 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
OIL-WATER-SEPERATOR-4-(OWS)-

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
