


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070219\
 Data File : BF115349.D
 Acq On : 2 Jul 2019 7:56
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 05:26:43 2019

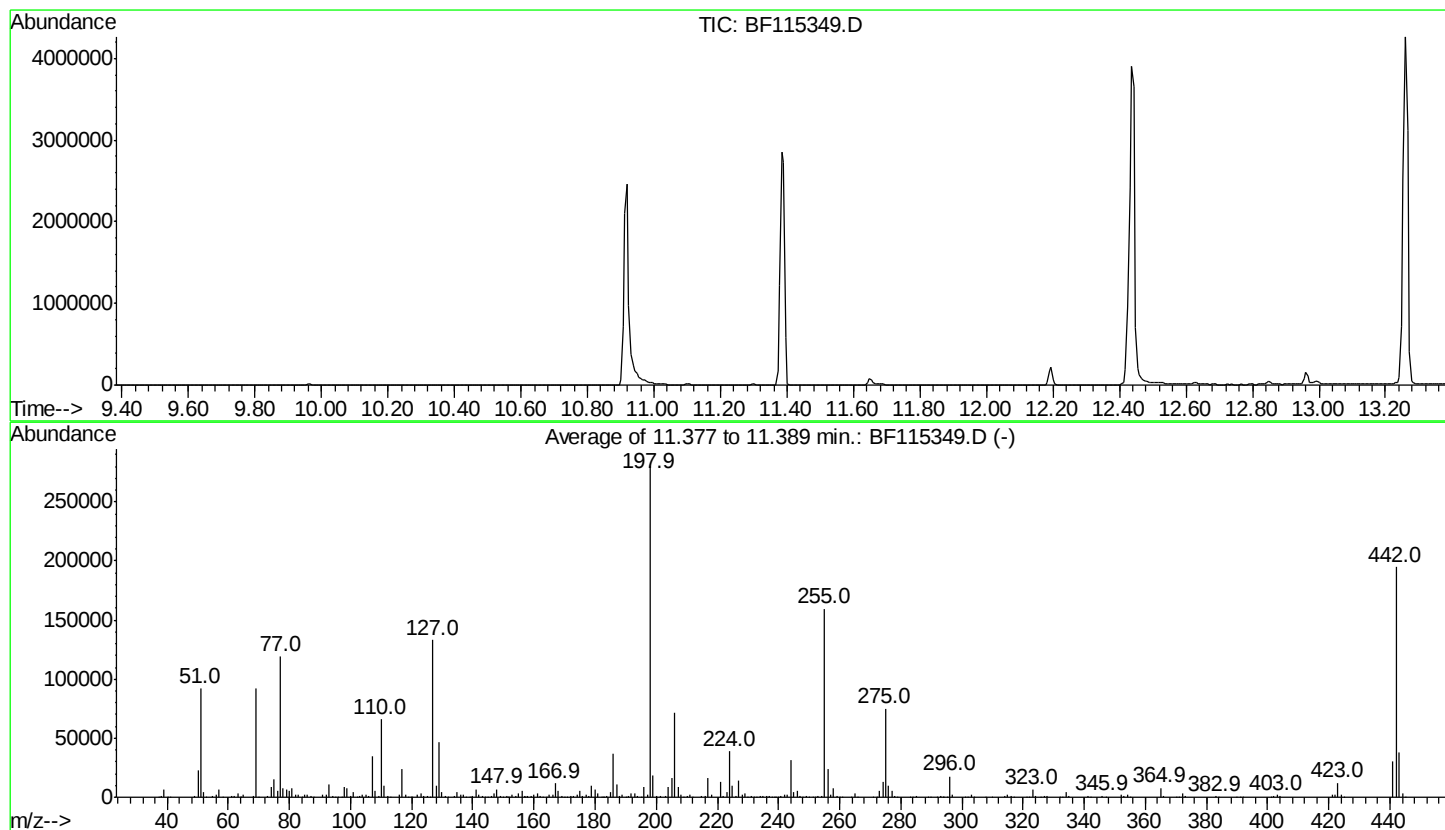

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	91701	PASS
68	69	0.00	2	1.8	1626	PASS
69	198	0.00	100	32.9	92282	PASS
70	69	0.00	2	0.6	529	PASS
127	198	10	80	47.4	132941	PASS
197	198	0.00	2	0.6	1798	PASS
198	198	100	100	100.0	280746	PASS
199	198	5	9	6.6	18620	PASS
275	198	10	60	26.7	74962	PASS
365	198	1	100	2.9	8168	PASS
441	198	0.01	100	10.9	30525	PASS
442	198	50	100	69.5	195024	PASS
443	442	15	24	19.5	37982	PASS