


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070219\
 Data File : BF115359.D
 Acq On : 2 Jul 2019 14:35
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF062119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 28 05:26:43 2019

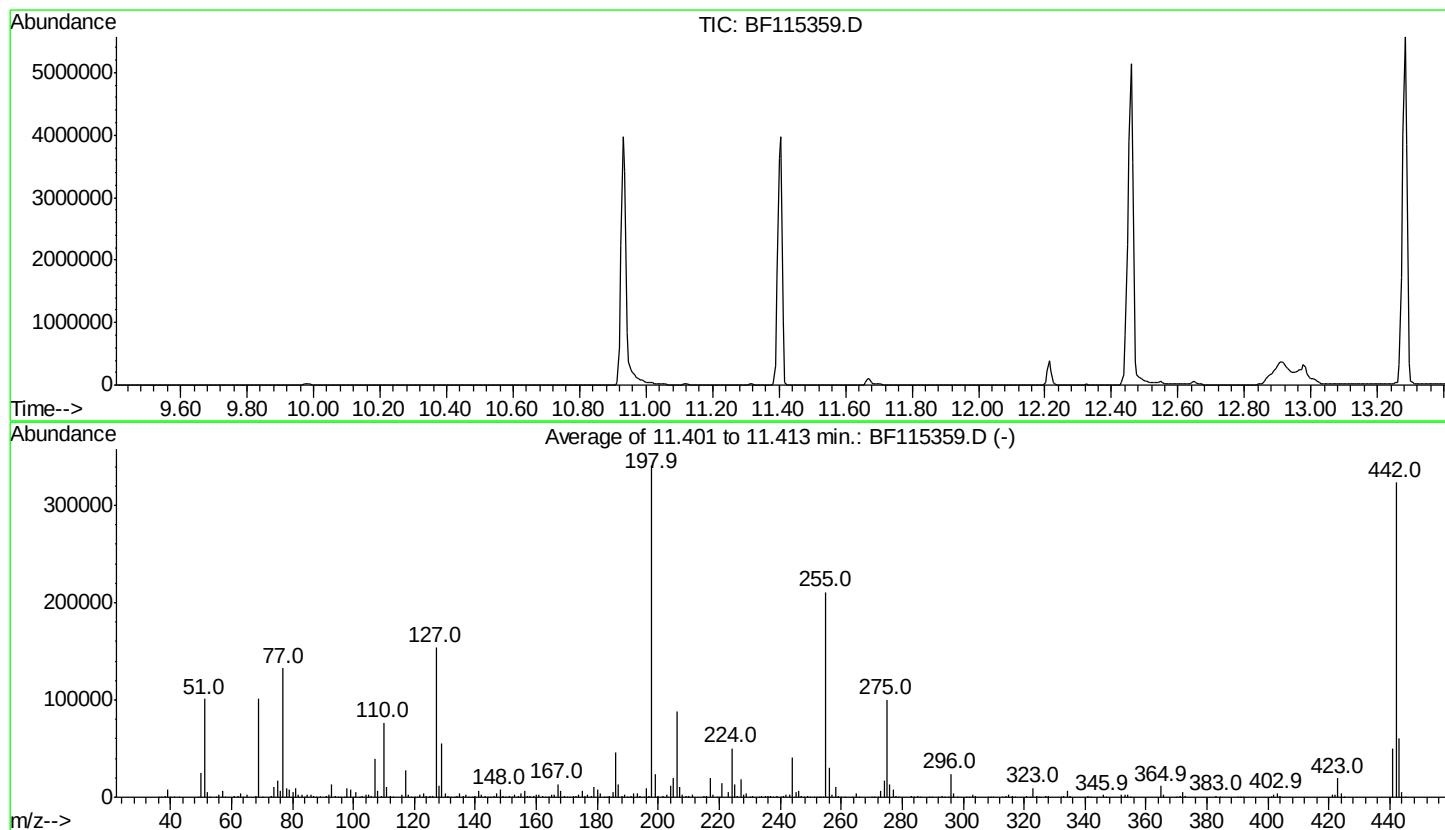

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	101191	PASS
68	69	0.00	2	1.9	1925	PASS
69	198	0.00	100	29.8	101688	PASS
70	69	0.00	2	0.5	545	PASS
127	198	10	80	45.1	153757	PASS
197	198	0.00	2	0.4	1217	PASS
198	198	100	100	100.0	340917	PASS
199	198	5	9	6.8	23143	PASS
275	198	10	60	29.4	100197	PASS
365	198	1	100	3.4	11759	PASS
441	198	0.01	100	14.9	50645	PASS
442	198	50	100	94.9	323413	PASS
443	442	15	24	18.9	61133	PASS