
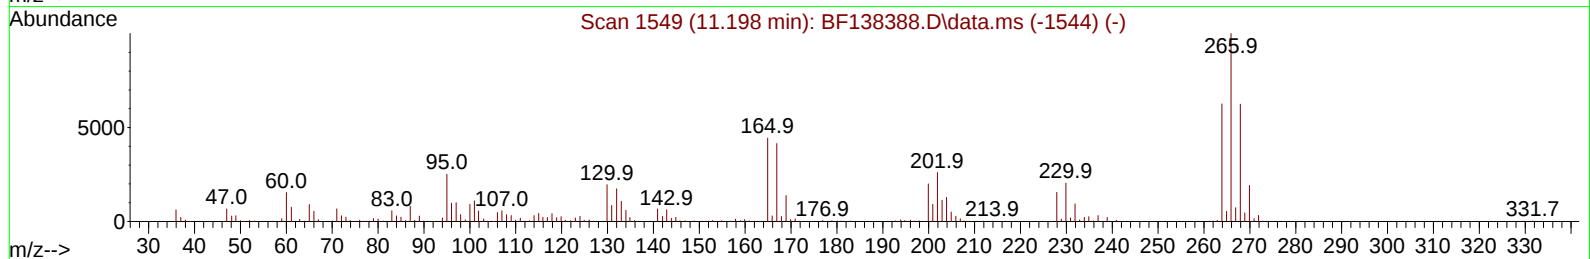
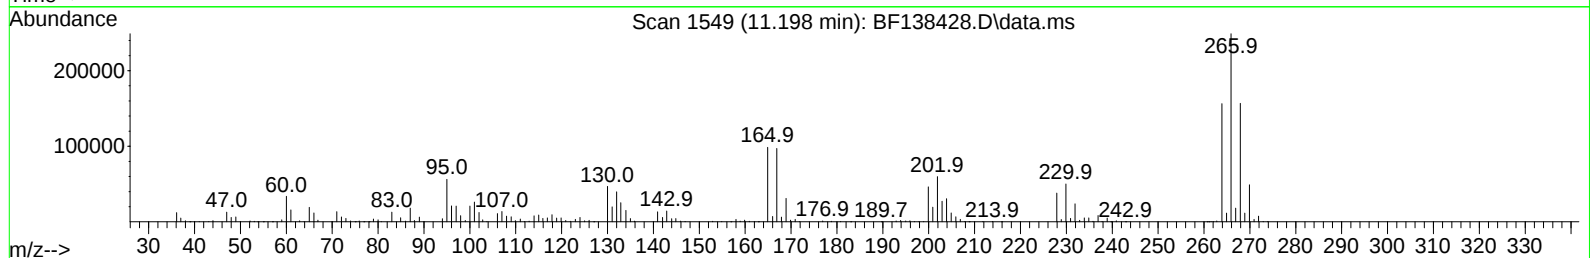


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070224\
Data File : BF138428.D
Acq On : 02 Jul 2024 14:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 15:35:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

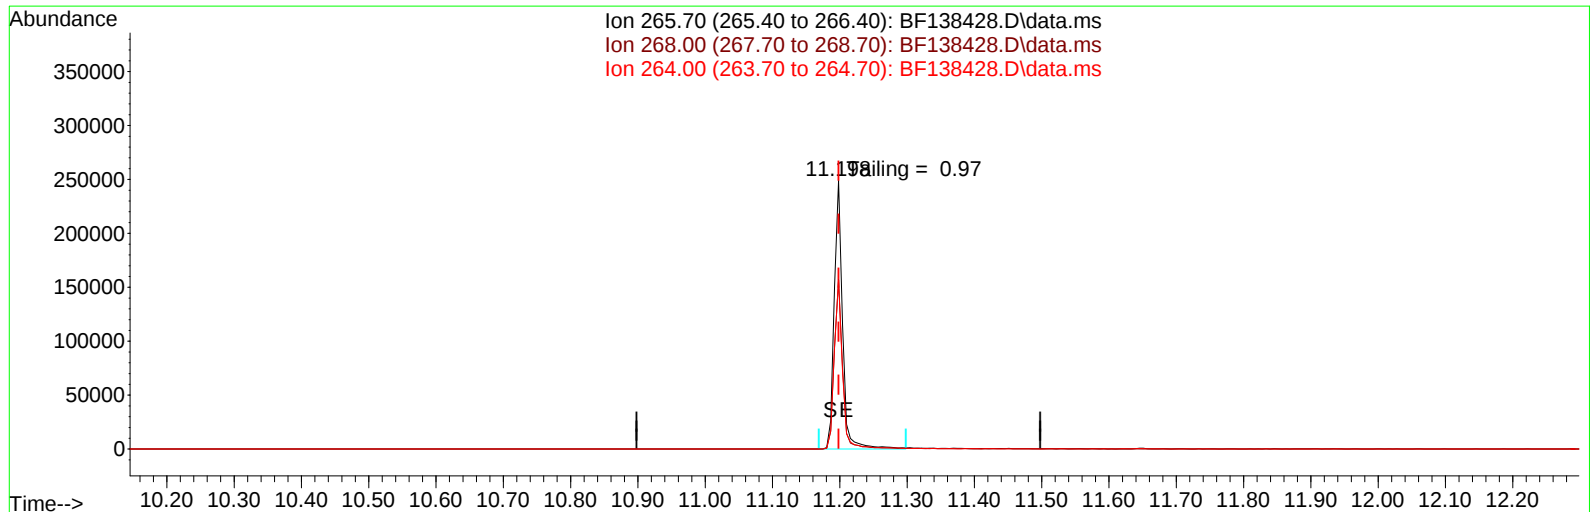

TIC: BF138428.D\data.ms

(70) Pentachlorophenol (C)




11.198min (+ 0.000) 32120.10 ng

response 215350

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.97
264.00	62.50	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070224\
Data File : BF138428.D
Acq On : 02 Jul 2024 14:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 02 15:35:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

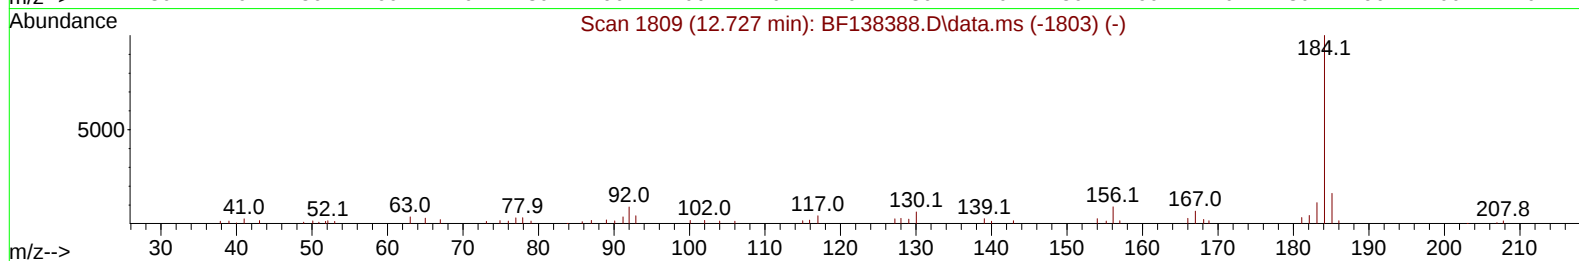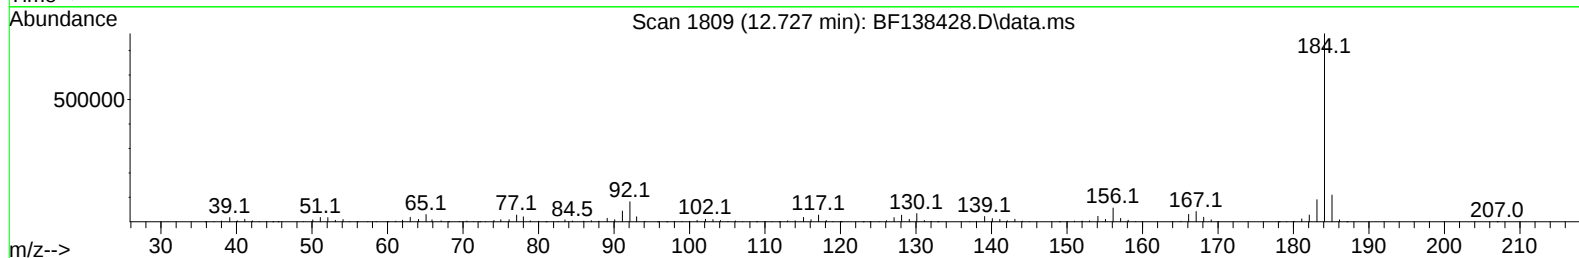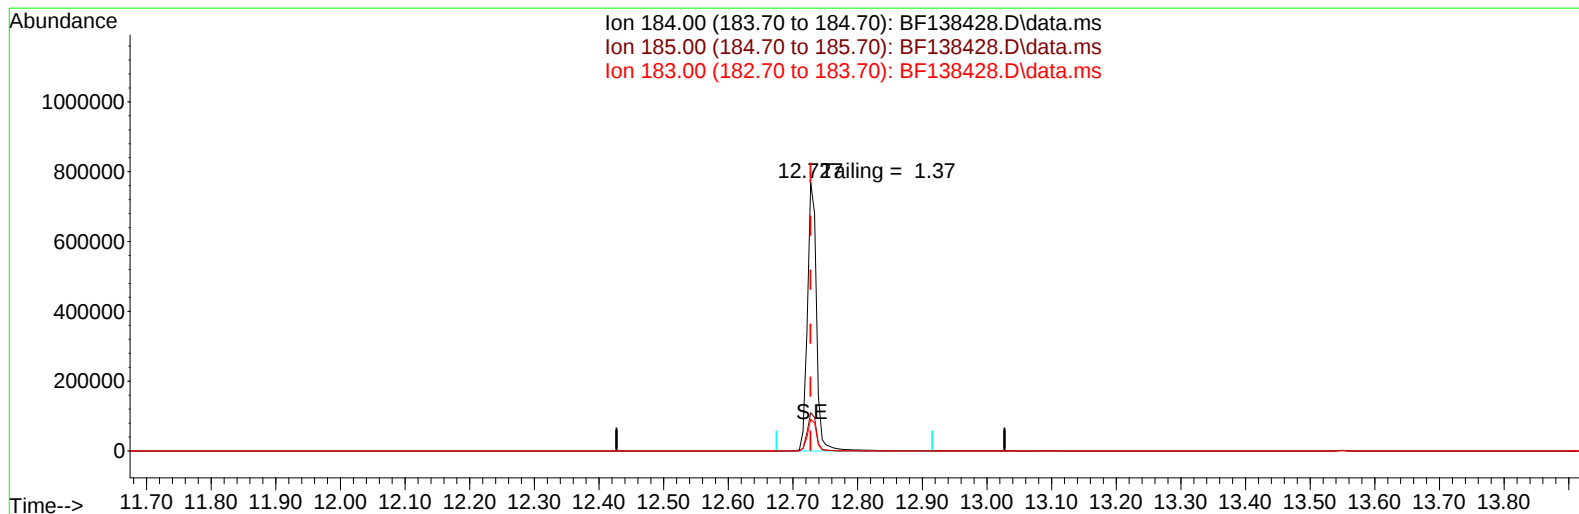

TIC: BF138428.D\data.ms

(77) Benzidine

12.727min (+ 0.000) 0.00 ng

response 750352

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	14.25
183.00	11.30	11.81
0.00	0.00	0.00