


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070224\
Data File : BF138417.D
Acq On : 02 Jul 2024 09:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jun 29 02:44:30 2024

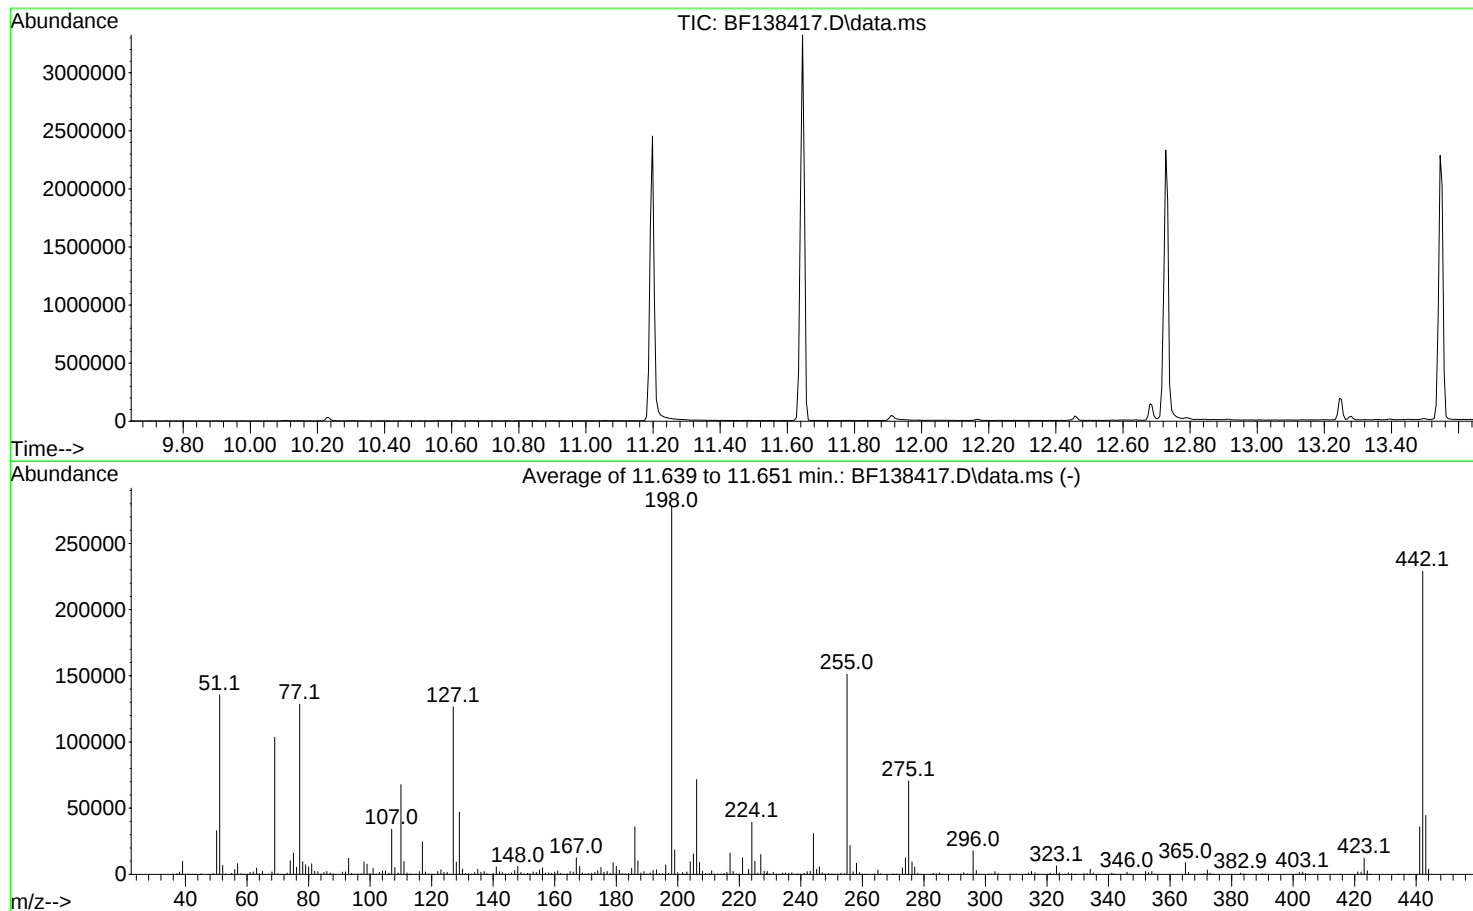

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	135693	PASS
68	69	0.00	2	1.8	1831	PASS
69	198	0.00	100	37.2	103493	PASS
70	69	0.00	2	0.6	654	PASS
127	198	10	80	45.6	126613	PASS
197	198	0.00	2	0.3	695	PASS
198	198	100	100	100.0	277909	PASS
199	198	5	9	6.7	18504	PASS
275	198	10	60	25.4	70605	PASS
365	198	1	100	3.2	8868	PASS
441	198	0.01	100	12.9	35960	PASS
442	442	50	100	100.0	229133	PASS
443	442	15	24	19.4	44363	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/2/2024	BNA_F	<u>BF138417.D</u>
Compound Name	Response	Retention Time
DDT	395679	13.545
DDD	38018	13.251
DDE	1007	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
39025	434704	8.98

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070224\
Data File : BF138417.D
Acq On : 02 Jul 2024 09:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 02 11:36:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

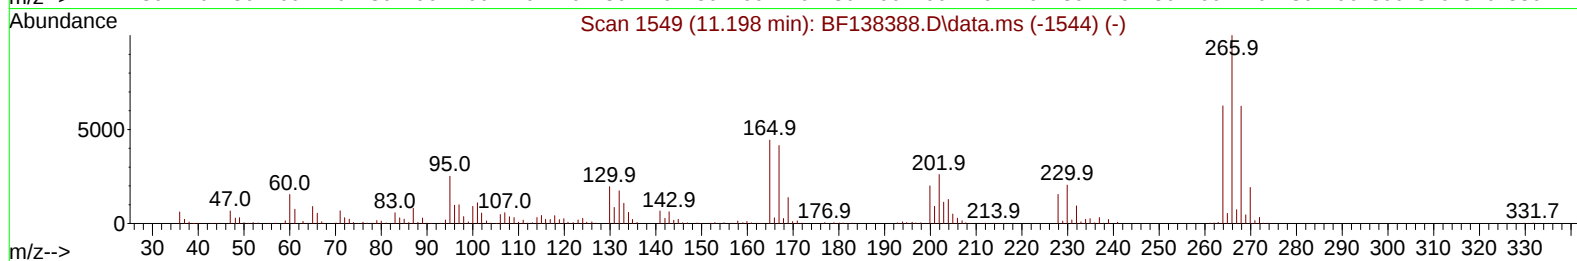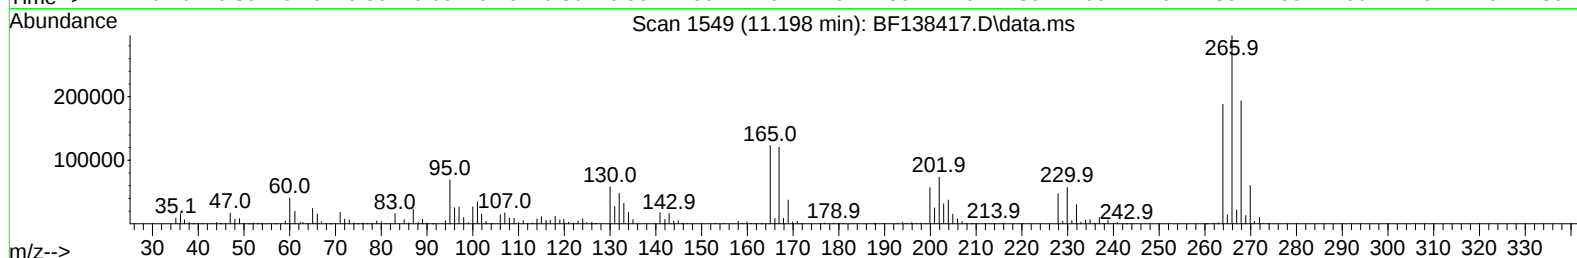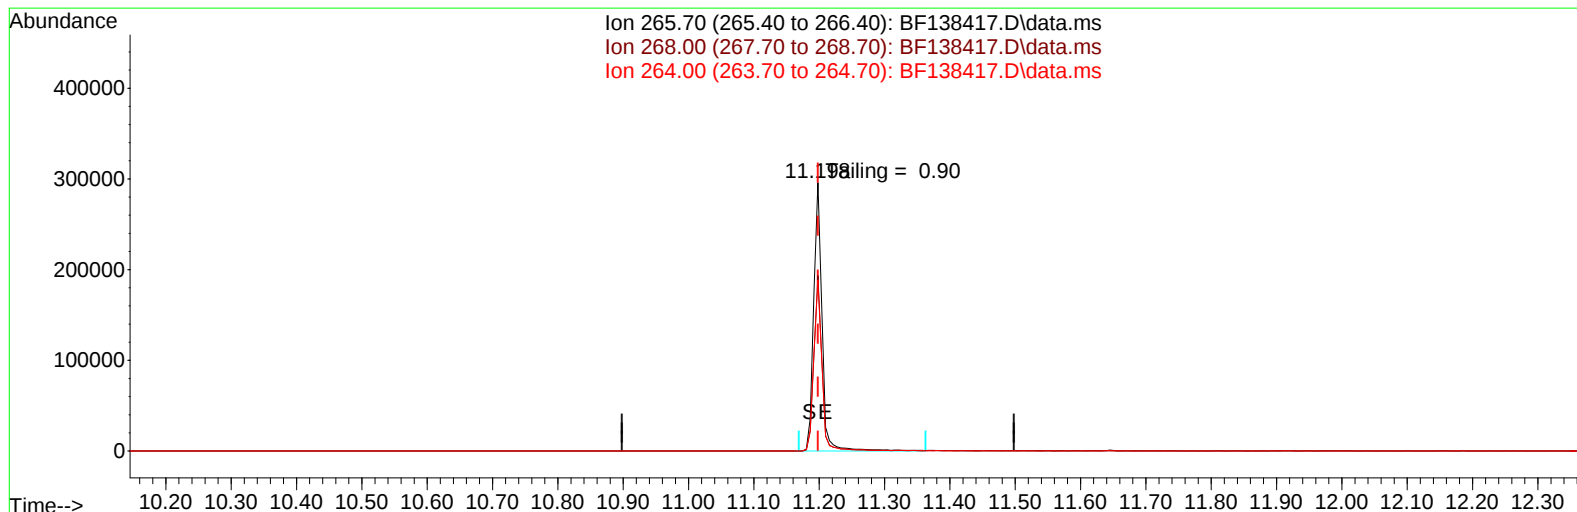

TIC: BF138417.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.000) 680194.93 ng




response 265852

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	65.35
264.00	62.50	63.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070224\
Data File : BF138417.D
Acq On : 02 Jul 2024 09:12
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 02 11:36:03 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

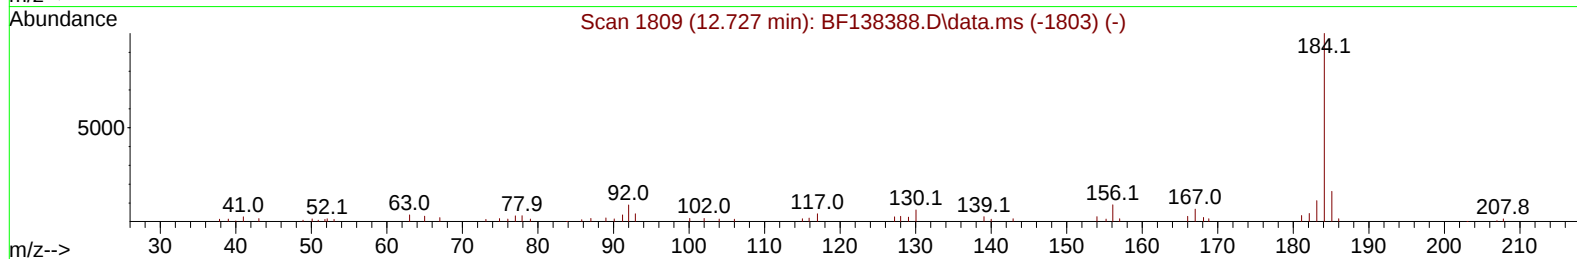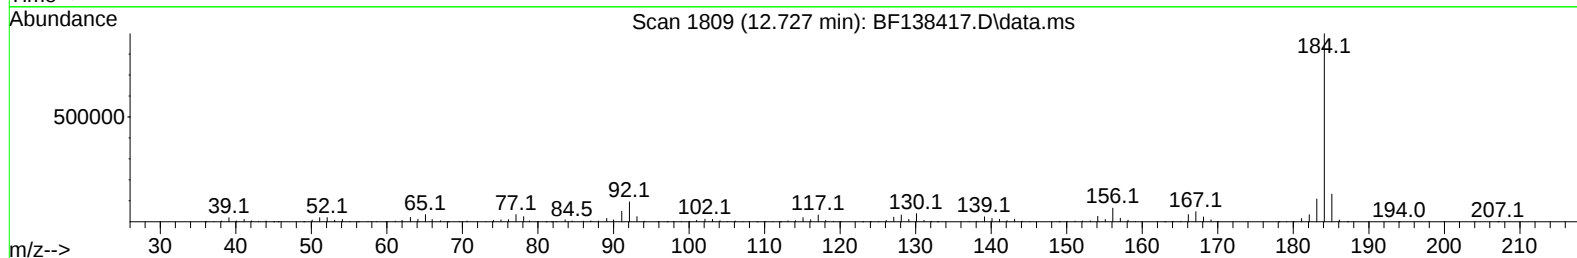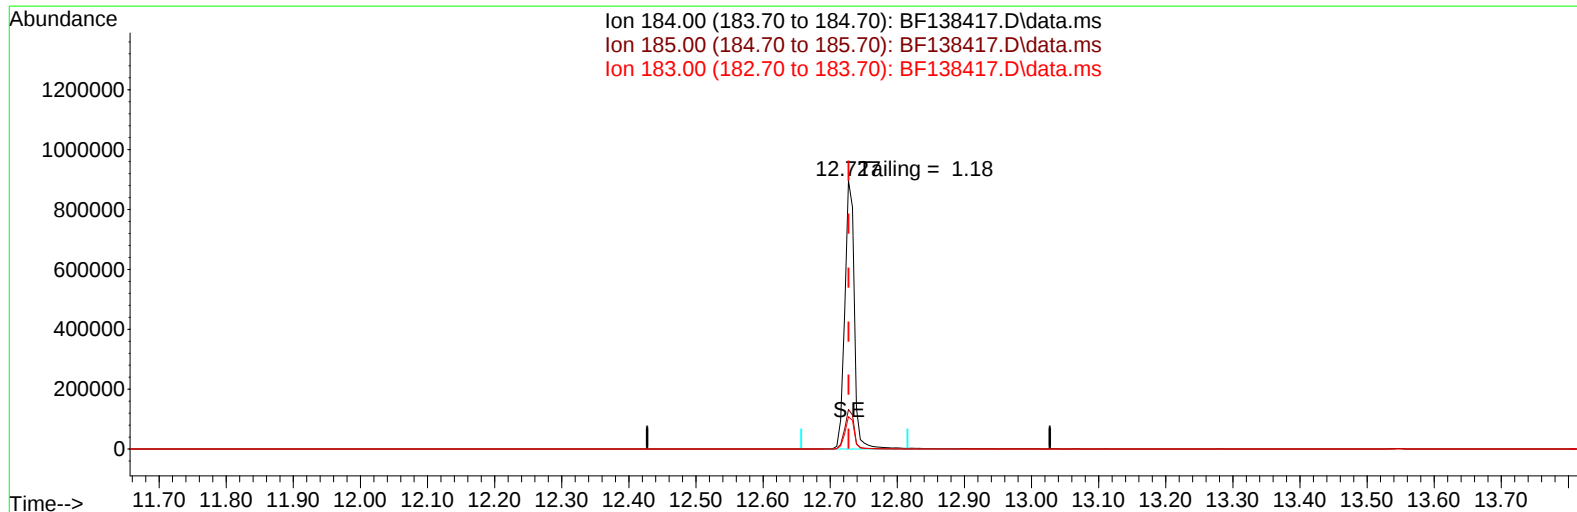

TIC: BF138417.D\data.ms

(77) Benzidine

12.727min (-0.000) 0.00 ng

response 886661

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	14.73
183.00	11.30	12.08
0.00	0.00	0.00