


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070224\
Data File : BF138428.D
Acq On : 02 Jul 2024 14:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jun 29 02:44:30 2024

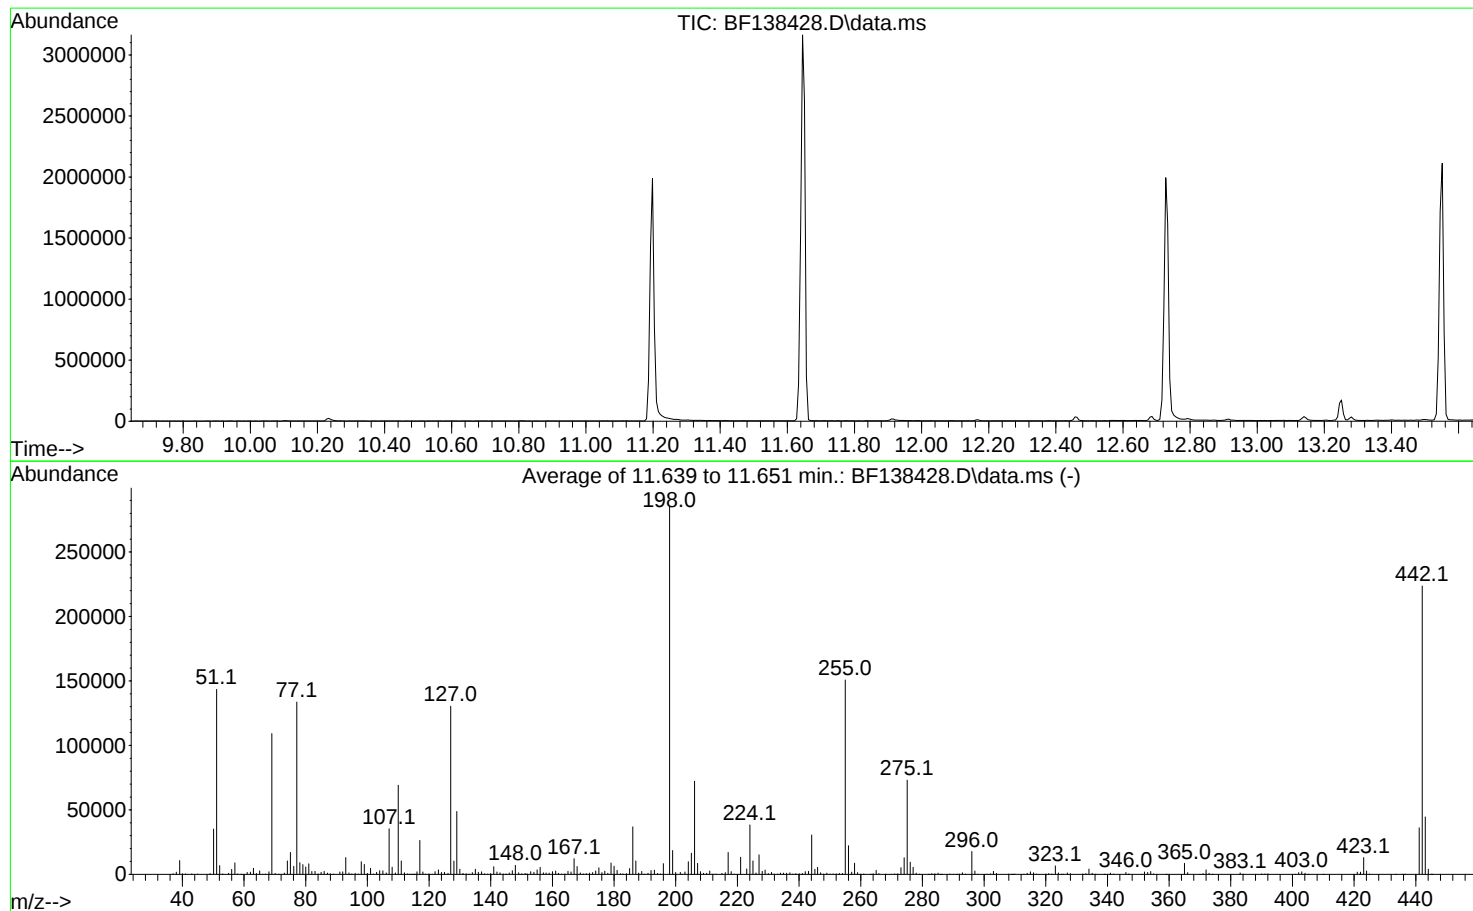

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	50.3	143477	PASS
68	69	0.00	2	1.8	1990	PASS
69	198	0.00	100	38.3	109224	PASS
70	69	0.00	2	0.7	723	PASS
127	198	10	80	45.7	130451	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	285312	PASS
199	198	5	9	6.5	18458	PASS
275	198	10	60	25.6	73048	PASS
365	198	1	100	3.0	8571	PASS
441	198	0.01	100	12.6	36066	PASS
442	442	50	100	100.0	223576	PASS
443	442	15	24	19.9	44516	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/2/2024	BNA_F	<u>BF138428.D</u>
Compound Name	Response	Retention Time
DDT	351178	13.551
DDD	32334	13.251
DDE	1524	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33858	385036	8.79

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070224\
Data File : BF138428.D
Acq On : 02 Jul 2024 14:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 02 15:35:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

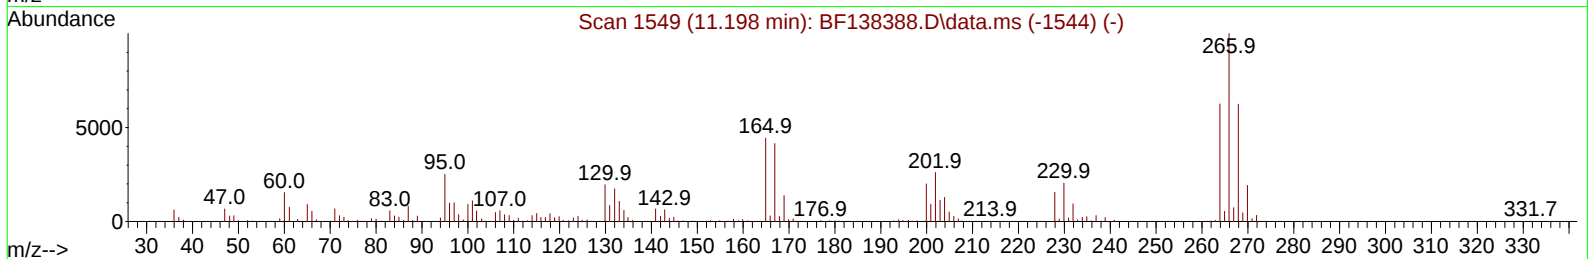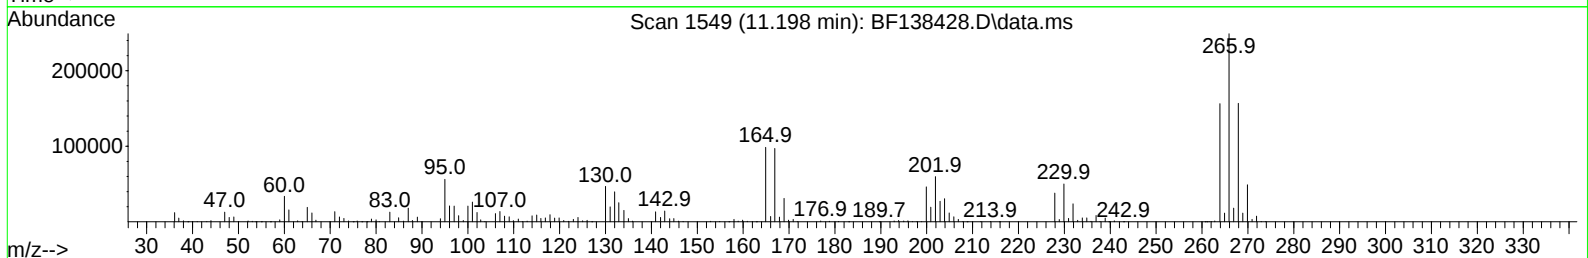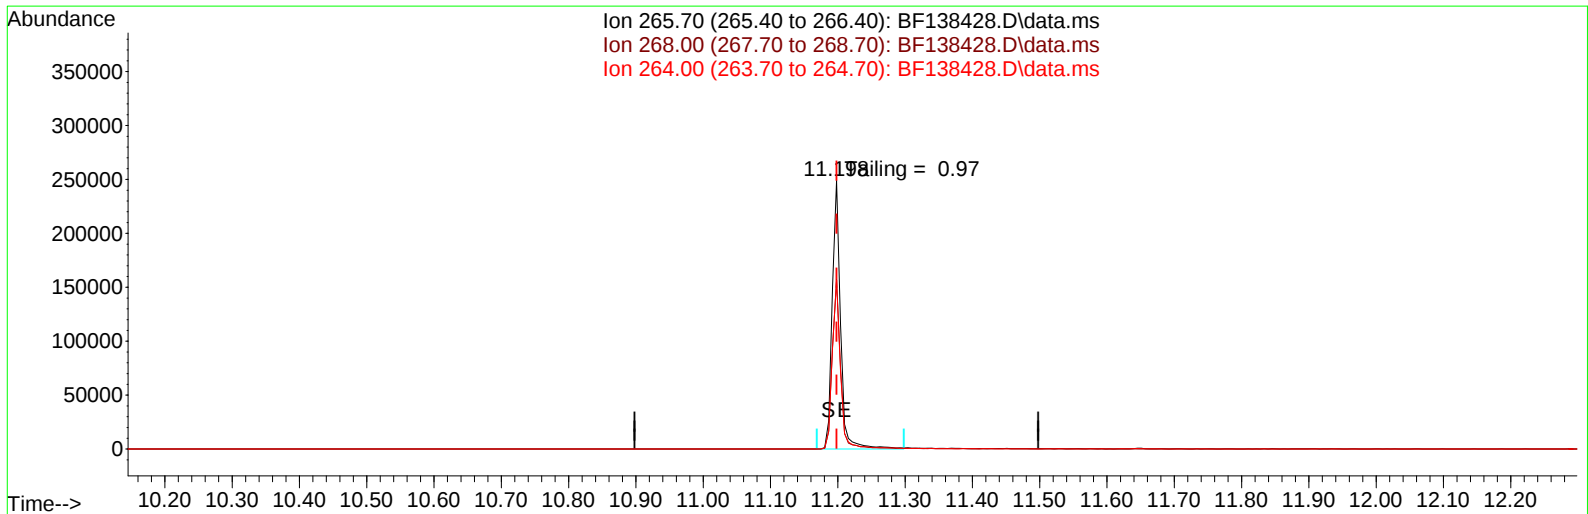

TIC: BF138428.D\data.ms

(70) Pentachlorophenol (C)

11.198min (+ 0.000) 32120.10 ng




response 215350

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.97
264.00	62.50	62.87
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070224\
Data File : BF138428.D
Acq On : 02 Jul 2024 14:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 02 15:35:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

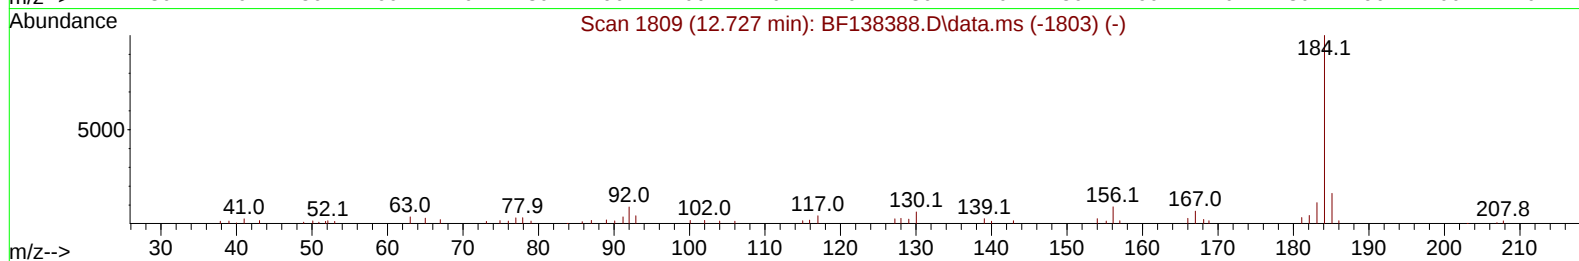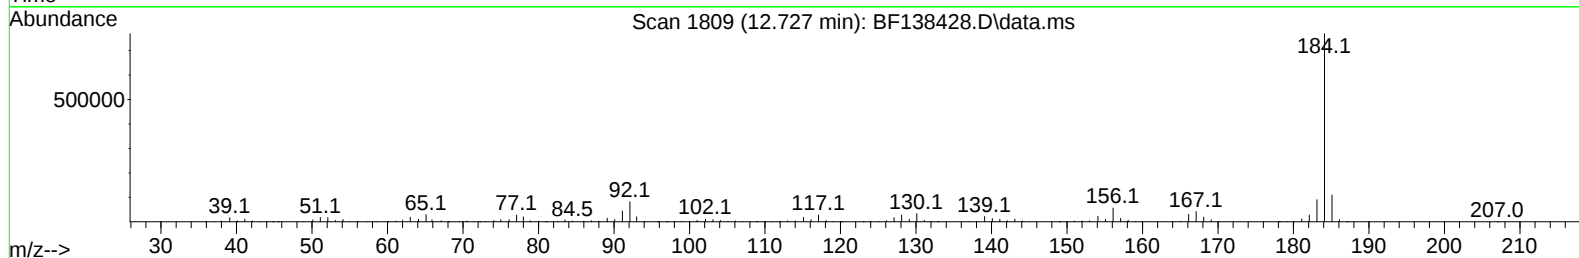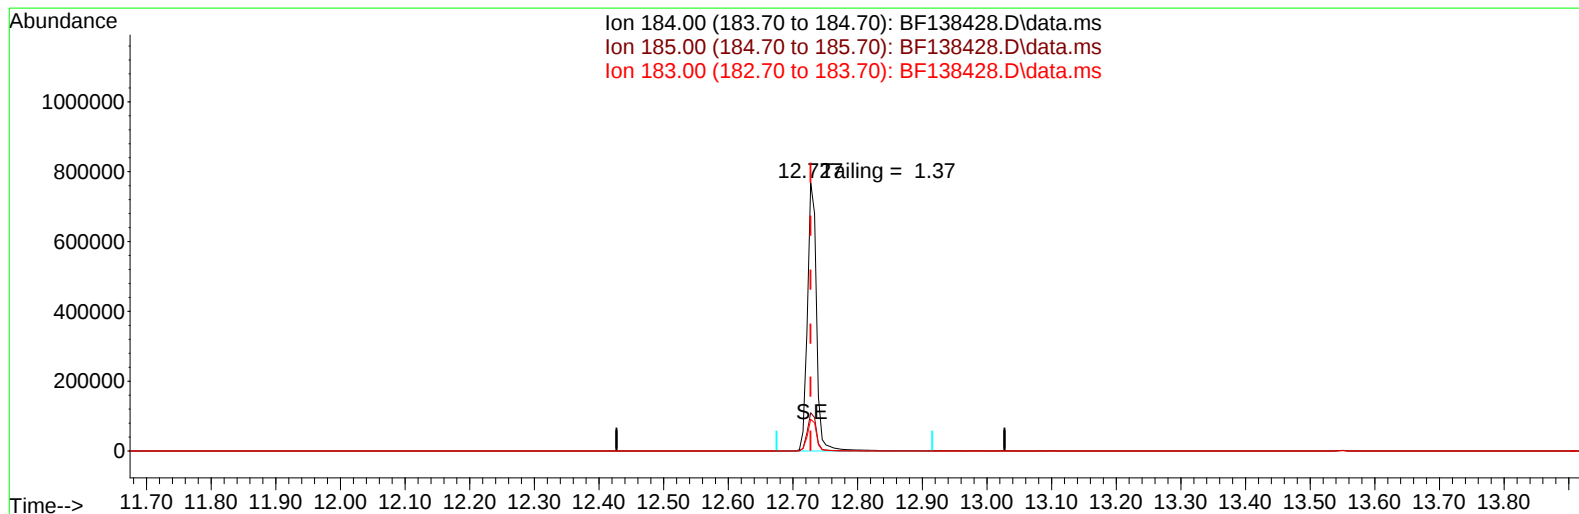

TIC: BF138428.D\data.ms

(77) Benzidine

12.727min (+ 0.000) 0.00 ng

response 750352

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	14.25
183.00	11.30	11.81
0.00	0.00	0.00