
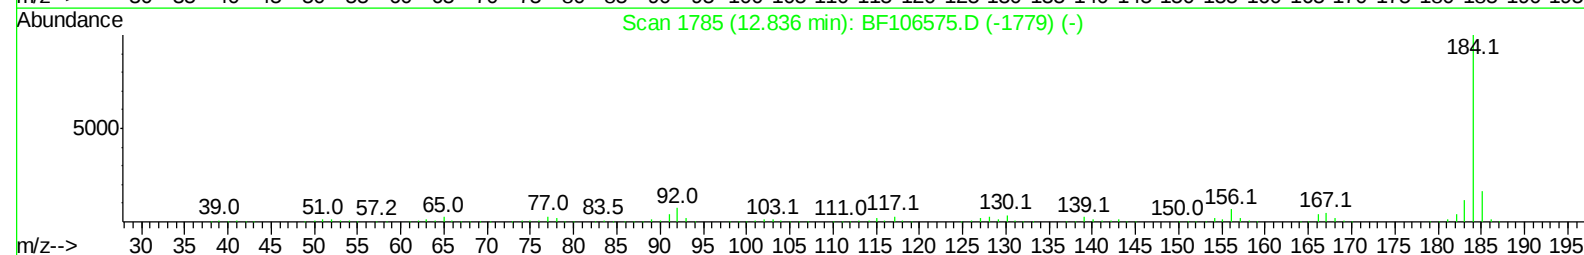
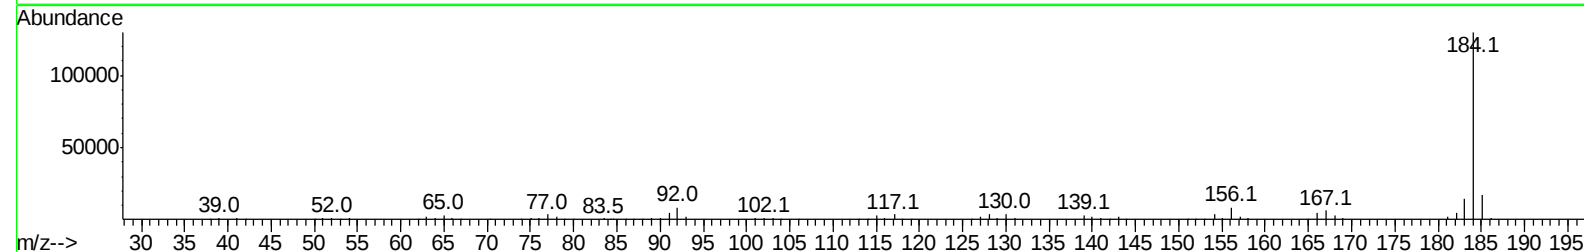


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070318\
Data File : BF107096.D
Acq On : 3 Jul 2018 22:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 04 03:57:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

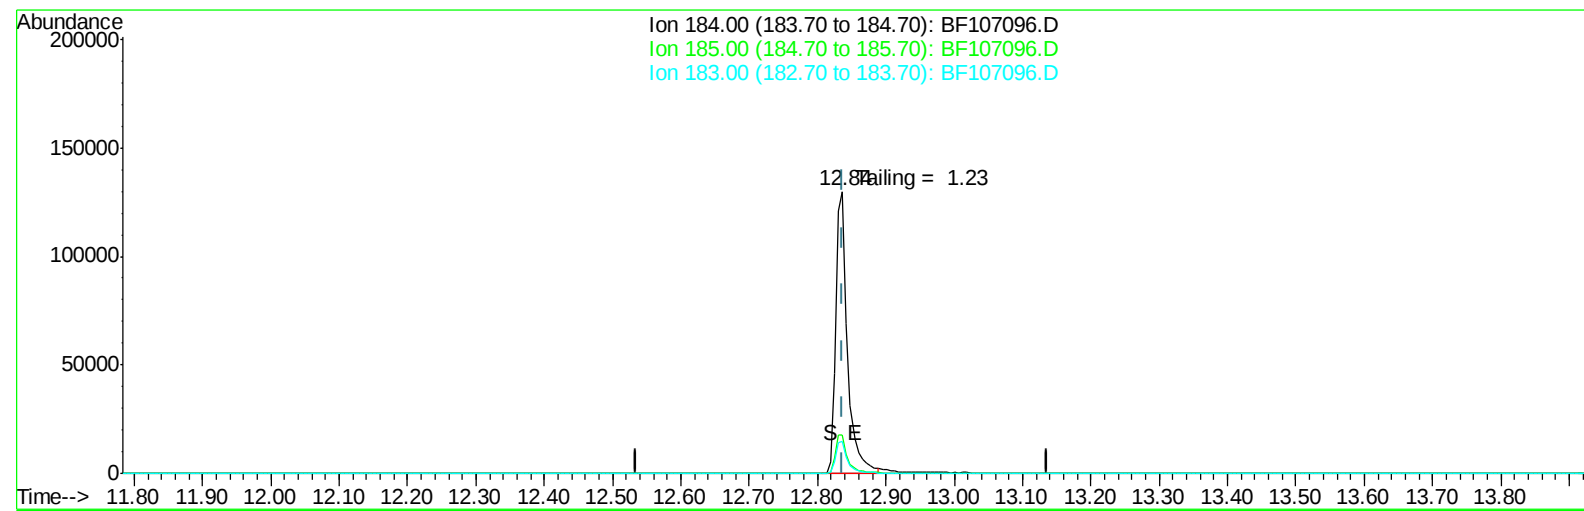

TIC: BF107096.D

(76) Benzidine

12.836min (+0.000) 0.00ng

response 160902

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.46
183.00	11.60	11.27
0.00	0.00	0.00