
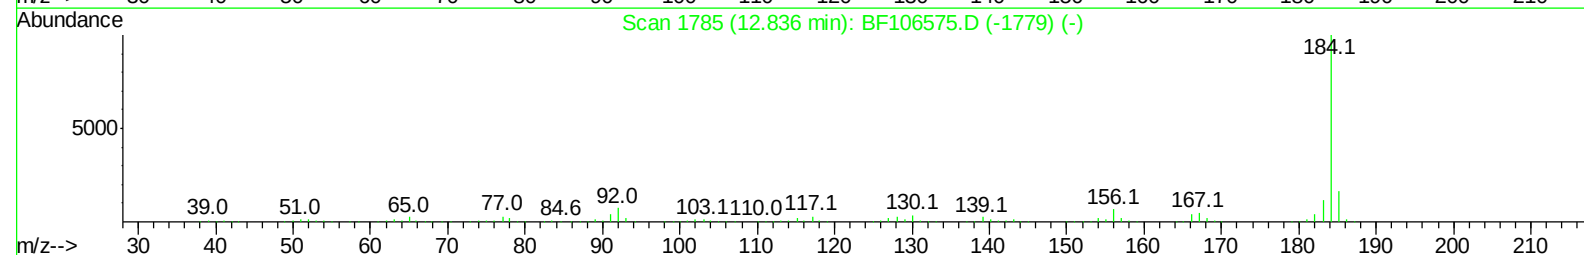
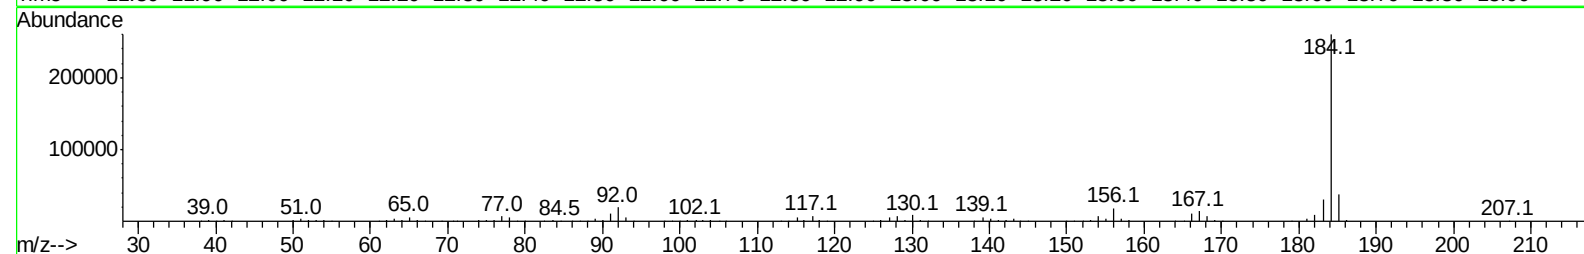


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070318\
 Data File : BF107070.D
 Acq On : 3 Jul 2018 9:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 04 03:59:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 29 14:38:29 2018
 Response via : Initial Calibration

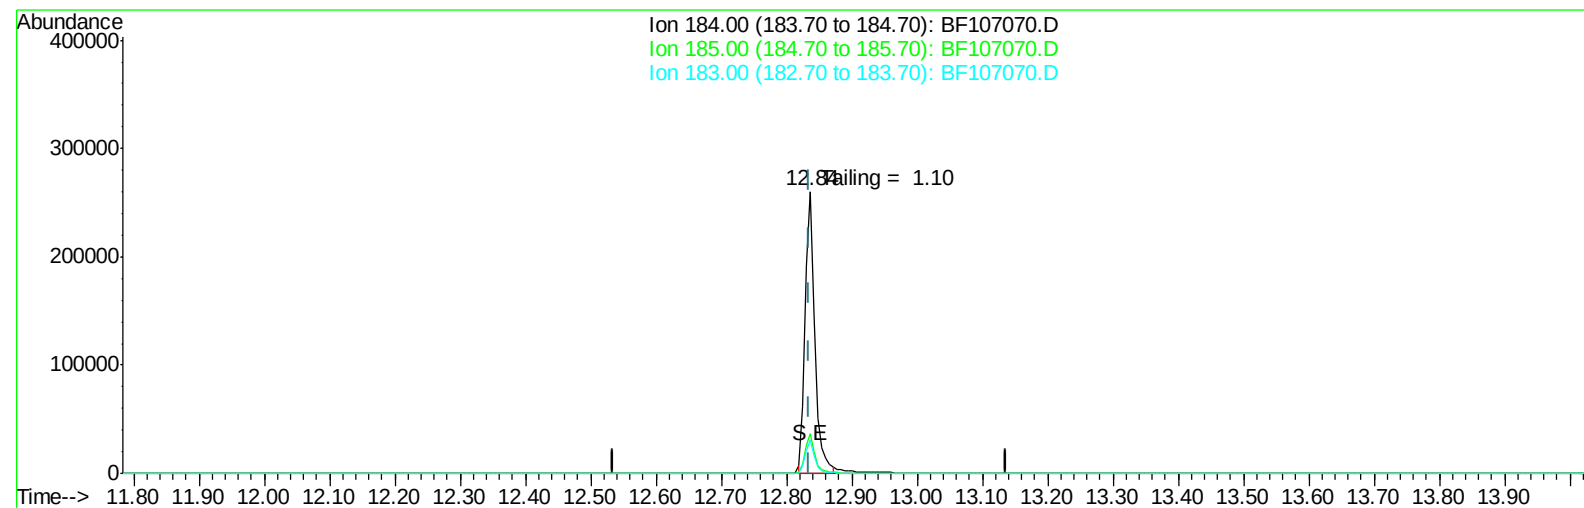

TIC: BF107070.D

(76) Benzidine

12.836min (-0.000) 0.00ng

response 282357

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.18
183.00	11.60	11.67
0.00	0.00	0.00