

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070318\
 Data File : BF107076.D
 Acq On : 3 Jul 2018 12:28
 Operator : JU/SJ
 Sample : J3755-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PS-BASELINEWATER

Quant Time: Jul 03 14:27:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 29 14:38:29 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	57316	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	201018	20.00	ng	0.00
38) Acenaphthene-d10	10.00	164	76818	20.00	ng	0.00
63) Phenanthrene-d10	11.50	188	137905	20.00	ng	0.00
75) Chrysene-d12	14.15	240	178974	20.00	ng	-0.01
86) Perylene-d12	15.71	264	152216	20.00	ng	-0.01

System Monitoring Compounds

5) 2-Fluorophenol	5.63	112	193928	57.29	ng	0.03
7) Phenol-d6	6.62	99	23551	5.57	ng	0.00
23) Nitrobenzene-d5	7.52	82	298206	82.44	ng	-0.01
41) 2,4,6-Tribromophenol	10.80	330	111500	125.23	ng	0.00
44) 2-Fluorobiphenyl	9.32	172	492984	113.59	ng	0.00
78) Terphenyl-d14	13.08	244	578202	78.26	ng	0.00

Target Compounds


						Qvalue
15) Benzyl Alcohol	7.11	79	7305	2.152	ng	# 65
17) 2-Methylphenol	7.27	107	9088	2.860	ng	# 86
19) n-Nitroso-di-n-propylamine	7.35	70	25875	9.286	ng	# 66
22) Acetophenone	7.36	105	37423	8.321	ng	# 94
25) Isophorone	7.78	82	517734	81.227	ng	98
32) Benzoic acid	8.04	122	1132	6.240	ng	# 23
36) 4-Chloro-3-methylphenol	8.82	107	19546	6.583	ng	# 34
47) 2-Nitroaniline	9.55	65	3443	2.125	ng	# 22
49) Dimethylphthalate	9.71	163	112892	19.594	ng	99
50) 2,6-Dinitrotoluene	9.74	165	22146	18.152	ng	# 29
52) 3-Nitroaniline	9.77	138	5063	3.606	ng	87
53) 2,4-Dinitrophenol	9.97	184	576	6.200	ng	# 52
54) Dibenzofuran	10.48	168	131525	20.049	ng	# 62
55) 4-Nitrophenol	10.14	139	2086	2.129	ng	# 56
59) Diethylphthalate	10.41	149	101919	18.328	ng	# 93
61) 4-Nitroaniline	10.48	138	3267	2.345	ng	89
62) Azobenzene	10.48	77	13489	2.463	ng	92
66) 4-Bromophenyl-phenylether	10.80	248	6708	4.076	ng	# 1
76) Benzidine	12.58	184	18510	3.631	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070318\
Data File : BF107076.D
Acq On : 3 Jul 2018 12:28
Operator : JU/SJ
Sample : J3755-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PS-BASELINEWATER

Quant Time: Jul 03 13:59:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

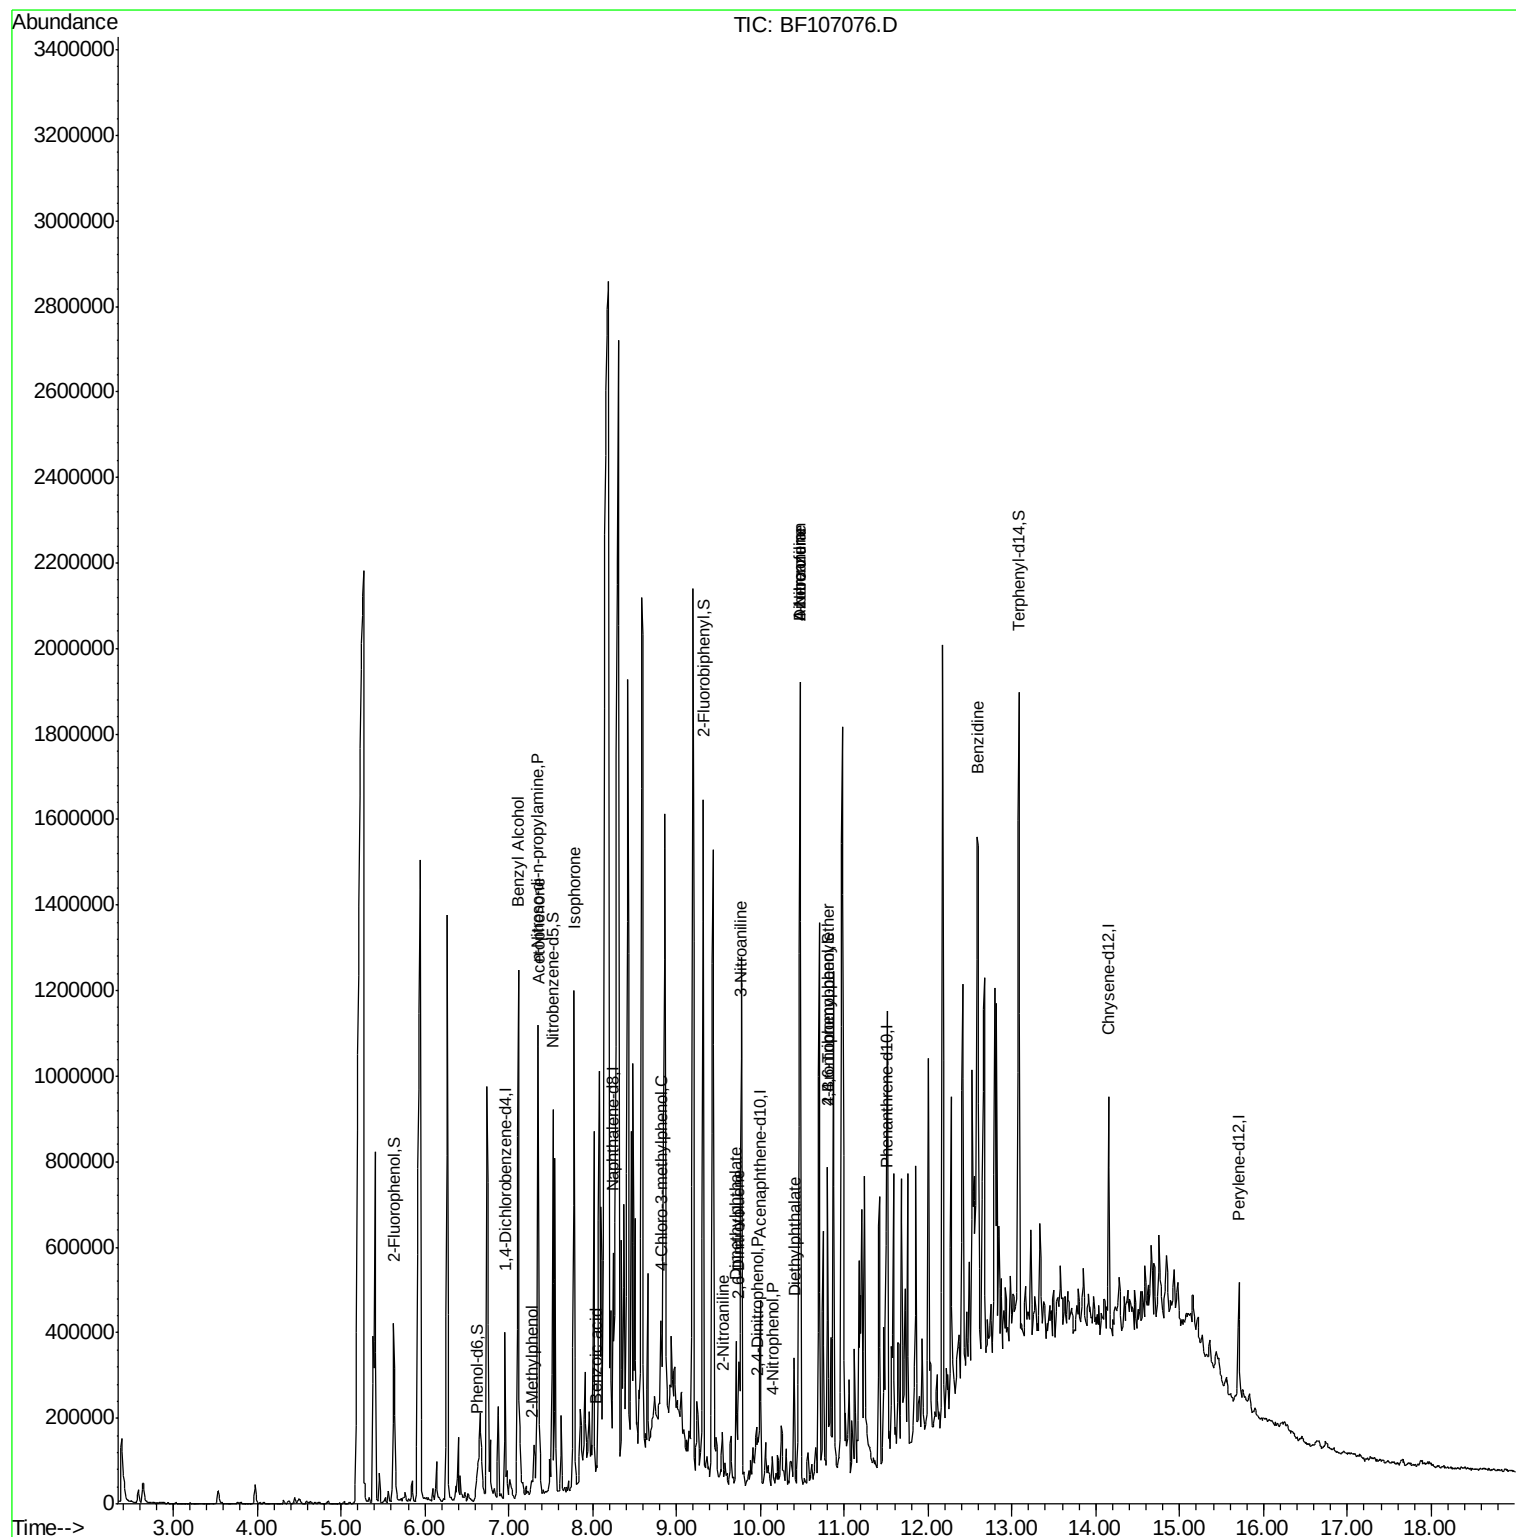

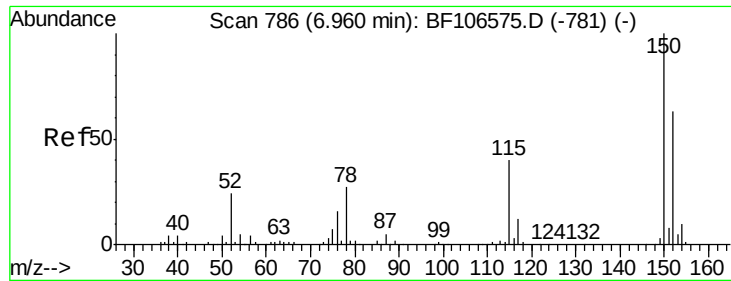


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF107076.D
Acq: 3 Jul 2018 12:28

Instrument :
BNA_F
ClientSampleId :
PS-BASELINEWATER

Tgt Ion:152 Resp: 57316
Ion Ratio Lower Upper
152 100
150 159.2 124.6 186.8
115 63.8 50.1 75.1




Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

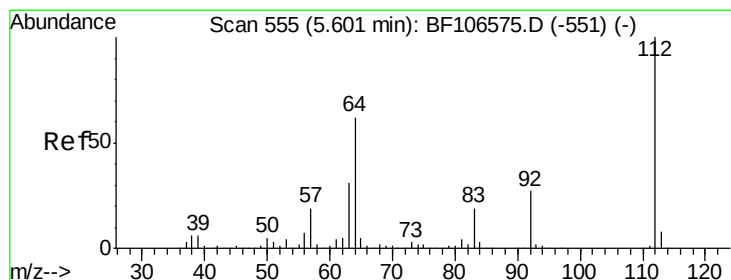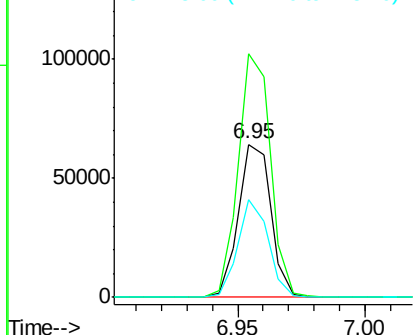



#5


2-Fluorophenol
Concen: 57.293 ng
RT: 5.63 min Scan# 560
Delta R.T. 0.03 min
Lab File: BF107076.D
Acq: 3 Jul 2018 12:28

Tgt Ion:112 Resp: 193928
Ion Ratio Lower Upper
112 100
64 56.7 47.9 71.9
63 27.4 23.7 35.5

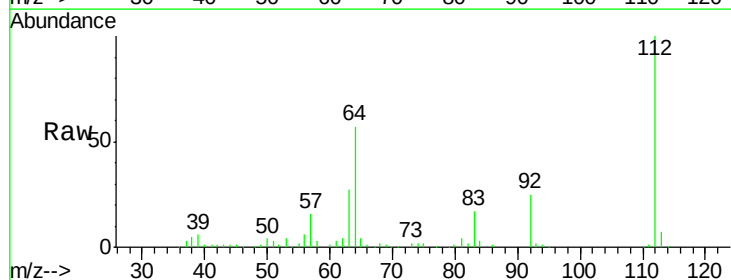

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

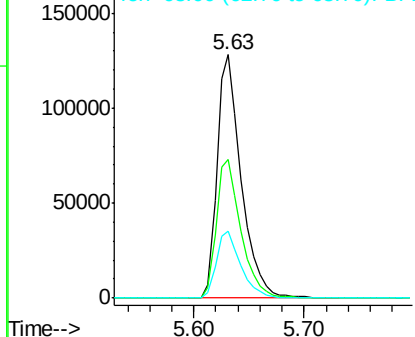



#7

Phenol-d6

Concen: 5.572 ng

RT: 6.62 min Scan# 728

Delta R.T. 0.01 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28

Instrument :

BNA_F

ClientSampleId :

PS-BASELINEWATER


Tgt Ion: 99 Resp: 23551

Ion Ratio Lower Upper

99 100

42 19.3 14.5 21.7




71 33.6 25.4 38.0



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

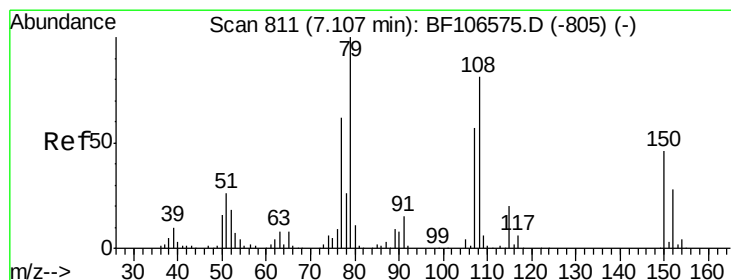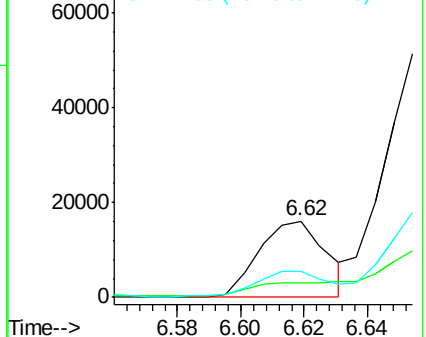

#15

Benzyl Alcohol

Concen: 2.152 ng

RT: 7.11 min Scan# 812

Delta R.T. 0.01 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28


Tgt Ion: 79 Resp: 7305

Ion Ratio Lower Upper

79 100

108 58.7 65.1 97.7#



77 99.8 50.6 75.8#




Abundance Ion 79.00 (78.70 to 79.70): BF1

Ion 108.00 (107.70 to 108.70): BF1

Ion 77.00 (76.70 to 77.70): BF1

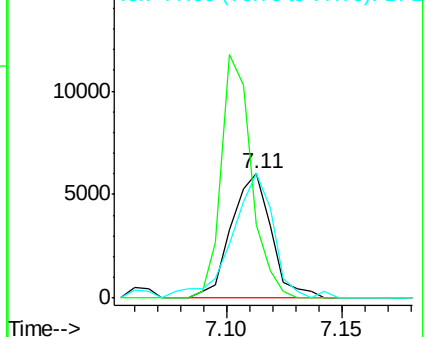

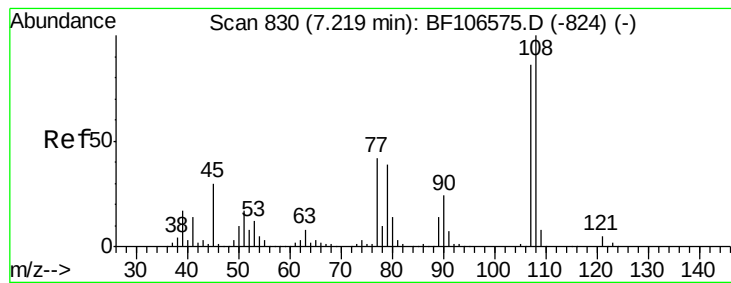

#17

2-Methylphenol

Concen: 2.860 ng

RT: 7.27 min Scan# 839

Delta R.T. 0.05 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28

Instrument :

BNA_F

ClientSampleId :

PS-BASELINEWATER

Tgt Ion: 107 Resp: 9088


Ion Ratio Lower Upper

107 100

108 101.0 91.7 137.5

77 57.8 33.8 50.8#

79 47.1 33.8 50.8






Abundance Ion 107.00 (106.70 to 107.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 77.00 (76.70 to 77.70): BF1

Ion 79.00 (78.70 to 79.70): BF1

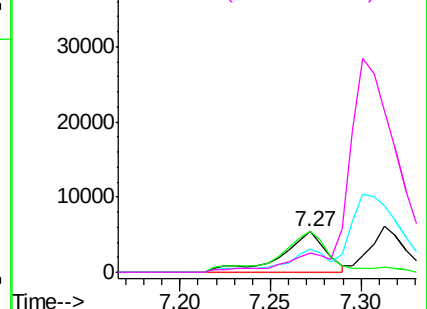

#19

n-Nitroso-di-n-propylamine

Concen: 9.286 ng

RT: 7.35 min Scan# 852

Delta R.T. -0.04 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28

Tgt Ion: 70 Resp: 25875


Ion Ratio Lower Upper

70 100

42 34.5 47.5 71.3#

101 4.9 7.4 11.2#

130 0.0 16.6 25.0#






Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): E

Ion 130.00 (129.70 to 130.70): E

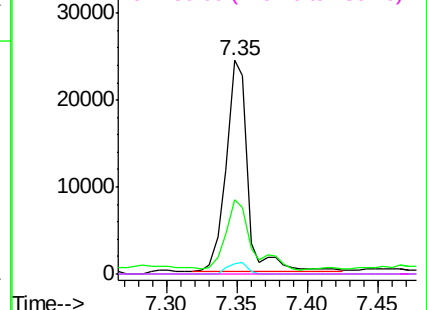

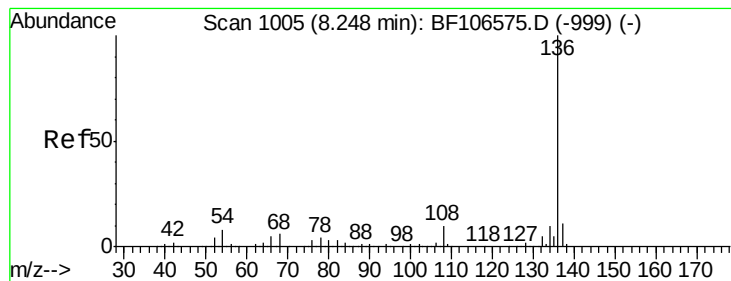

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1005

Delta R.T. -0.00 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28

Instrument :

BNA_F

ClientSampleId :

PS-BASELINEWATER

Tgt Ion:136 Resp: 201018


Ion Ratio Lower Upper

136 100

137 10.8 8.9 13.3

54 7.6 6.6 9.8

68 6.4 5.0 7.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

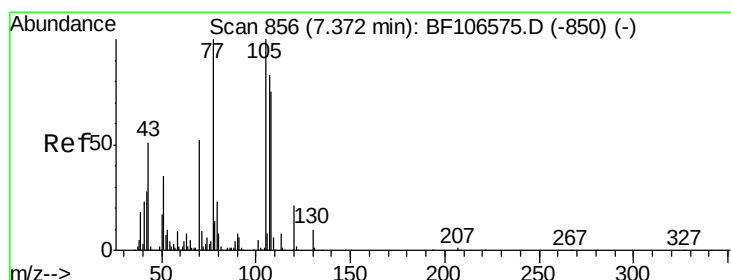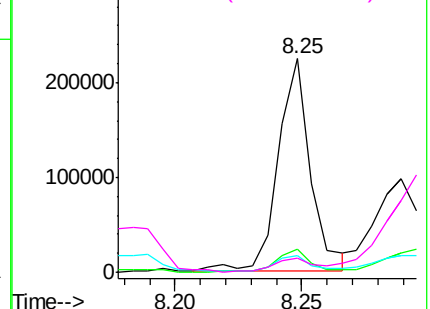

#22

Acetophenone

Concen: 8.321 ng

RT: 7.36 min Scan# 854

Delta R.T. -0.01 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28

Tgt Ion:105 Resp: 37423


Ion Ratio Lower Upper

105 100

71 21.1 4.4 6.6#

51 28.7 22.3 33.5

120 21.3 16.9 25.3






Abundance Ion 105.00 (104.70 to 105.70): E

Ion 71.00 (70.70 to 71.70): BF1

Ion 51.00 (50.70 to 51.70): BF1

Ion 120.00 (119.70 to 120.70): E

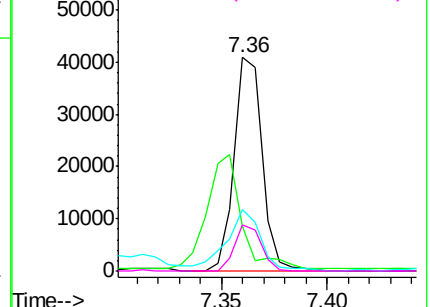



#23

Nitrobenzene-d5

Concen: 82.442 ng

RT: 7.52 min Scan# 882

Delta R.T. -0.01 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28

Instrument :

BNA_F

ClientSampleId :

PS-BASELINEWATER


Tgt Ion: 82 Resp: 298206

Ion Ratio Lower Upper

82 100

128 44.7 36.1 54.1




54 48.4 41.4 62.2



Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

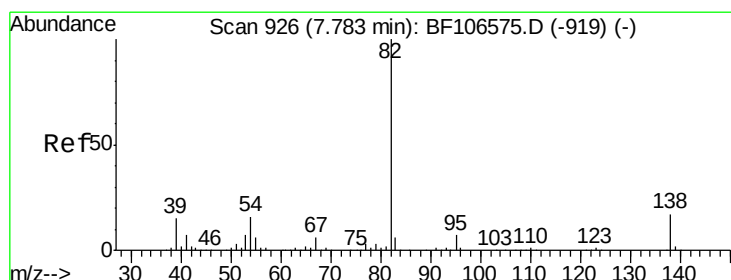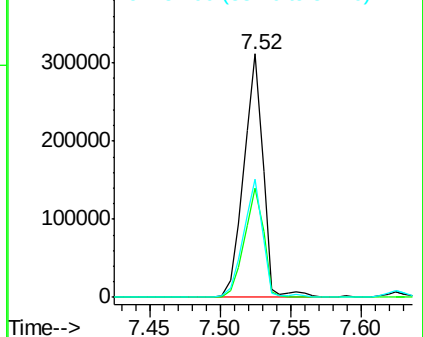

#25

Isophorone

Concen: 81.227 ng

RT: 7.78 min Scan# 926

Delta R.T. -0.01 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28


Tgt Ion: 82 Resp: 517734

Ion Ratio Lower Upper

82 100

95 7.3 5.2 7.8



138 19.4 14.9 22.3




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1




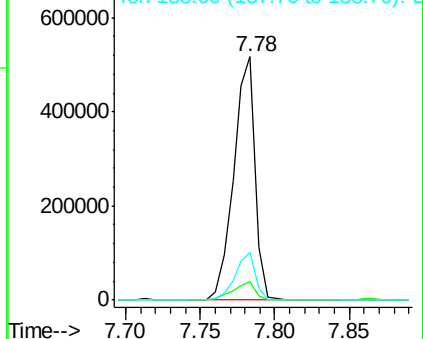




#32
Benzoic acid
Concen: 6.240 ng
RT: 8.04 min Scan# 970
Delta R.T. -0.00 min
Lab File: BF107076.D
Acq: 3 Jul 2018 12:28




Instrument :
BNA_F
ClientSampleId :
PS-BASELINEWATER


Tgt Ion:122 Resp: 1132
Ion Ratio Lower Upper
122 100
105 0.0 101.1 141.1#
77 123.4 70.7 110.7#

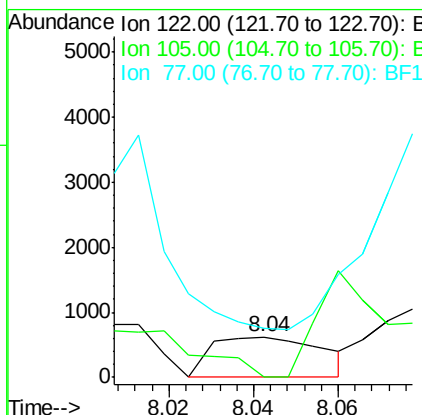

#36
4-Chloro-3-methylphenol
Concen: 6.583 ng
RT: 8.82 min Scan# 1103
Delta R.T. 0.02 min
Lab File: BF107076.D
Acq: 3 Jul 2018 12:28

Tgt Ion:107 Resp: 19546
Ion Ratio Lower Upper
107 100
144 0.0 20.5 30.7#
142 15.5 62.0 93.0#

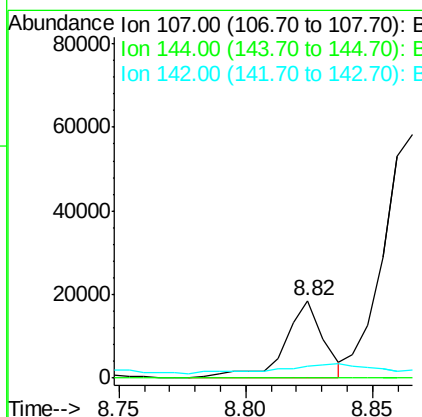


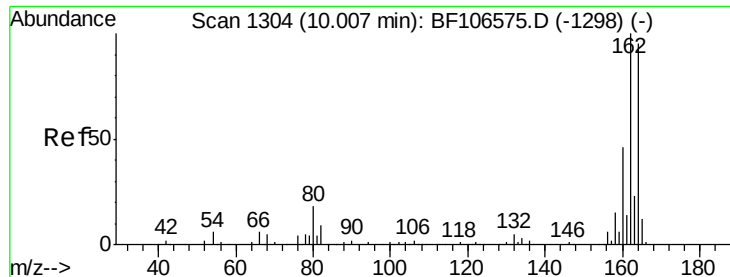




#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.00 min Scan# 1303
 Delta R.T. -0.01 min
 Lab File: BF107076.D
 Acq: 3 Jul 2018 12:28

Instrument :
 BNA_F
 ClientSampleId :
 PS-BASELINEWATER

Tgt Ion:164 Resp: 76818
 Ion Ratio Lower Upper
 164 100
 162 98.4 86.1 129.1
 160 43.5 38.3 57.5

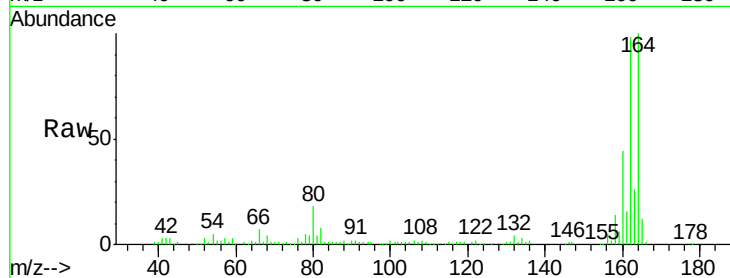


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

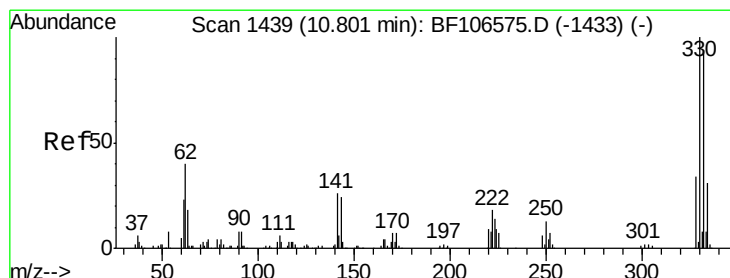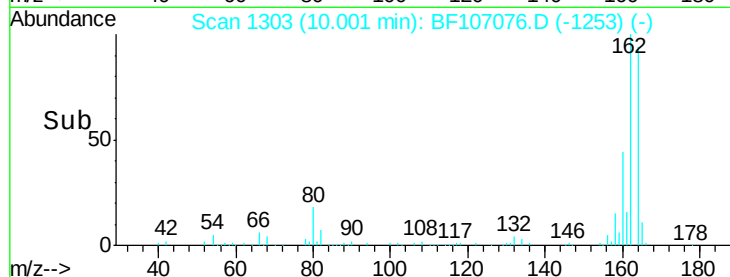
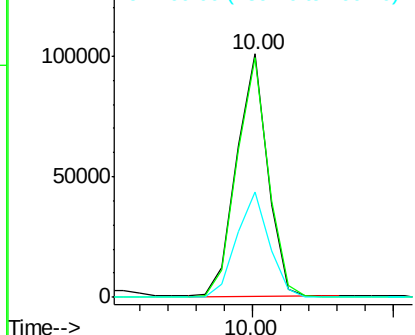



#41
 2,4,6-Tribromophenol
 Concen: 125.233 ng
 RT: 10.80 min Scan# 1439
 Delta R.T. -0.00 min
 Lab File: BF107076.D
 Acq: 3 Jul 2018 12:28

Tgt Ion:330 Resp: 111500
 Ion Ratio Lower Upper
 330 100
 332 97.9 77.0 115.6
 141 24.2 29.9 44.9#

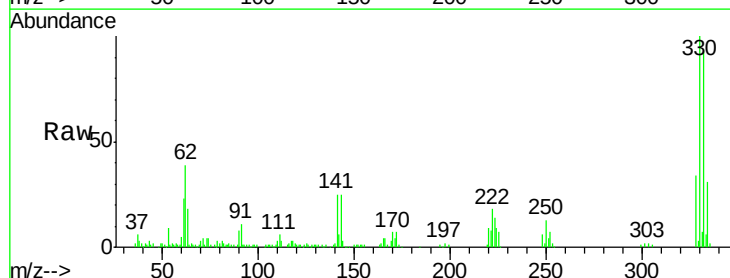

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

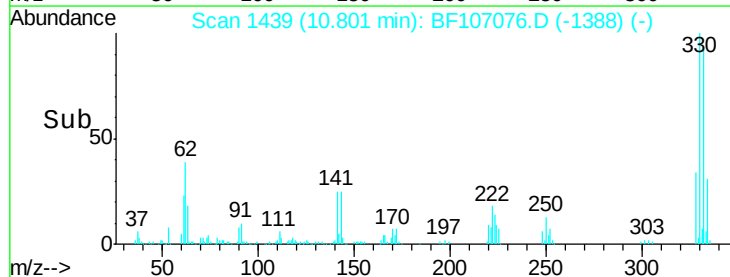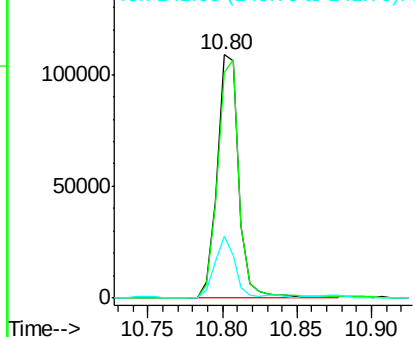


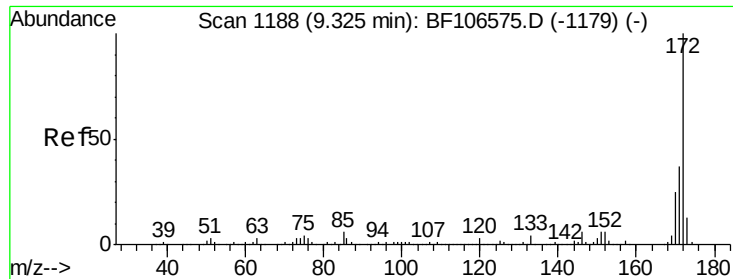




#44
 2-Fluorobiphenyl
 Concen: 113.586 ng
 RT: 9.32 min Scan# 1187
 Delta R.T. -0.01 min
 Lab File: BF107076.D
 Acq: 3 Jul 2018 12:28

Instrument :
 BNA_F
 ClientSampleId :
 PS-BASELINEWATER

Tgt Ion: 172 Resp: 492984
 Ion Ratio Lower Upper
 172 100
 171 36.4 29.7 44.5
 170 24.2 19.6 29.4

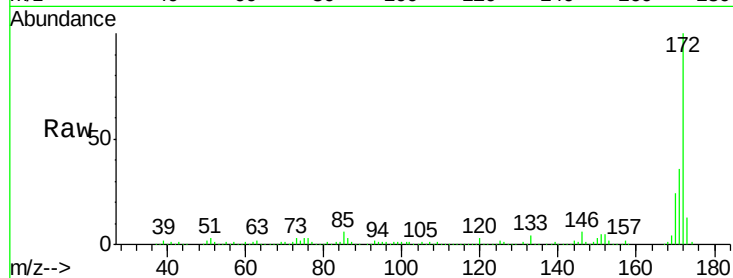


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

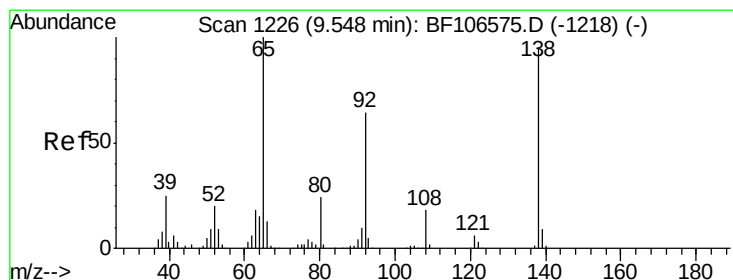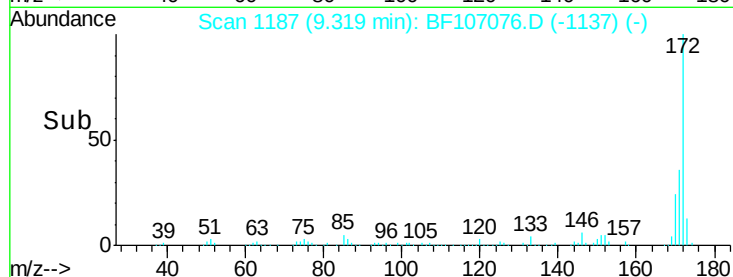
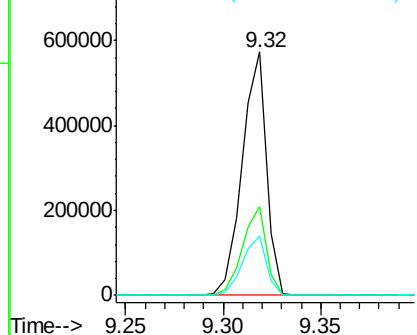



#47
 2-Nitroaniline
 Concen: 2.125 ng
 RT: 9.55 min Scan# 1226
 Delta R.T. -0.01 min
 Lab File: BF107076.D
 Acq: 3 Jul 2018 12:28

Tgt Ion: 65 Resp: 3443
 Ion Ratio Lower Upper
 65 100
 92 96.8 55.8 83.6#
 138 0.0 91.2 136.8#

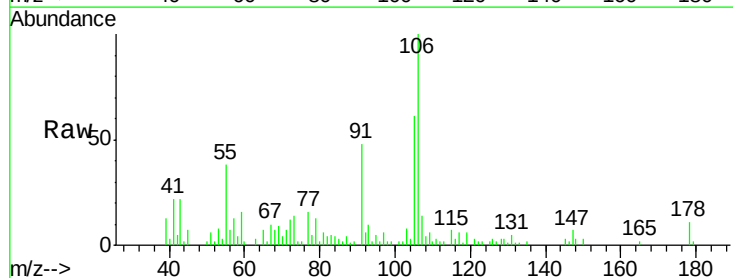

Abundance Ion 65.00 (64.70 to 65.70): BF1
 Ion 92.00 (91.70 to 92.70): BF1
 Ion 138.00 (137.70 to 138.70): E

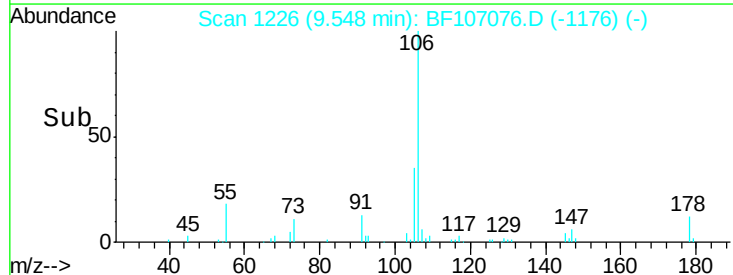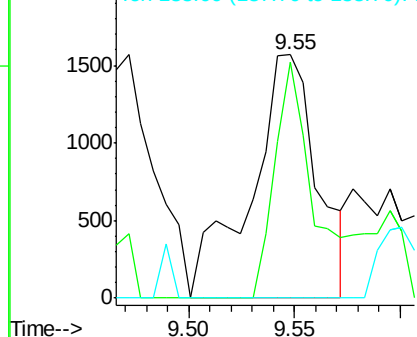


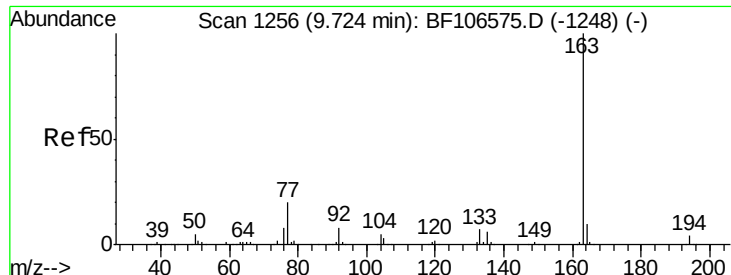




#49
Dimethylphthalate
Concen: 19.594 ng
RT: 9.71 min Scan# 1254
Delta R.T. -0.01 min
Lab File: BF107076.D
Acq: 3 Jul 2018 12:28

Instrument :
BNA_F
ClientSampleId :
PS-BASELINEWATER

Tgt Ion:163 Resp: 112892
Ion Ratio Lower Upper
163 100
194 4.1 2.7 4.1
164 10.7 8.2 12.2




Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

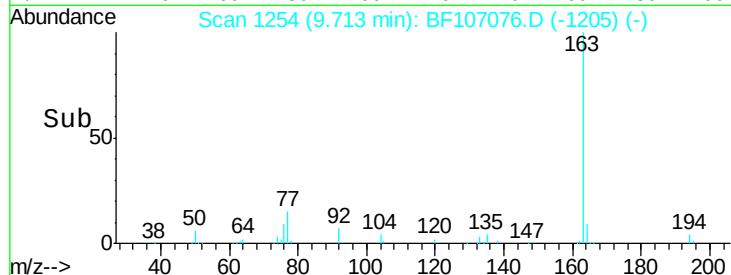
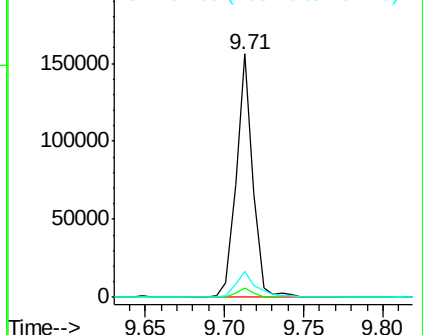



#50
2,6-Dinitrotoluene
Concen: 18.152 ng
RT: 9.74 min Scan# 1258
Delta R.T. -0.06 min
Lab File: BF107076.D
Acq: 3 Jul 2018 12:28

Tgt Ion:165 Resp: 22146
Ion Ratio Lower Upper
165 100
63 2.3 44.7 67.1#
89 5.9 44.0 66.0#



Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1

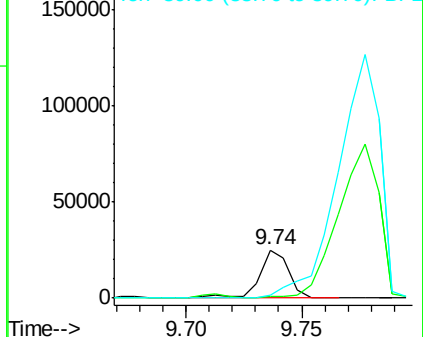

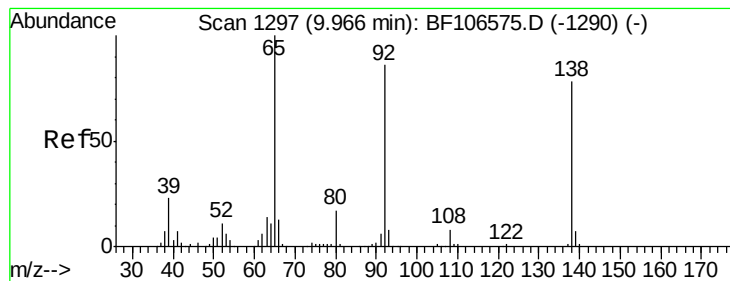

#52

3-Nitroaniline

Concen: 3.606 ng

RT: 9.77 min Scan# 1263

Delta R.T. -0.21 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28

Instrument :

BNA_F

ClientSampleId :

PS-BASELINEWATER


Tgt Ion:138 Resp: 5063

Ion Ratio Lower Upper

138 100

108 12.1 9.4 14.0




92 96.8 89.4 134.2

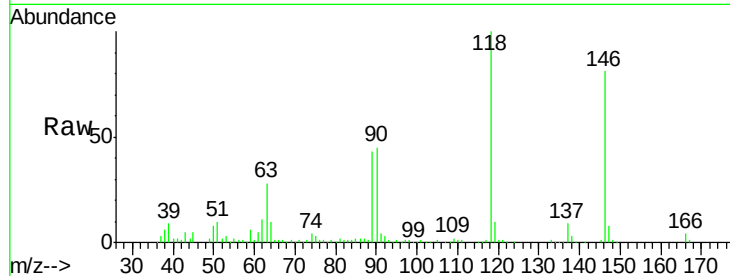

Abundance Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): BF1

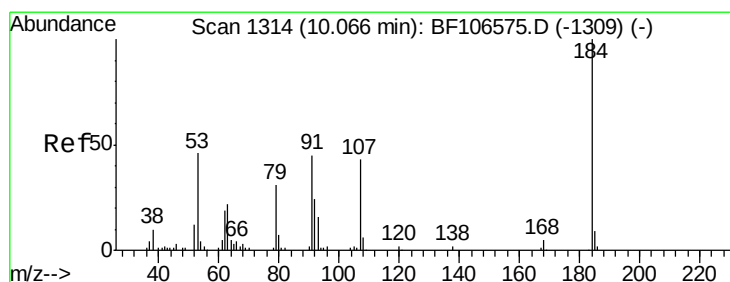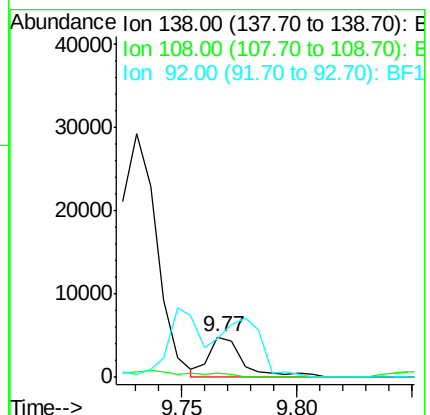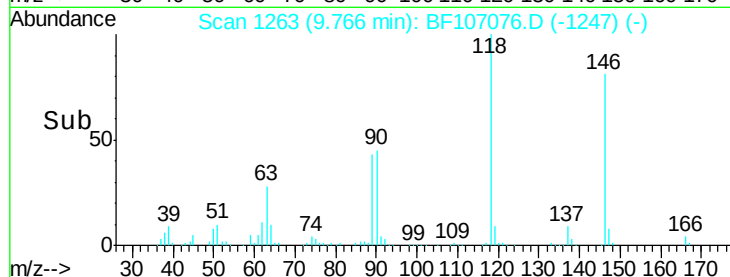

#53

2,4-Dinitrophenol

Concen: 6.200 ng

RT: 9.97 min Scan# 1297

Delta R.T. -0.11 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28


Tgt Ion:184 Resp: 576

Ion Ratio Lower Upper

184 100

63 83.6 54.2 81.2#



154 137.5 184.0 276.0#

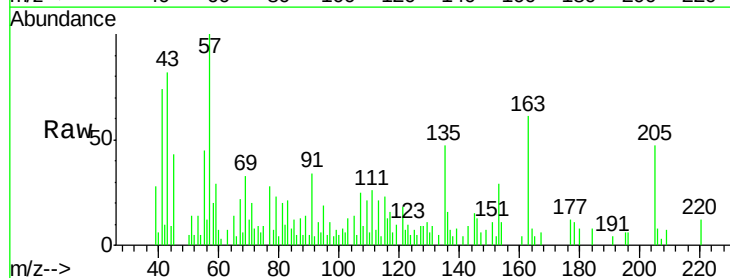


Abundance Ion 184.00 (183.70 to 184.70): E

Ion 63.00 (62.70 to 63.70): BF1

Ion 154.00 (153.70 to 154.70): E

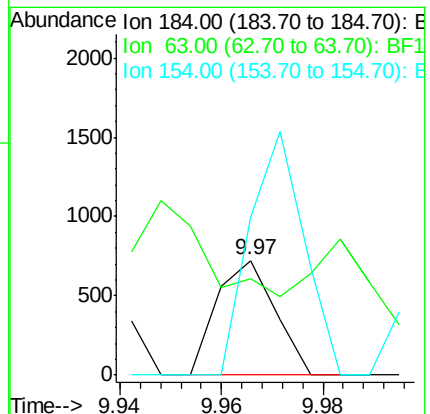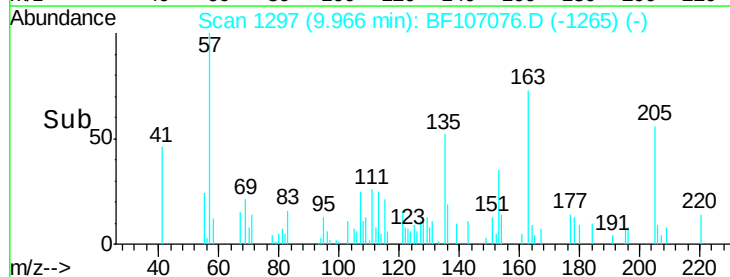

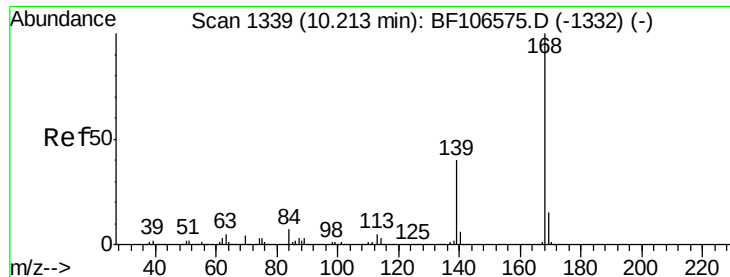

#54

Dibenzofuran

Concen: 20.049 ng

RT: 10.48 min Scan# 1384

Delta R.T. 0.26 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28

Instrument :

BNA_F

ClientSampleId :

PS-BASELINEWATER


Tgt Ion:168 Resp: 131525

Ion Ratio Lower Upper

168 100

139 7.0 30.1 45.1#




169 12.7 10.9 16.3

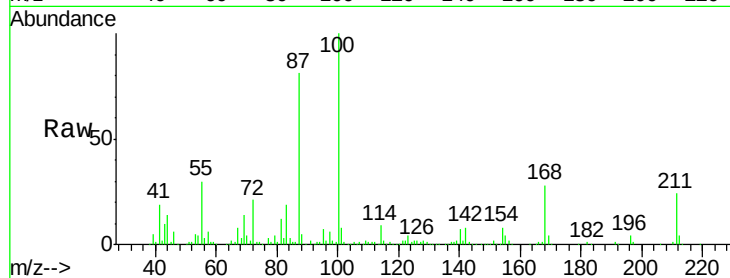

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E

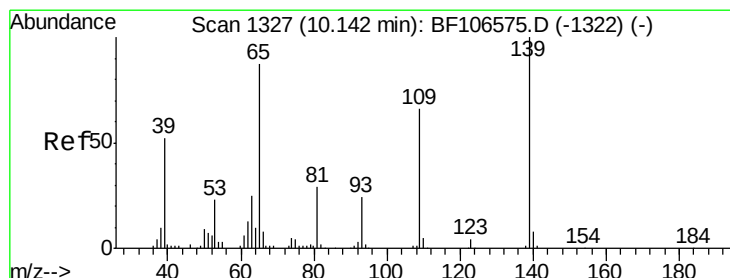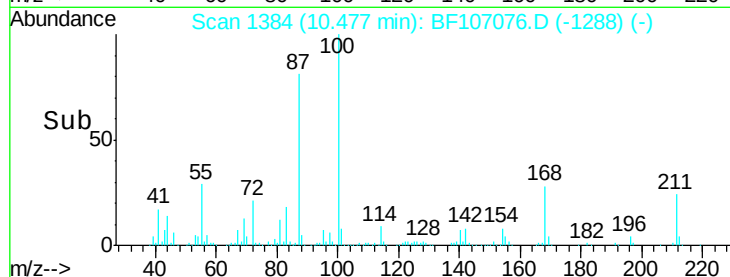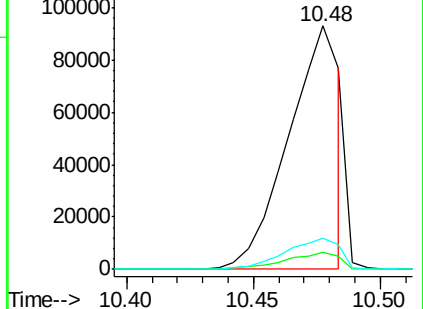

#55

4-Nitrophenol

Concen: 2.129 ng

RT: 10.14 min Scan# 1326

Delta R.T. -0.01 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28


Tgt Ion:139 Resp: 2086

Ion Ratio Lower Upper

139 100

109 39.0 48.4 88.4#



65 45.6 72.6 112.6#

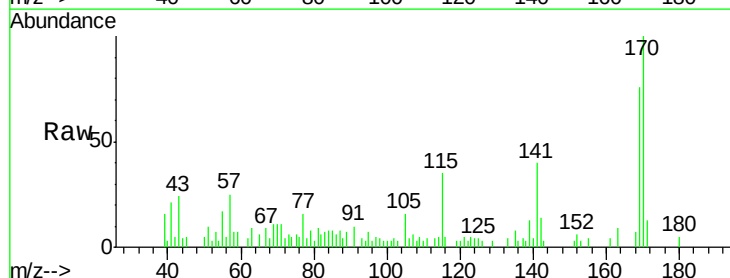


Abundance Ion 139.00 (138.70 to 139.70): E

Ion 109.00 (108.70 to 109.70): E

Ion 65.00 (64.70 to 65.70): BF1

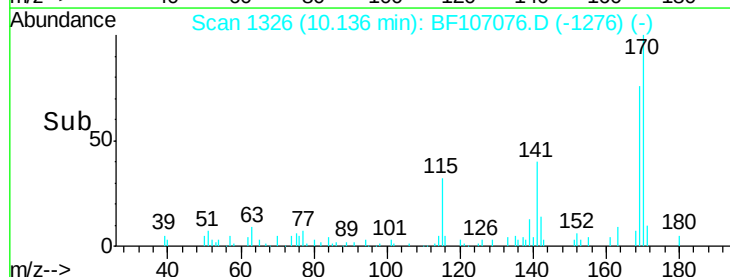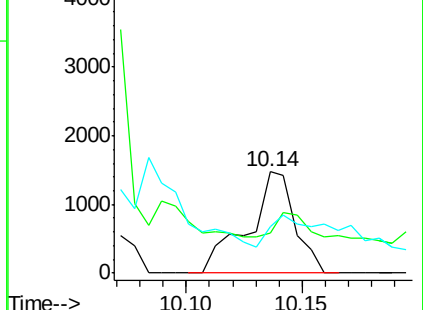







#59
Diethylphthalate
Concen: 18.328 ng
RT: 10.41 min Scan# 1372
Delta R.T. -0.01 min
Lab File: BF107076.D
Acq: 3 Jul 2018 12:28

Instrument :
BNA_F
ClientSampleId :
PS-BASELINEWATER

Tgt Ion:149 Resp: 101919
Ion Ratio Lower Upper
149 100
177 25.1 16.1 24.1#
150 12.0 10.1 15.1




Abundance Ion 149.00 (148.70 to 149.70): E
Ion 177.00 (176.70 to 177.70): E
Ion 150.00 (149.70 to 150.70): E


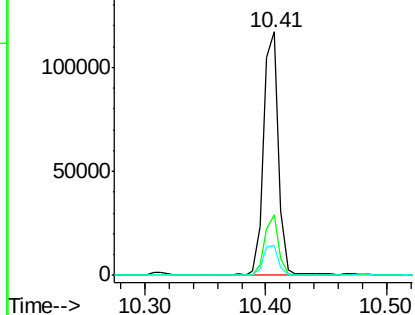



#61
4-Nitroaniline
Concen: 2.345 ng
RT: 10.48 min Scan# 1384
Delta R.T. -0.11 min
Lab File: BF107076.D
Acq: 3 Jul 2018 12:28

Tgt Ion:138 Resp: 3267
Ion Ratio Lower Upper
138 100
92 61.2 30.2 70.2
108 66.2 52.5 92.5



Abundance Ion 138.00 (137.70 to 138.70): E
Ion 92.00 (91.70 to 92.70): BF1
Ion 108.00 (107.70 to 108.70): E




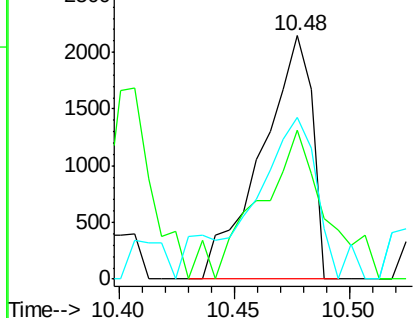




#62
Azobenzene
Concen: 2.463 ng
RT: 10.48 min Scan# 1384
Delta R.T. -0.23 min
Lab File: BF107076.D
Acq: 3 Jul 2018 12:28




Instrument :
BNA_F
ClientSampleId :
PS-BASELINEWATER


Tgt Ion: 77 Resp: 13489
Ion Ratio Lower Upper
77 100
182 30.8 1.7 41.7
105 21.3 3.0 43.0
51 32.1 9.9 49.9

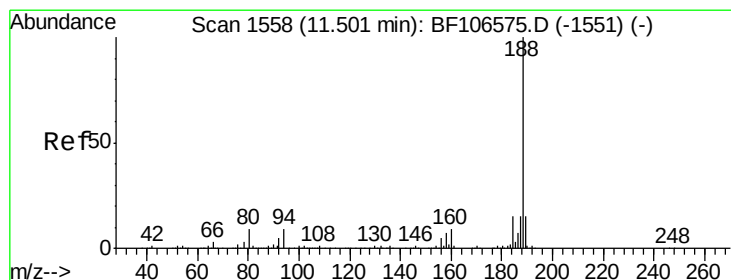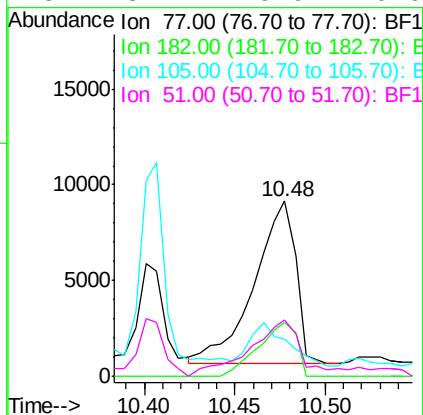

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.50 min Scan# 1557
Delta R.T. -0.01 min
Lab File: BF107076.D
Acq: 3 Jul 2018 12:28

Tgt Ion: 188 Resp: 137905
Ion Ratio Lower Upper
188 100
94 9.7 8.5 12.7
80 9.9 9.2 13.8

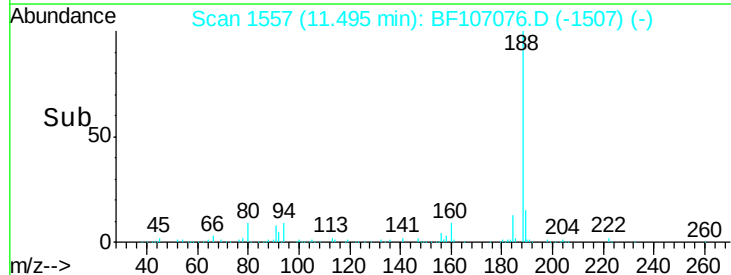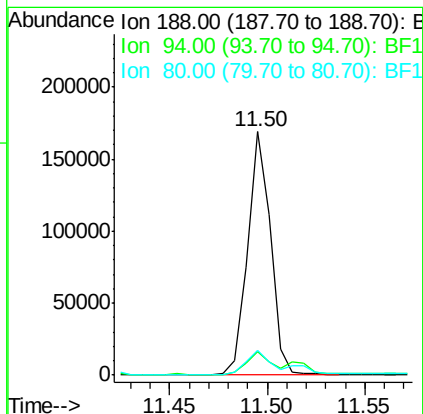


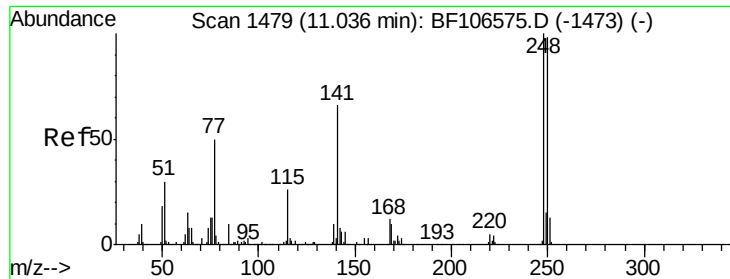




#66
 4-Bromophenyl-phenylether
 Concen: 4.076 ng
 RT: 10.80 min Scan# 1439
 Delta R.T. -0.24 min
 Lab File: BF107076.D
 Acq: 3 Jul 2018 12:28

Instrument :
 BNA_F
 ClientSampleId :
 PS-BASELINEWATER

Tgt Ion:248 Resp: 6708
 Ion Ratio Lower Upper
 248 100
 250 202.7 76.9 115.3#
 141 395.2 74.4 111.6#

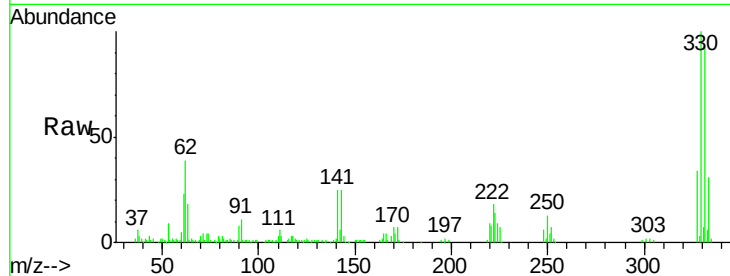


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

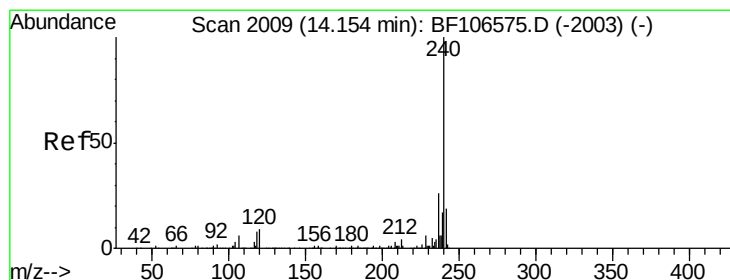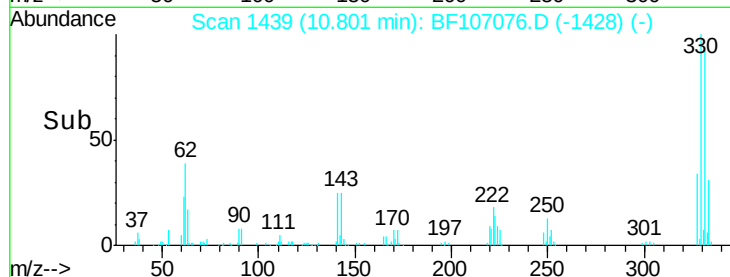
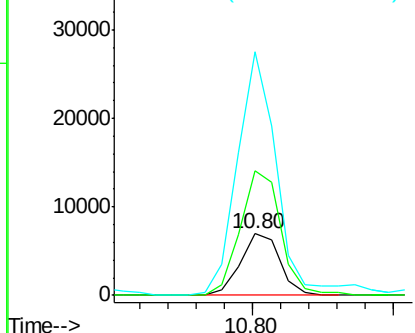



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.15 min Scan# 2009
 Delta R.T. -0.01 min
 Lab File: BF107076.D
 Acq: 3 Jul 2018 12:28

Tgt Ion:240 Resp: 178974
 Ion Ratio Lower Upper
 240 100
 120 9.3 9.5 14.3#
 236 24.5 20.7 31.1

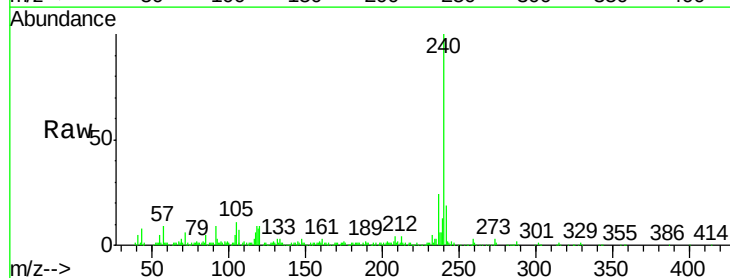

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E

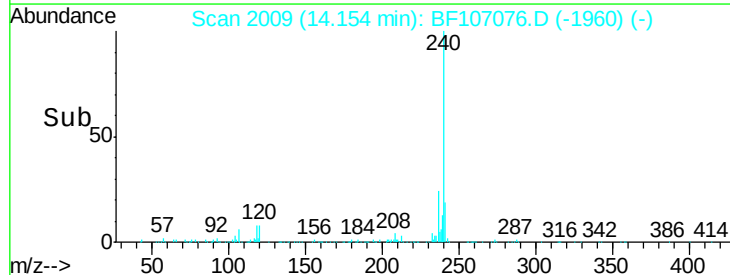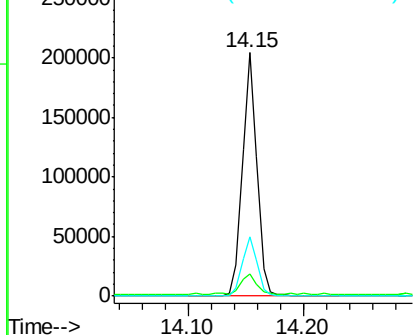



#76

Benzidine

Concen: 3.631 ng

RT: 12.58 min Scan# 1742

Delta R.T. -0.25 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28

Instrument :

BNA_F

ClientSampleId :

PS-BASELINEWATER


Tgt Ion:184 Resp: 18510

Ion Ratio Lower Upper

184 100

185 17.4 12.6 18.8




183 10.1 9.3 13.9



Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

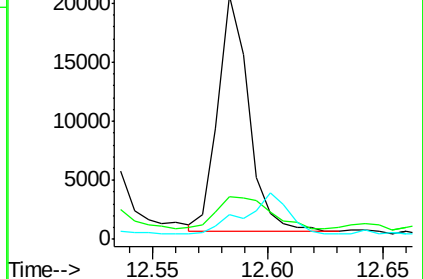

#78

Terphenyl-d14

Concen: 78.256 ng

RT: 13.08 min Scan# 1827

Delta R.T. -0.00 min

Lab File: BF107076.D

Acq: 3 Jul 2018 12:28


Tgt Ion:244 Resp: 578202

Ion Ratio Lower Upper

244 100

212 6.6 5.4 8.0



122 8.6 11.0 16.4#




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

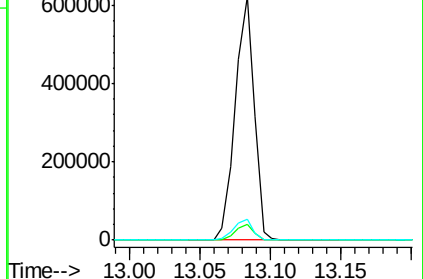



#86
Perylene-d12
Concen: 20.000 ng
RT: 15.71 min Scan# 2273
Delta R.T. -0.01 min
Lab File: BF107076.D
Acq: 3 Jul 2018 12:28

Instrument :
BNA_F
ClientSampleId :
PS-BASELINEWATER

Tgt Ion: 264 Resp: 152216

Ion	Ratio	Lower	Upper
264	100		
260	23.2	19.2	28.8
265	21.3	17.5	26.3

