

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070318\
 Data File : BF107100.D
 Acq On : 4 Jul 2018 00:22
 Operator : JU/SJ
 Sample : J3812-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DPC-81753-FB-07

Quant Time: Jul 04 01:12:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 29 14:38:29 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	56488	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	198710	20.00	ng	-0.01
38) Acenaphthene-d10	10.00	164	85158	20.00	ng	-0.01
63) Phenanthrene-d10	11.49	188	171138	20.00	ng	0.00
75) Chrysene-d12	14.15	240	138226	20.00	ng	-0.02
86) Perylene-d12	15.68	264	99252	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	209807	62.89	ng	0.00
7) Phenol-d6	6.60	99	253246	60.79	ng	-0.01
23) Nitrobenzene-d5	7.52	82	143368	40.10	ng	-0.02
41) 2,4,6-Tribromophenol	10.79	330	60469	61.27	ng	0.00
44) 2-Fluorobiphenyl	9.31	172	289738	51.83	ng	-0.02
78) Terphenyl-d14	13.07	244	357337	62.62	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.52	70	18342	6.679	ng	# 75
25) Isophorone	7.52	82	143364	22.753	ng	# 64
50) 2,6-Dinitrotoluene	10.00	165	11141	8.238	ng	# 24
56) 2,4-Dinitrotoluene	10.00	165	11141	6.311	ng	# 21
83) Bis(2-ethylhexyl)phthalate	14.09	149	13314	2.779	ng	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070318\
Data File : BF107100.D
Acq On : 4 Jul 2018 00:22
Operator : JU/SJ
Sample : J3812-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DPC-81753-FB-07

Quant Time: Jul 04 01:12:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

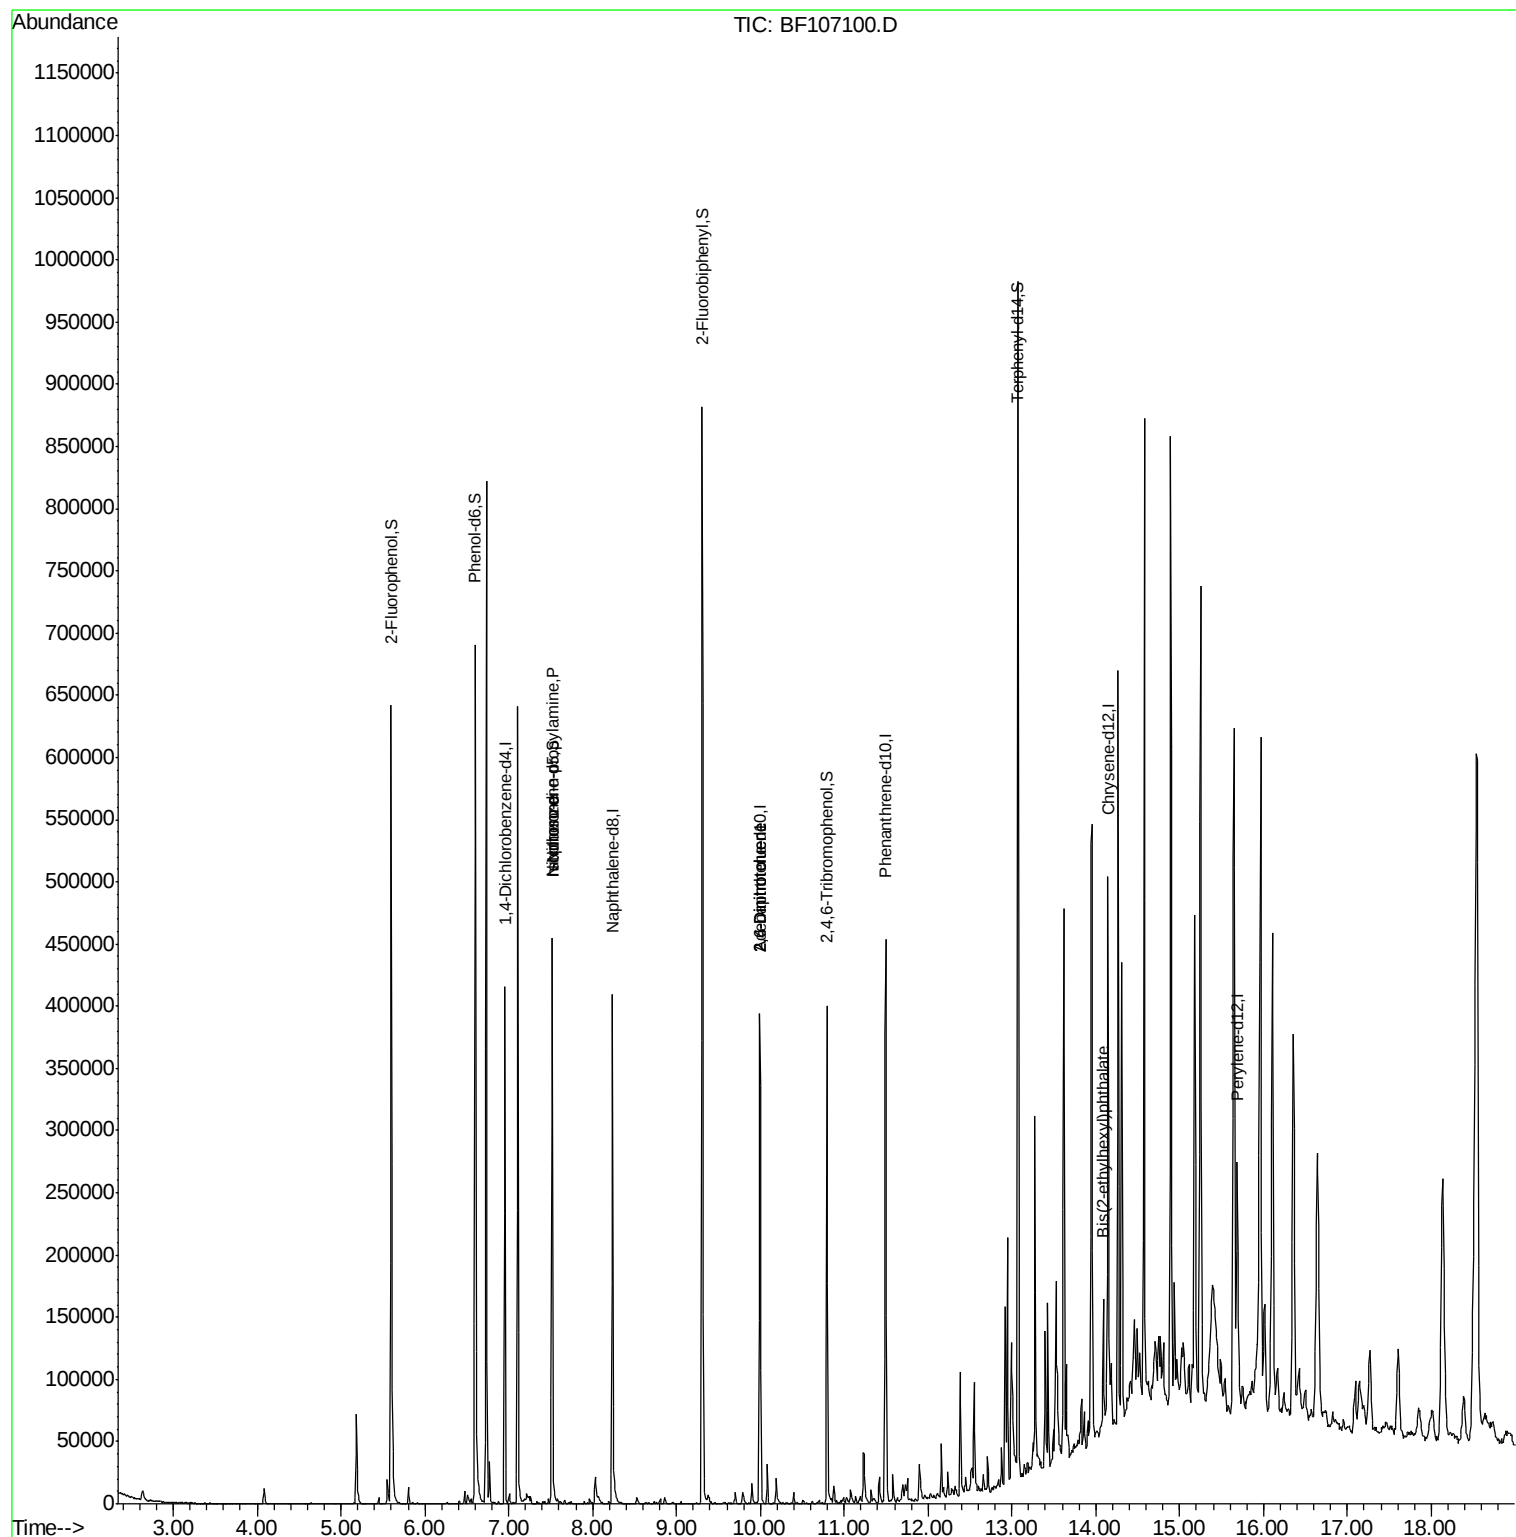




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF107100.D
Acq: 4 Jul 2018 00:22

Instrument :
BNA_F
ClientSampleId :
DPC-81753-FB-07

Tot Ion:152 Resp: 56488
Ion Ratio Lower Upper
152 100
150 156.7 124.6 186.8
115 58.8 50.1 75.1

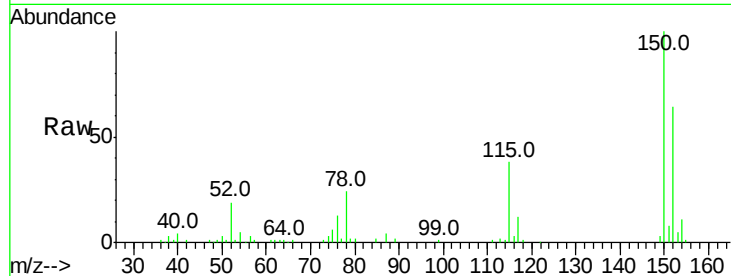


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

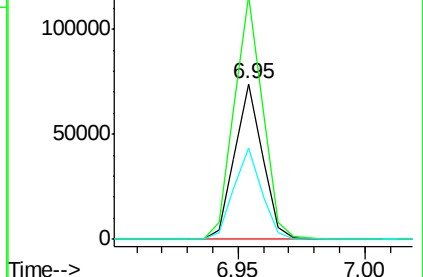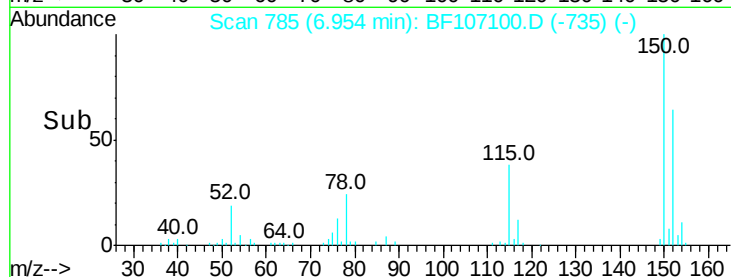



#5

2-Fluorophenol
Concen: 62.893 ng
RT: 5.60 min Scan# 555
Delta R.T. -0.00 min
Lab File: BF107100.D
Acq: 4 Jul 2018 00:22

Tgt Ion:112 Resp: 209807
Ion Ratio Lower Upper
112 100
64 56.6 47.9 71.9
63 27.1 23.7 35.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

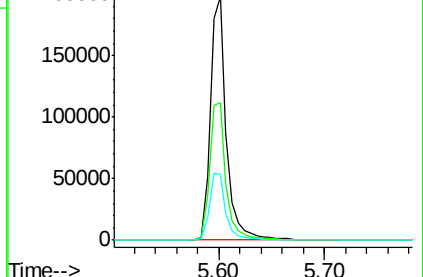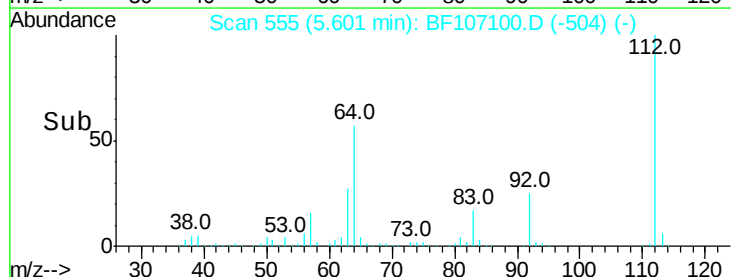



#7

Phenol-d6

Concen: 60.790 ng

RT: 6.60 min Scan# 725

Delta R.T. -0.01 min

Lab File: BF107100.D

Acq: 4 Jul 2018 00:22

Instrument :

BNA_F

ClientSampleId :

DPC-81753-FB-07


Tot Ion: 99 Resp: 253246

Ion Ratio Lower Upper

99 100

42 16.1 14.5 21.7




71 33.5 25.4 38.0

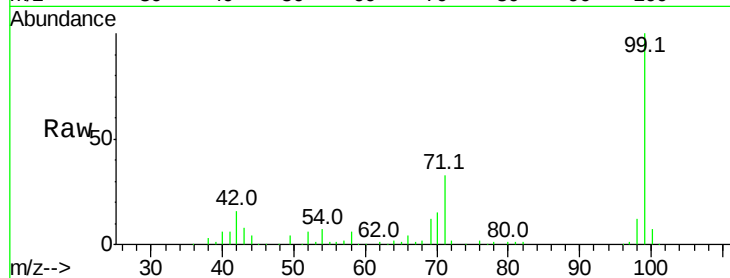

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

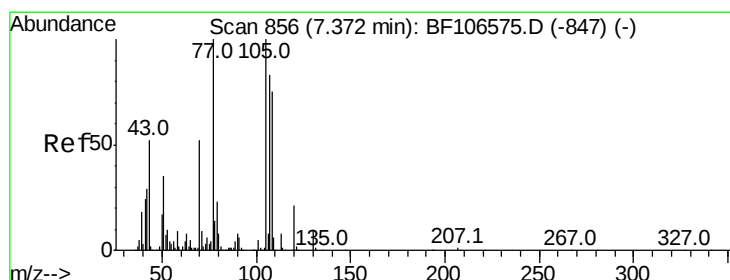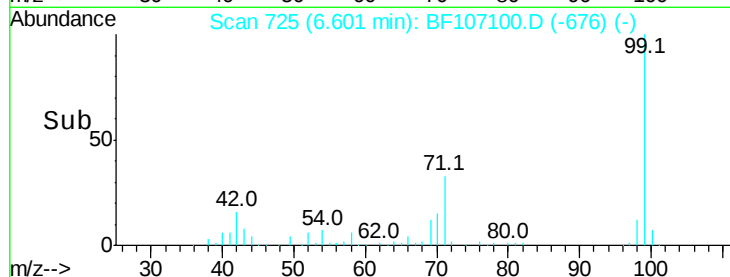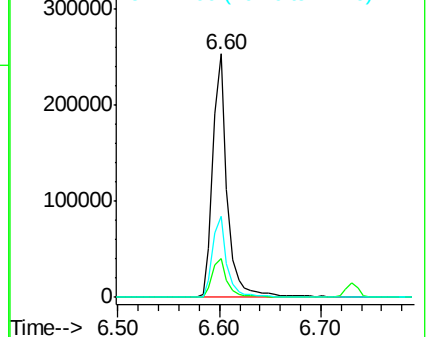

#19

n-Nitroso-di-n-propylamine

Concen: 6.679 ng

RT: 7.52 min Scan# 881

Delta R.T. 0.14 min

Lab File: BF107100.D

Acq: 4 Jul 2018 00:22

Tgt Ion: 70 Resp: 18342


Ion Ratio Lower Upper

70 100

42 45.0 47.5 71.3#

101 0.0 7.4 11.2#

130 2.4 16.6 25.0#


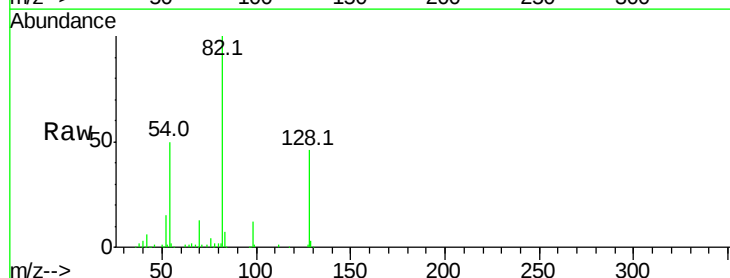


Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

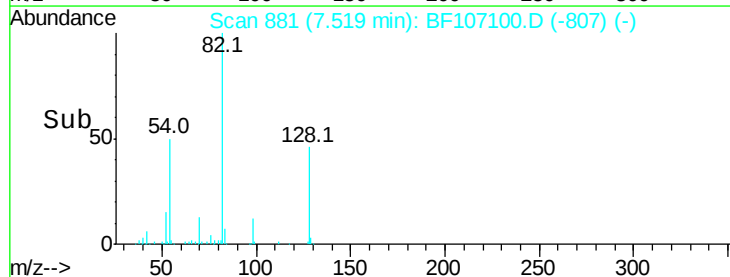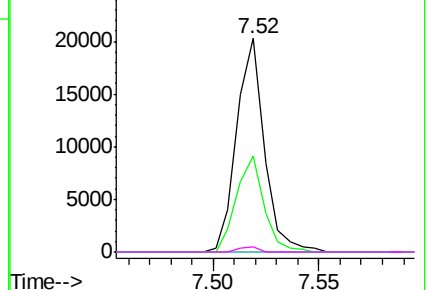



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.24 min Scan# 1003

Delta R.T. -0.01 min

Lab File: BF107100.D

Acq: 4 Jul 2018 00:22

Instrument :

BNA_F

ClientSampleId :

DPC-81753-FB-07

Tot Ion:136 Resp: 198710


Ion Ratio Lower Upper

136 100

137 10.8 8.9 13.3

54 8.1 6.6 9.8

68 6.0 5.0 7.4






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

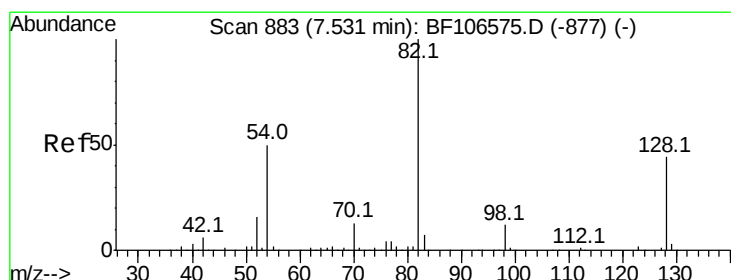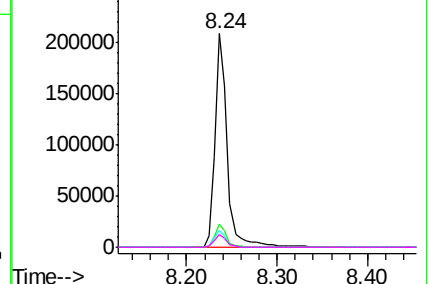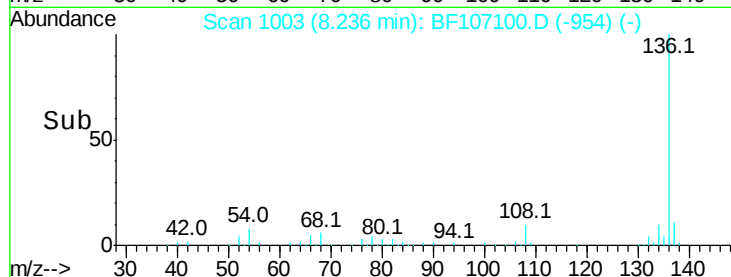

#23

Nitrobenzene-d5

Concen: 40.096 ng

RT: 7.52 min Scan# 881

Delta R.T. -0.02 min

Lab File: BF107100.D

Acq: 4 Jul 2018 00:22


Tgt Ion: 82 Resp: 143368

Ion Ratio Lower Upper

82 100

128 45.8 36.1 54.1



54 49.8 41.4 62.2




Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

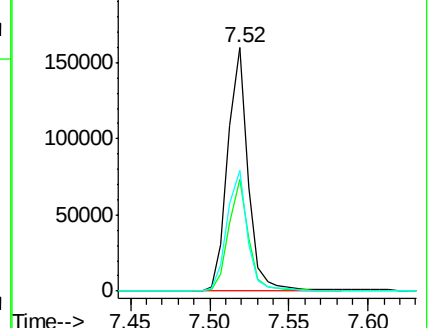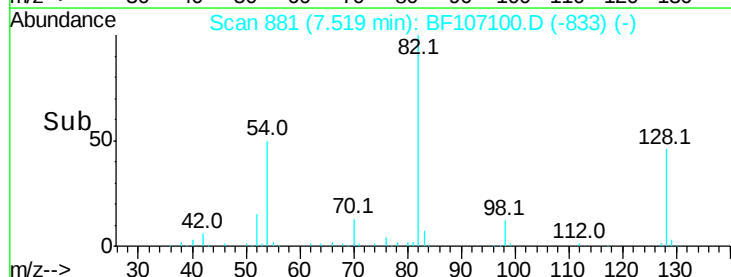

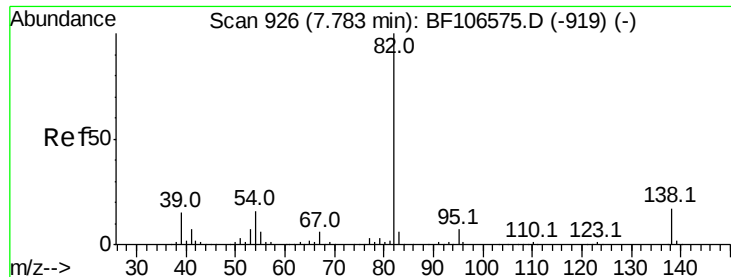

#25

Isophorone

Concen: 22.753 ng

RT: 7.52 min Scan# 881

Delta R.T. -0.27 min

Lab File: BF107100.D

Acq: 4 Jul 2018 00:22

Instrument :

BNA_F

ClientSampleId :

DPC-81753-FB-07


Tot Ion: 82 Resp: 143364

Ion Ratio Lower Upper

82 100

95 0.0 5.2 7.8#




138 0.0 14.9 22.3#

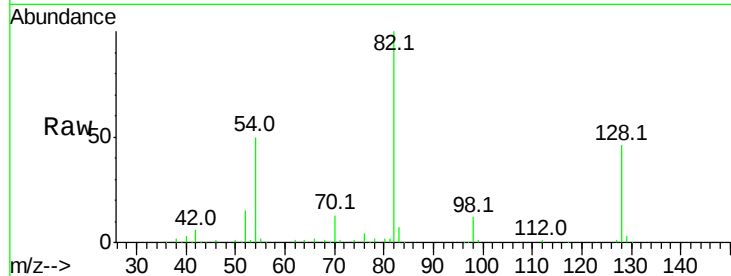

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

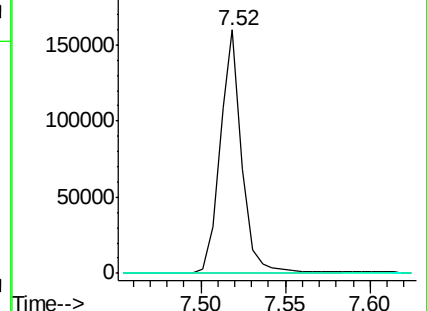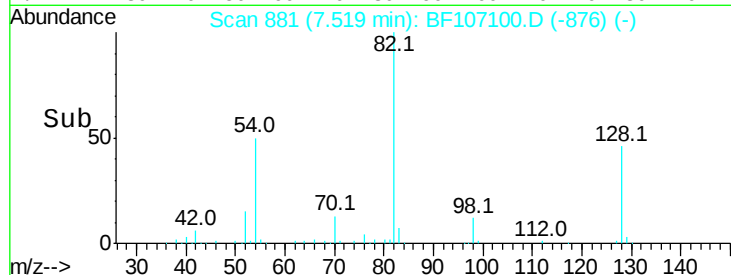

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 10.00 min Scan# 1302

Delta R.T. -0.01 min

Lab File: BF107100.D

Acq: 4 Jul 2018 00:22


Tgt Ion:164 Resp: 85158

Ion Ratio Lower Upper

164 100

162 97.0 86.1 129.1



160 41.7 38.3 57.5



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

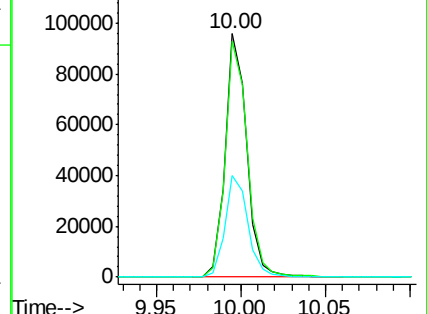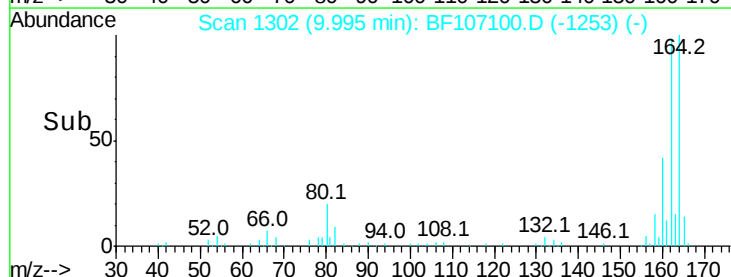







#41
 2,4,6-Tribromophenol
 Concen: 61.265 ng
 RT: 10.79 min Scan# 1438
 Delta R.T. -0.01 min
 Lab File: BF107100.D
 Acq: 4 Jul 2018 00:22

Instrument :
 BNA_F
 ClientSampleId :
 DPC-81753-FB-07

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.7	77.0	115.6
141	24.5	29.9	44.9#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

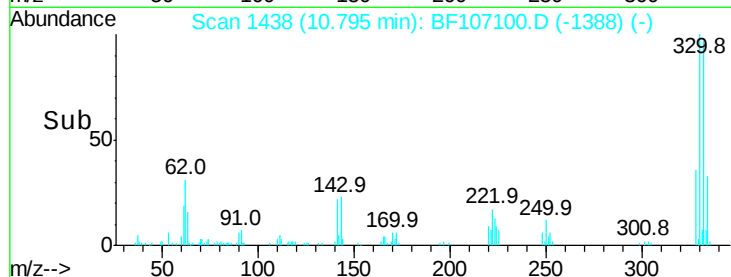
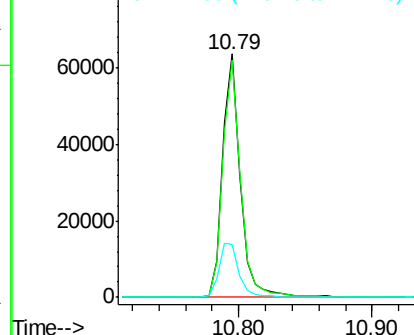



#44
 2-Fluorobiphenyl
 Concen: 51.833 ng
 RT: 9.31 min Scan# 1185
 Delta R.T. -0.02 min
 Lab File: BF107100.D
 Acq: 4 Jul 2018 00:22

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.0	29.7	44.5
170	23.6	19.6	29.4



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



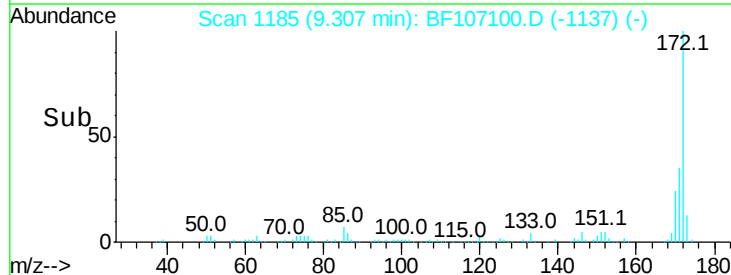
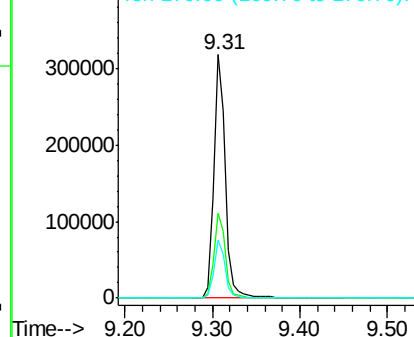


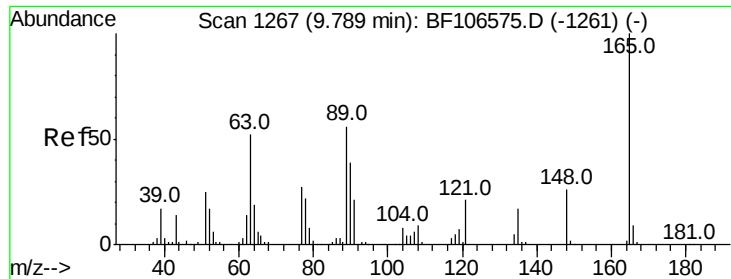

#50
 2,6-Dinitrotoluene
 Concen: 8.238 ng
 RT: 10.00 min Scan# 1302
 Delta R.T. 0.20 min
 Lab File: BF107100.D
 Acq: 4 Jul 2018 00:22




Instrument :
 BNA_F
 ClientSampleId :
 DPC-81753-FB-07

Tot Ion:165 Resp: 11141
 Ion Ratio Lower Upper
 165 100
 63 0.0 44.7 67.1#
 89 0.0 44.0 66.0#

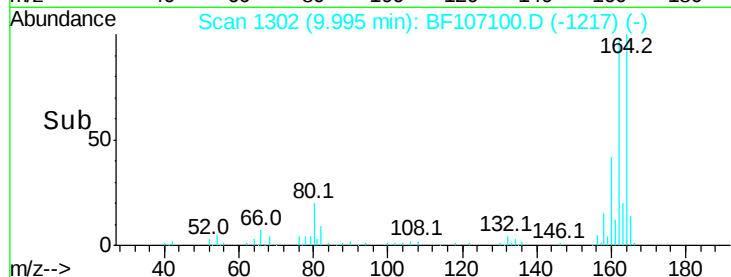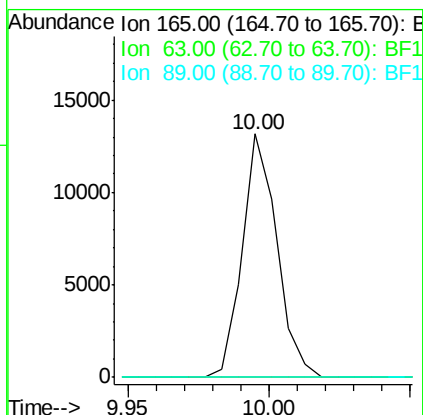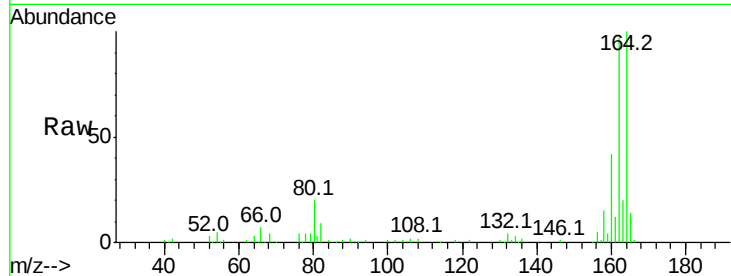

#56
 2,4-Dinitrotoluene
 Concen: 6.311 ng
 RT: 10.00 min Scan# 1302
 Delta R.T. -0.21 min
 Lab File: BF107100.D
 Acq: 4 Jul 2018 00:22

Tgt Ion:165 Resp: 11141
 Ion Ratio Lower Upper
 165 100
 63 0.0 36.4 54.6#
 89 0.0 57.8 86.6#
 182 0.0 1.6 2.4#

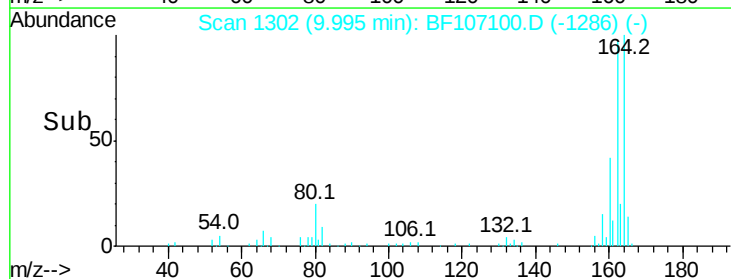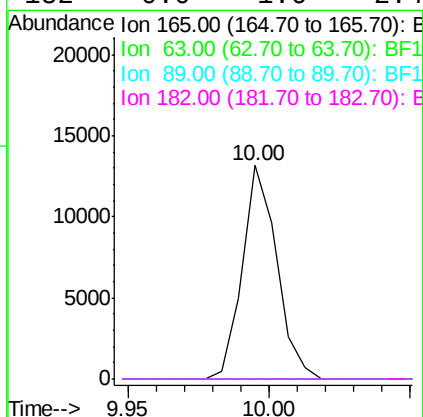



#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.49 min Scan# 1557

Delta R.T. -0.01 min

Lab File: BF107100.D

Acq: 4 Jul 2018 00:22

Instrument :

BNA_F

ClientSampleId :

DPC-81753-FB-07


Tot Ion:188 Resp: 171138

Ion Ratio Lower Upper

188 100

94 8.0 8.5 12.7#




80 9.0 9.2 13.8#

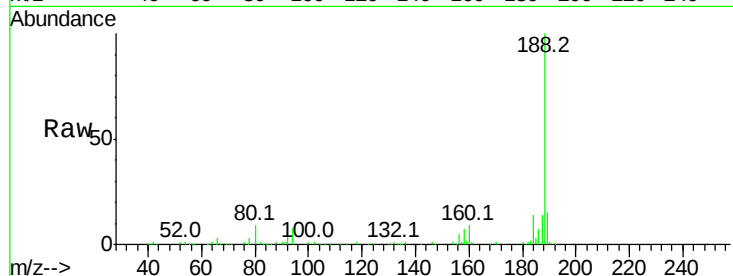

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

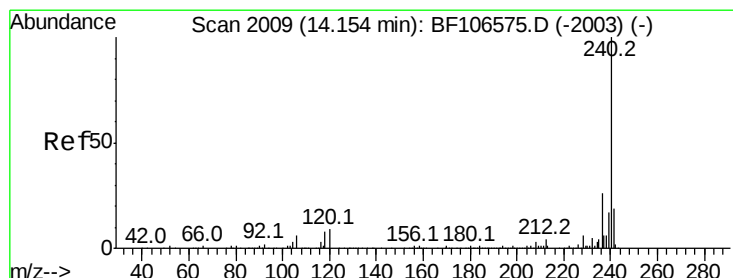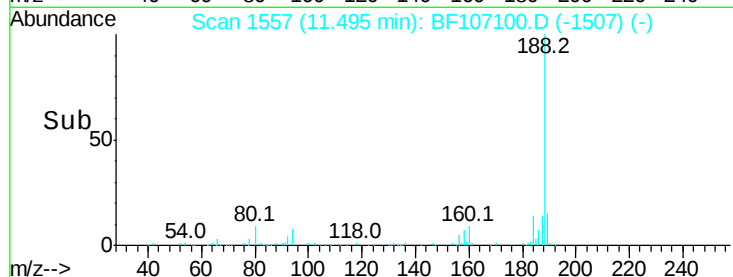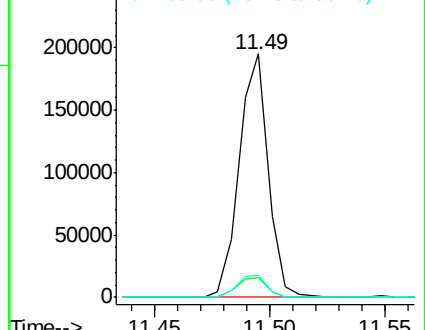

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.15 min Scan# 2008

Delta R.T. -0.02 min

Lab File: BF107100.D

Acq: 4 Jul 2018 00:22


Tgt Ion:240 Resp: 138226

Ion Ratio Lower Upper

240 100

120 8.2 9.5 14.3#



236 25.4 20.7 31.1

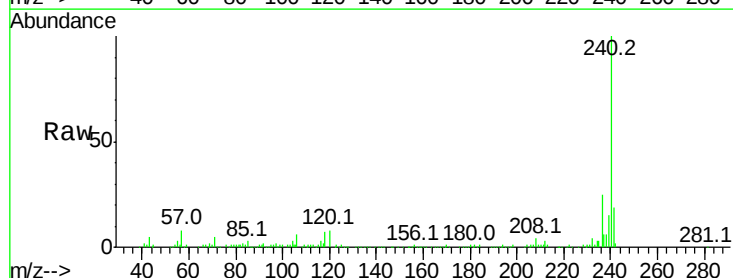


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



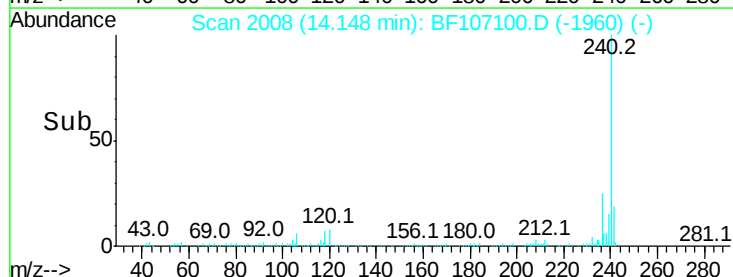
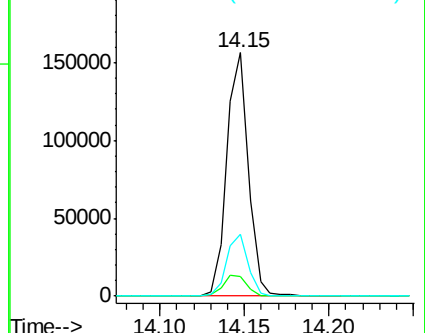


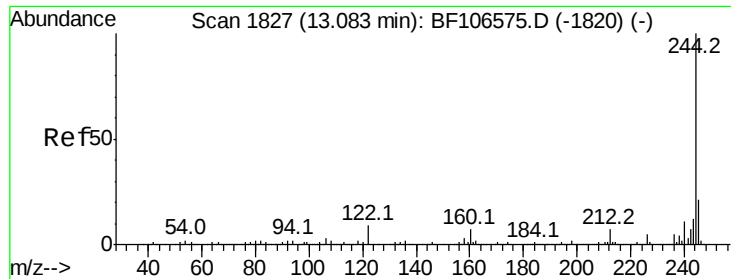

#78
 Terphenyl-d14
 Concen: 62.620 ng
 RT: 13.07 min Scan# 1825
 Delta R.T. -0.01 min
 Lab File: BF107100.D
 Acq: 4 Jul 2018 00:22




Instrument :
 BNA_F
 ClientSampleId :
 DPC-81753-FB-07


Tot Ion:244 Resp: 357337
 Ion Ratio Lower Upper
 244 100
 212 6.6 5.4 8.0
 122 9.4 11.0 16.4#

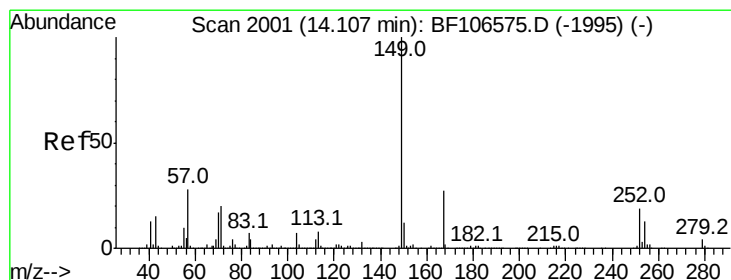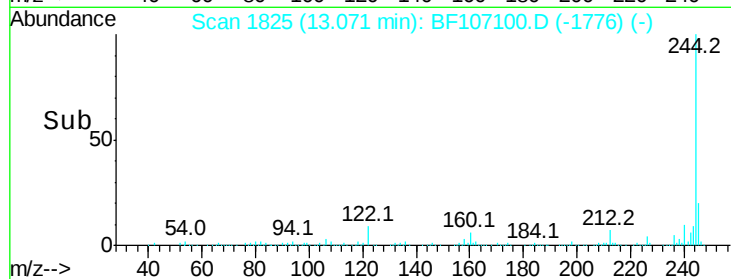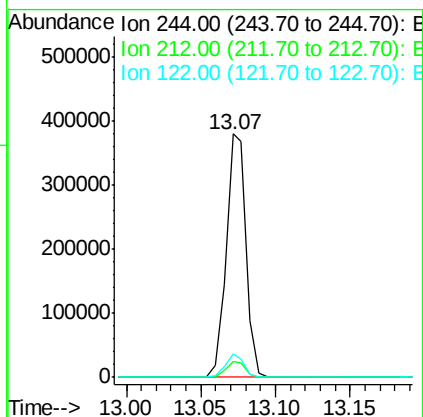

#83
 Bis(2-ethylhexyl)phthalate
 Concen: 2.779 ng
 RT: 14.09 min Scan# 1998
 Delta R.T. -0.02 min
 Lab File: BF107100.D
 Acq: 4 Jul 2018 00:22

Tgt Ion:149 Resp: 13314
 Ion Ratio Lower Upper
 149 100
 167 29.8 21.3 31.9
 279 4.4 3.0 4.4

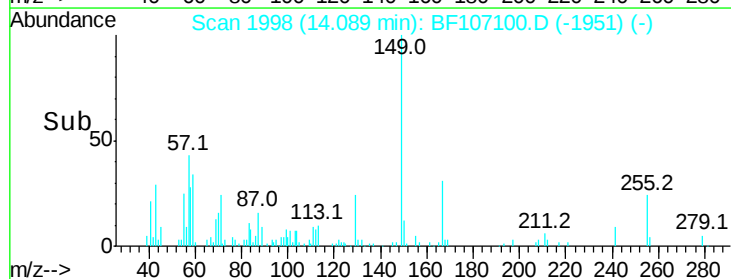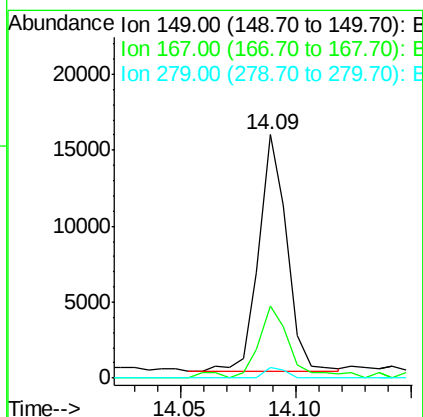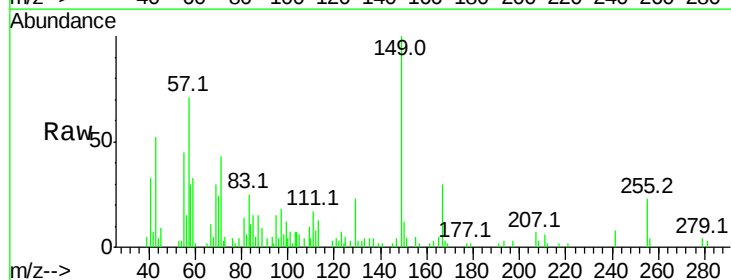

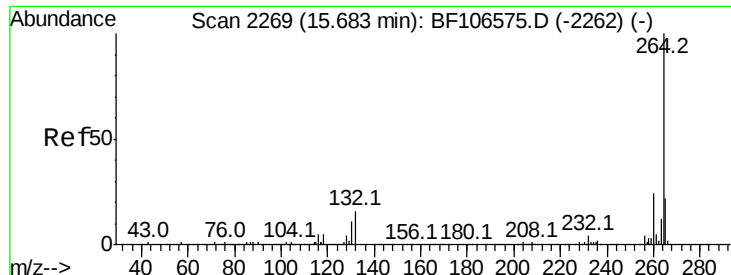

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.68 min Scan# 2269
 Delta R.T. -0.04 min
 Lab File: BF107100.D
 Acq: 4 Jul 2018 00:22

Instrument :
 BNA_F
 ClientSampleId :
 DPC-81753-FB-07

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.2	28.8
265	20.8	17.5	26.3

