
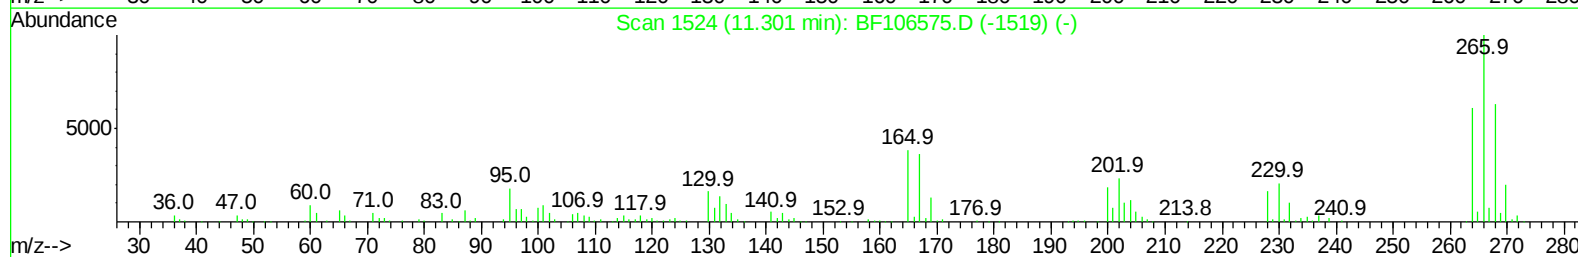
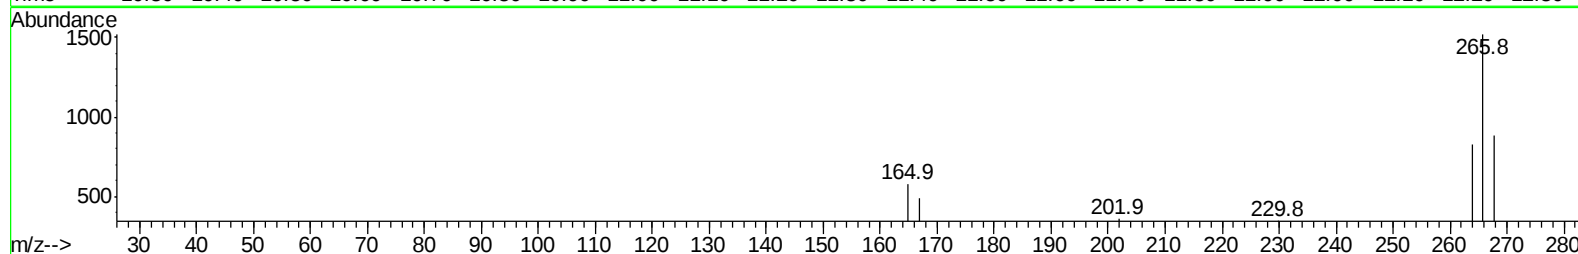


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070318\
Data File : BF107096.D
Acq On : 3 Jul 2018 22:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 04 03:57:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

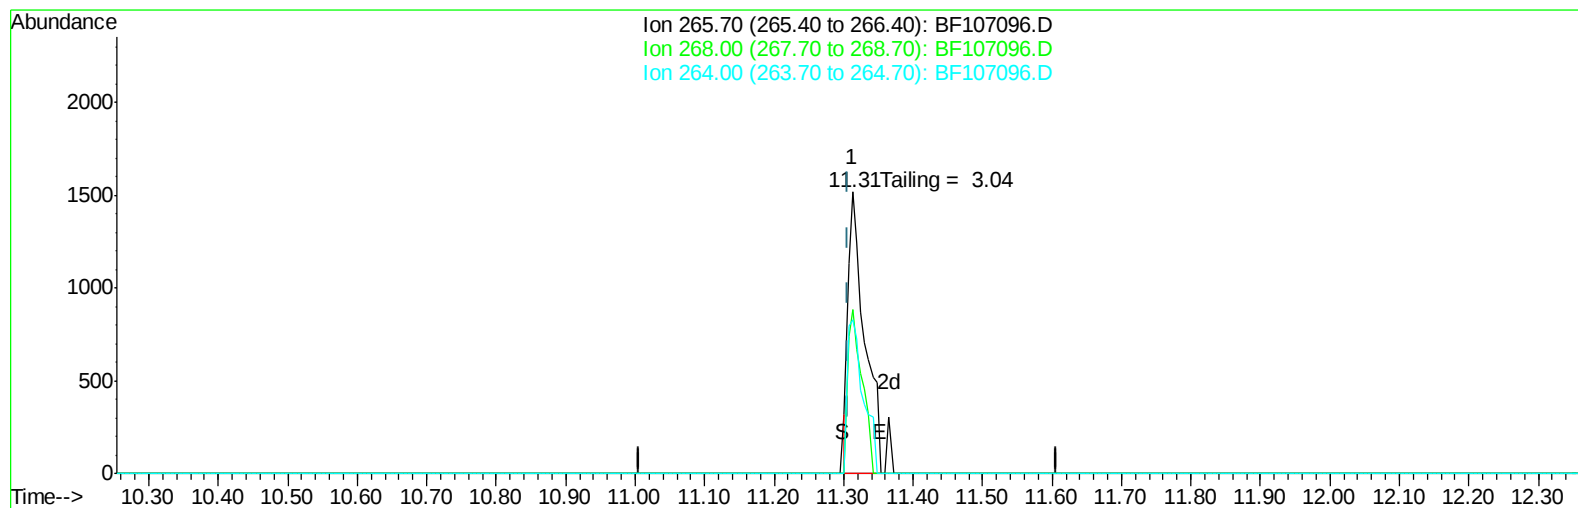

TIC: BF107096.D

(69) Pentachlorophenol (C)

11.313min (+0.006) 0.00ng

response 2613

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	58.10
264.00	61.90	54.41
0.00	0.00	0.00

