

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070318\
 Data File : BF107108.D
 Acq On : 4 Jul 2018 3:57
 Operator : JU/SJ
 Sample : J3816-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 161-TAN-BRICK

Quant Time: Jul 04 04:35:47 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 29 14:38:29 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.95	152	53398	20.00	ng	0.00
21) Naphthalene-d8	8.24	136	184943	20.00	ng	-0.01
38) Acenaphthene-d10	10.00	164	81863	20.00	ng	-0.01
63) Phenanthrene-d10	11.50	188	171678	20.00	ng	0.00
75) Chrysene-d12	14.15	240	138053	20.00	ng	-0.02
86) Perylene-d12	15.69	264	97188	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	311228	98.69	ng	0.00
7) Phenol-d6	6.61	99	371641	94.37	ng	0.00
23) Nitrobenzene-d5	7.52	82	218423	65.63	ng	-0.02
41) 2,4,6-Tribromophenol	10.80	330	106622	112.37	ng	0.00
44) 2-Fluorobiphenyl	9.31	172	409544	84.61	ng	-0.02
78) Terphenyl-d14	13.08	244	525473	92.20	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.70	163	47682	7.766	ng	98
73) Di-n-butylphthalate	12.04	149	23353	2.505	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070318\
Data File : BF107108.D
Acq On : 4 Jul 2018 3:57
Operator : JU/SJ
Sample : J3816-06
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
161-TAN-BRICK

Quant Time: Jul 04 04:35:47 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

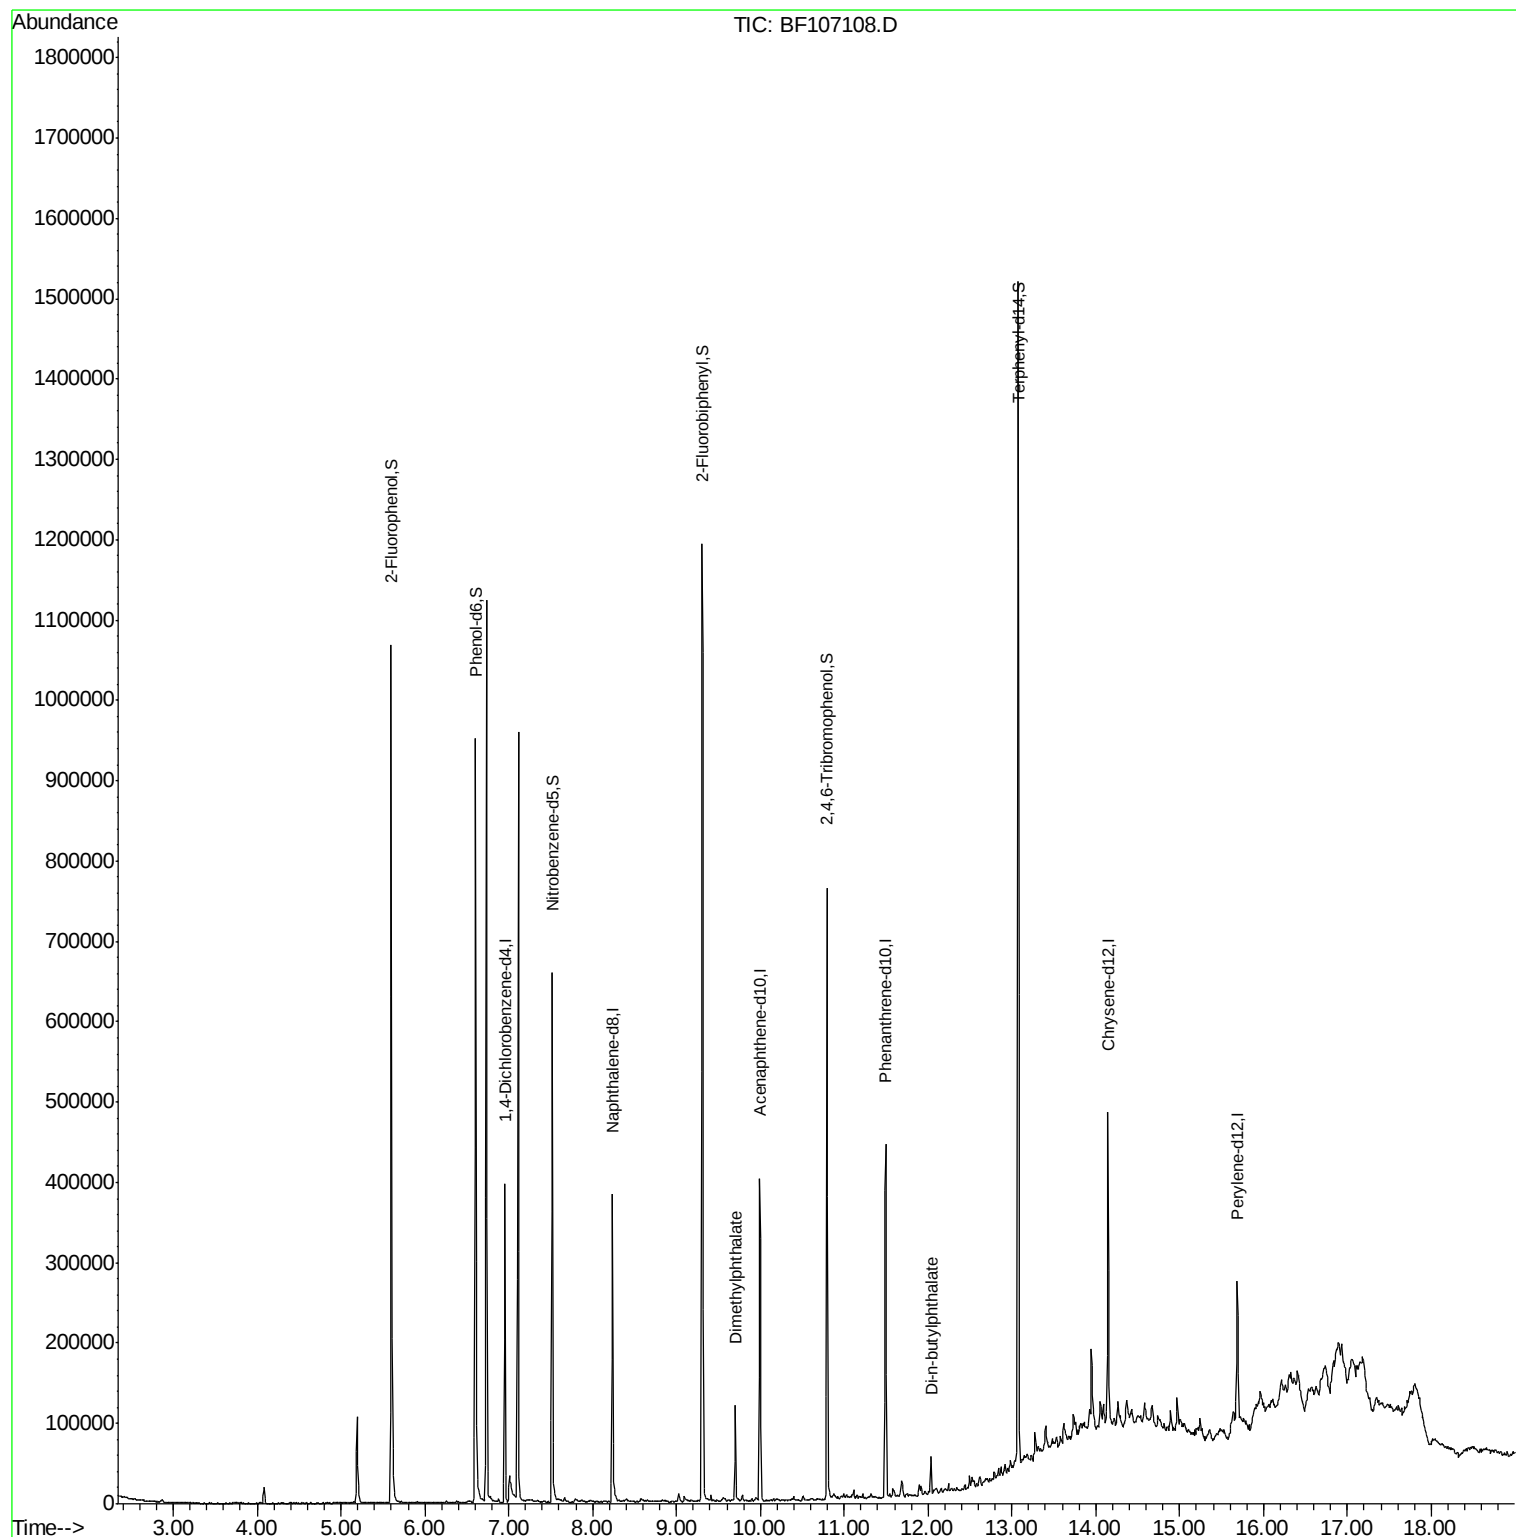

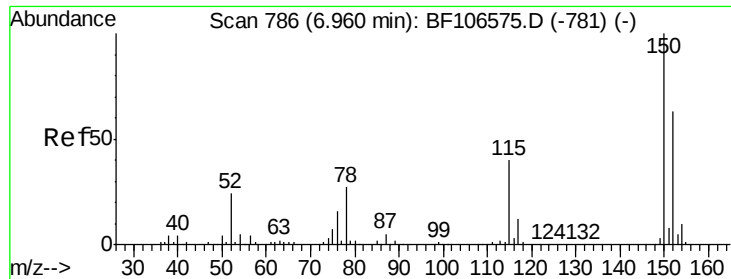


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.95 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF107108.D
Acq: 4 Jul 2018 3:57

Instrument :
BNA_F
ClientSampleId :
161-TAN-BRICK

Tot Ion	Ratio	Lower	Upper
152	100		
150	155.4	124.6	186.8
115	59.9	50.1	75.1

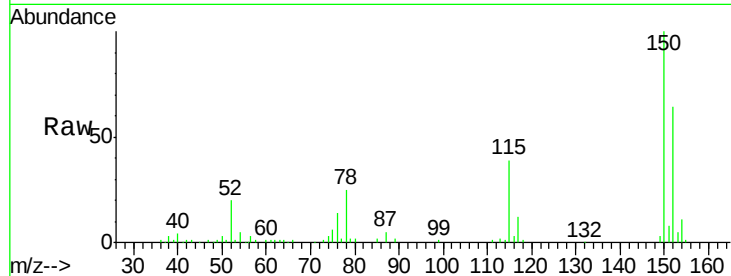


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

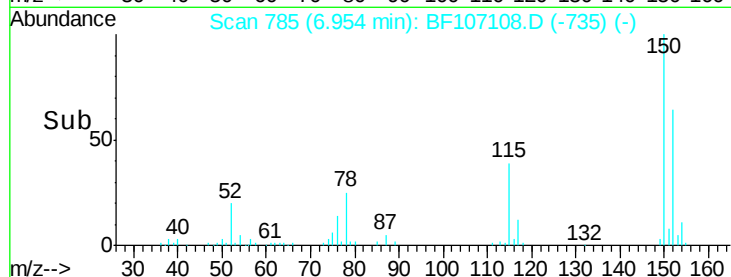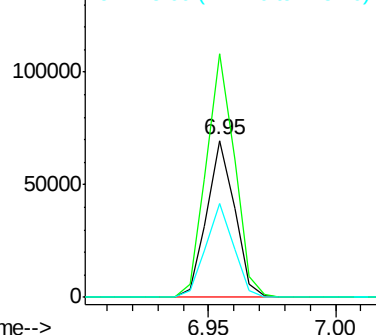



#5

2-Fluorophenol
Concen: 98.694 ng
RT: 5.60 min Scan# 555
Delta R.T. 0.00 min
Lab File: BF107108.D
Acq: 4 Jul 2018 3:57

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.3	47.9	71.9
63	29.2	23.7	35.5

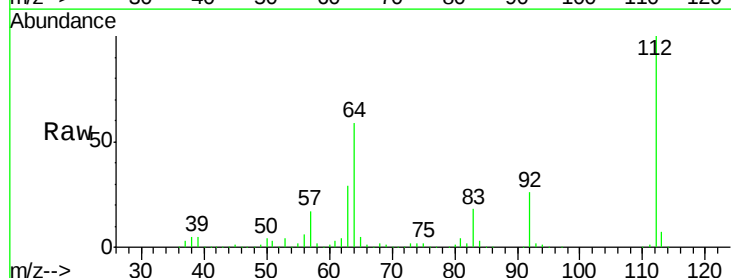

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

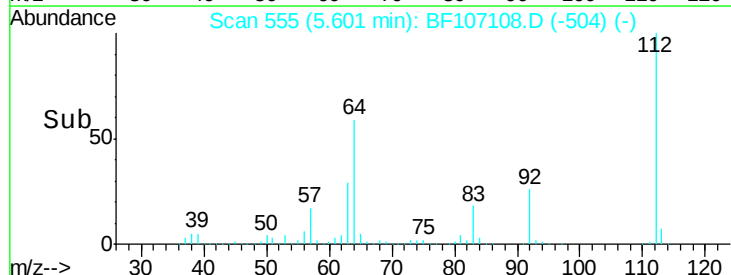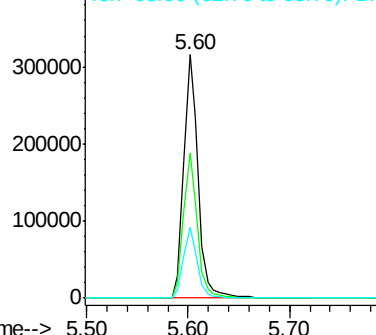



#7

Phenol-d6

Concen: 94.372 ng

RT: 6.61 min Scan# 726

Delta R.T. -0.01 min

Lab File: BF107108.D

Acq: 4 Jul 2018 3:57

Instrument :

BNA_F

ClientSampleId :

161-TAN-BRICK


Tot Ion: 99 Resp: 371641

Ion Ratio Lower Upper

99 100

42 15.5 14.5 21.7




71 32.8 25.4 38.0

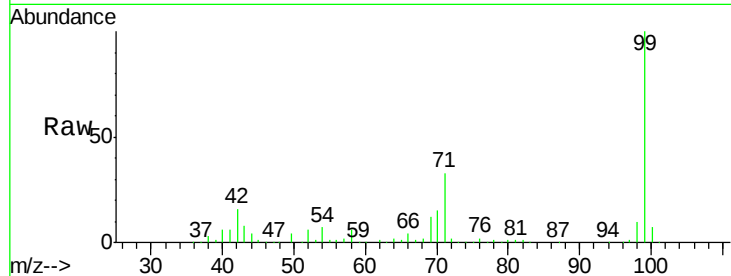

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

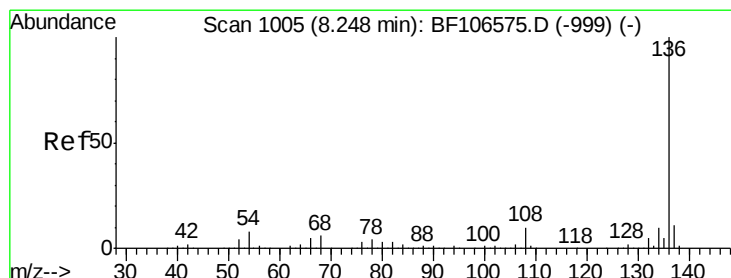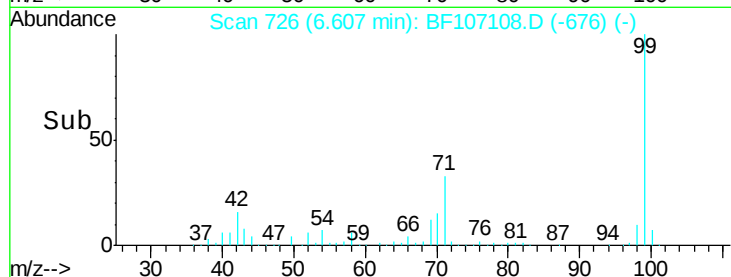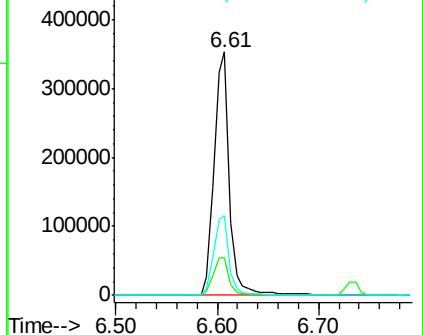

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.24 min Scan# 1003

Delta R.T. -0.01 min

Lab File: BF107108.D

Acq: 4 Jul 2018 3:57

Tgt Ion: 136 Resp: 184943


Ion Ratio Lower Upper

136 100

137 11.1 8.9 13.3

54 8.1 6.6 9.8

68 6.7 5.0 7.4


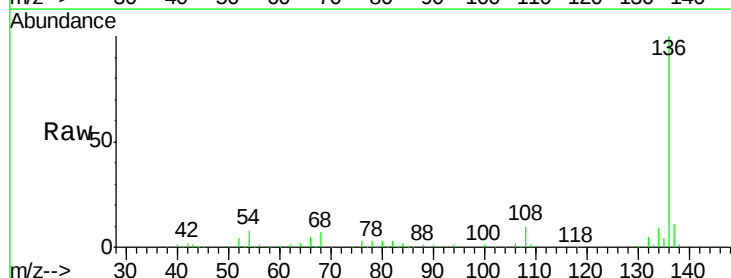



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

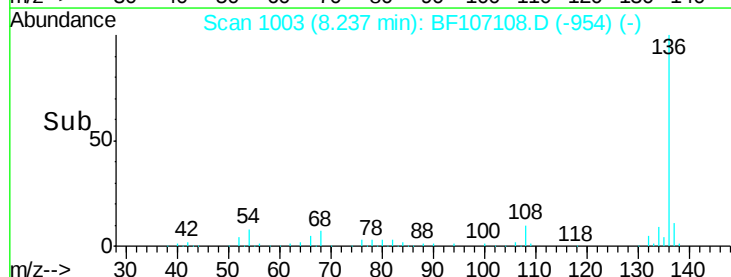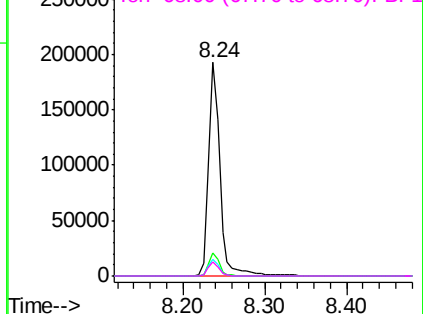


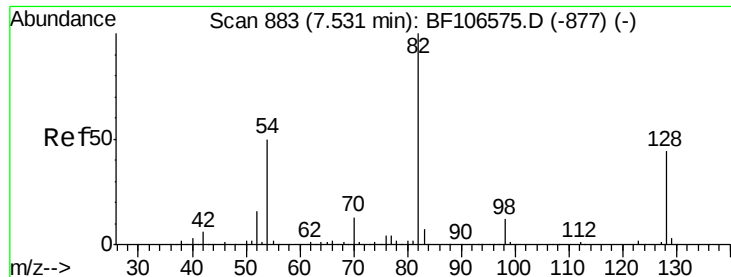




#23
Nitrobenzene-d5
Concen: 65.634 ng
RT: 7.52 min Scan# 881
Delta R.T. -0.02 min
Lab File: BF107108.D
Acq: 4 Jul 2018 3:57

Instrument :
BNA_F
ClientSampleId :
161-TAN-BRICK

Tot Ion: 82 Resp: 218423
Ion Ratio Lower Upper
82 100
128 43.5 36.1 54.1
54 49.6 41.4 62.2

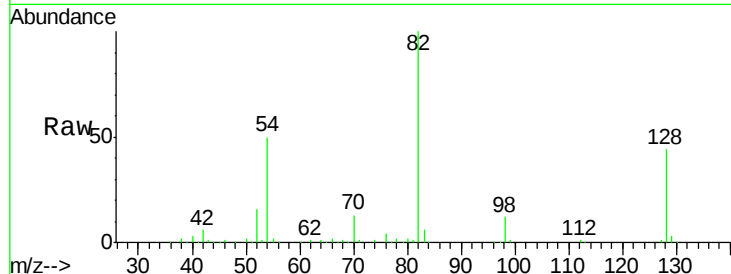


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

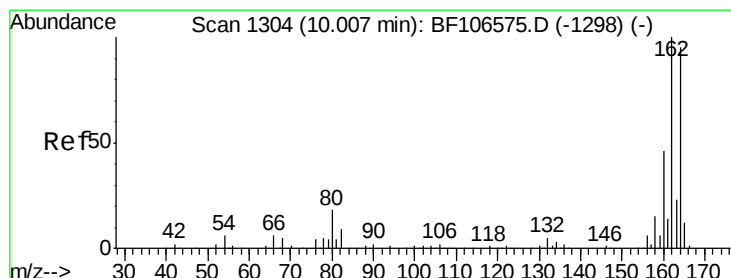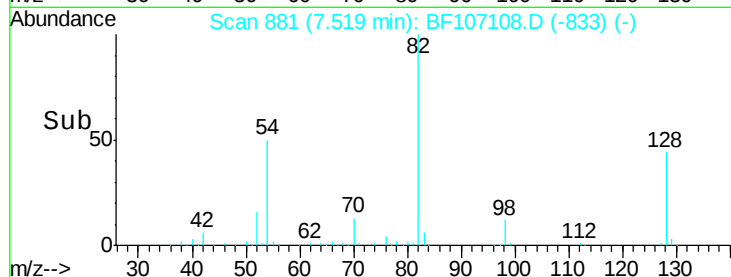
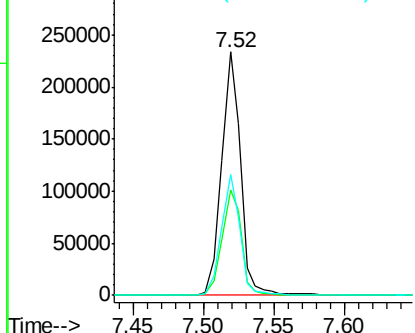



#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.00 min Scan# 1302
Delta R.T. -0.01 min
Lab File: BF107108.D
Acq: 4 Jul 2018 3:57

Tgt Ion: 164 Resp: 81863
Ion Ratio Lower Upper
164 100
162 98.9 86.1 129.1
160 44.6 38.3 57.5

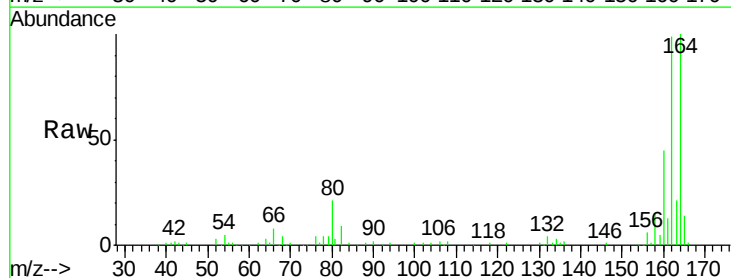

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1



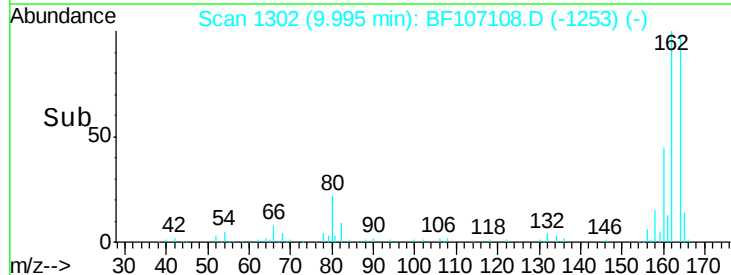
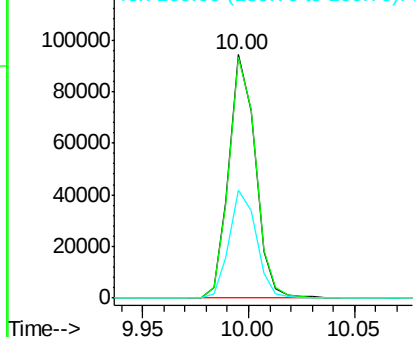


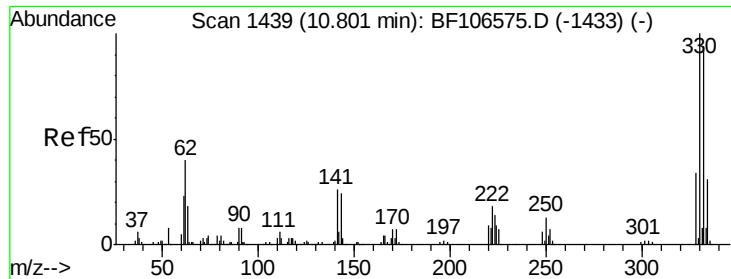

#41
 2,4,6-Tribromophenol
 Concen: 112.374 ng
 RT: 10.80 min Scan# 1438
 Delta R.T. -0.01 min
 Lab File: BF107108.D
 Acq: 4 Jul 2018 3:57




Instrument :
 BNA_F
 ClientSampleId :
 161-TAN-BRICK


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	77.0	115.6
141	23.0	29.9	44.9#

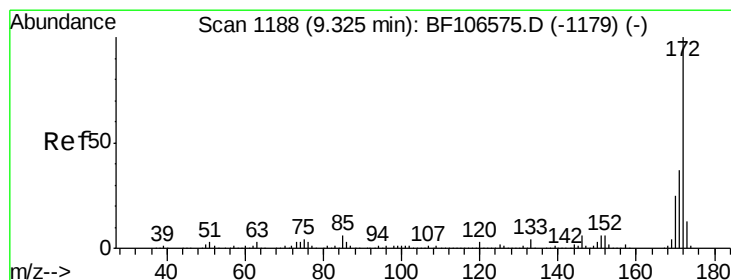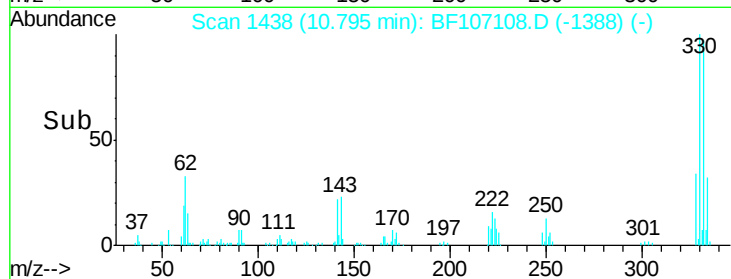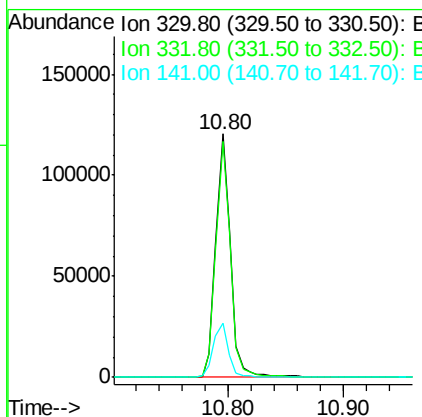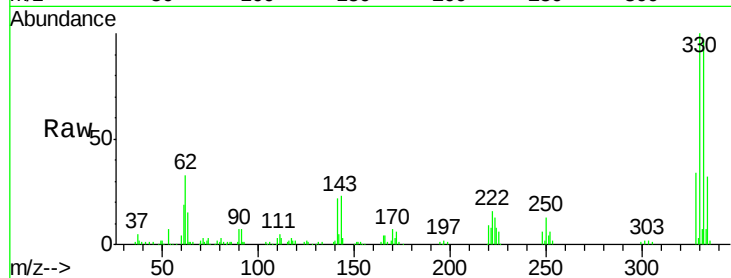

#44
 2-Fluorobiphenyl
 Concen: 84.611 ng
 RT: 9.31 min Scan# 1185
 Delta R.T. -0.02 min
 Lab File: BF107108.D
 Acq: 4 Jul 2018 3:57

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	29.7	44.5
170	24.3	19.6	29.4

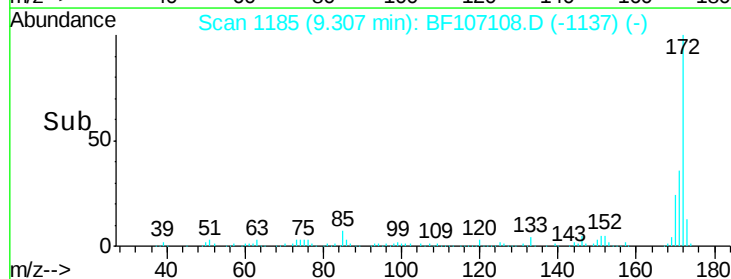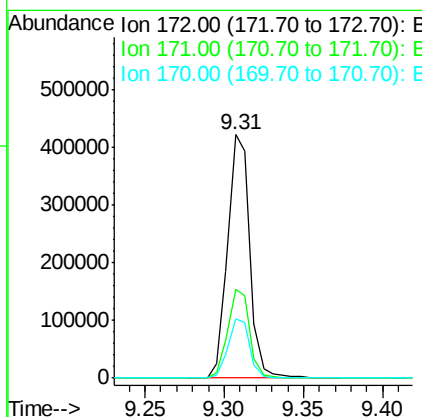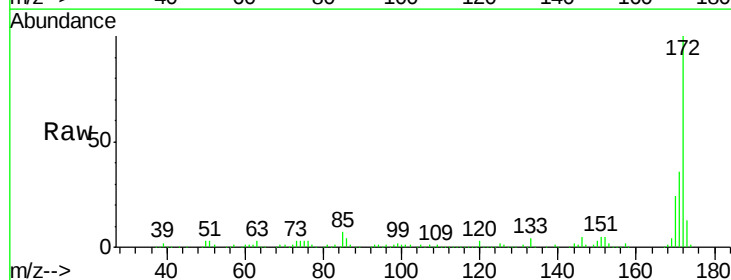


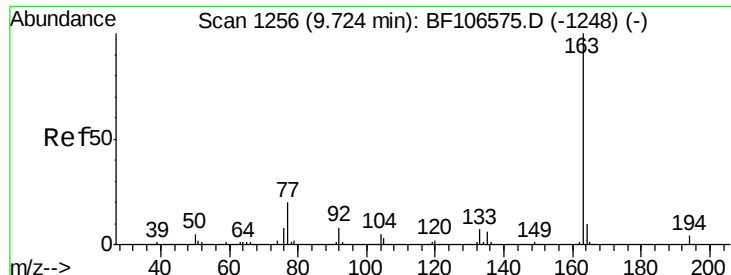




#49
Dimethylphthalate
Concen: 7.766 ng
RT: 9.70 min Scan# 1252
Delta R.T. -0.02 min
Lab File: BF107108.D
Acq: 4 Jul 2018 3:57

Instrument :
BNA_F
ClientSampleId :
161-TAN-BRICK

Tot Ion:163 Resp: 47682
Ion Ratio Lower Upper
163 100
194 3.7 2.7 4.1
164 10.9 8.2 12.2

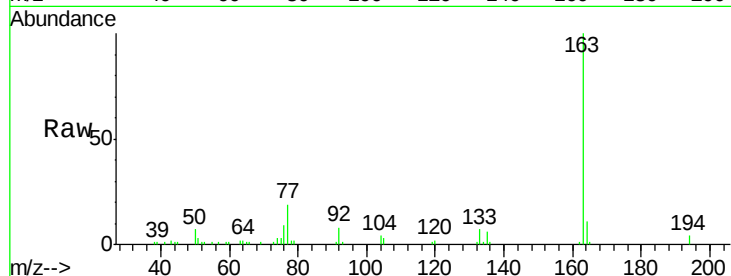


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

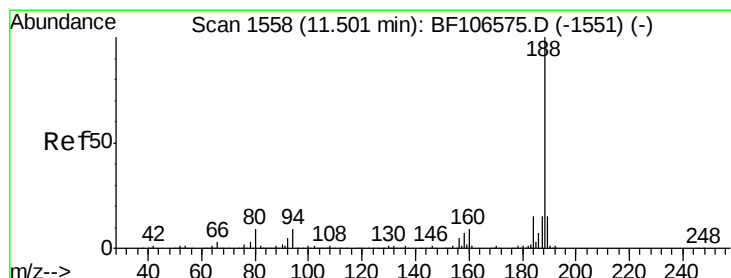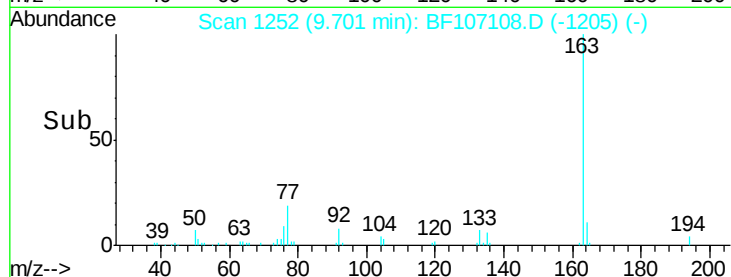
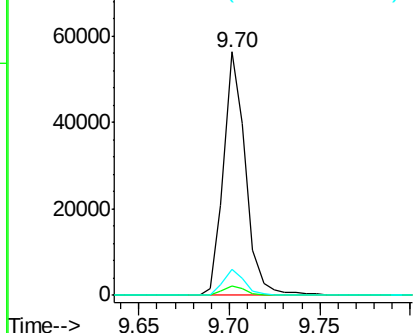



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.50 min Scan# 1557
Delta R.T. -0.01 min
Lab File: BF107108.D
Acq: 4 Jul 2018 3:57

Tgt Ion:188 Resp: 171678
Ion Ratio Lower Upper
188 100
94 8.5 8.5 12.7
80 8.6 9.2 13.8#

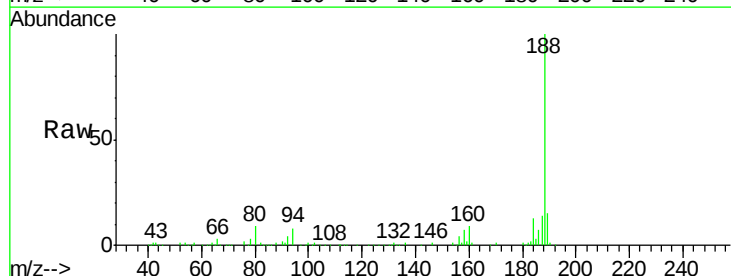

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1



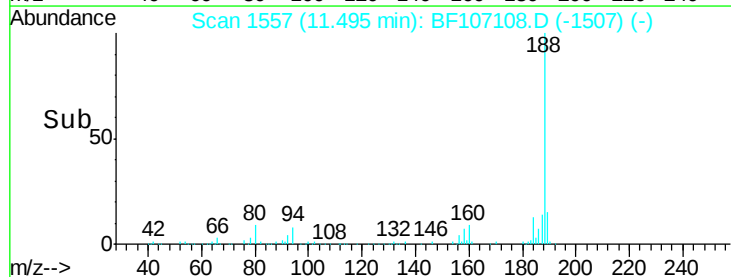
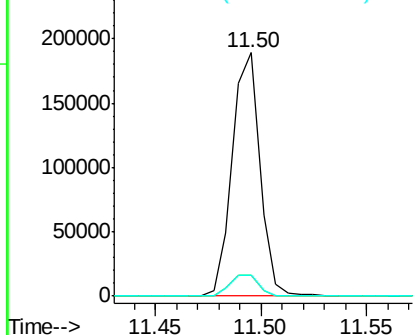


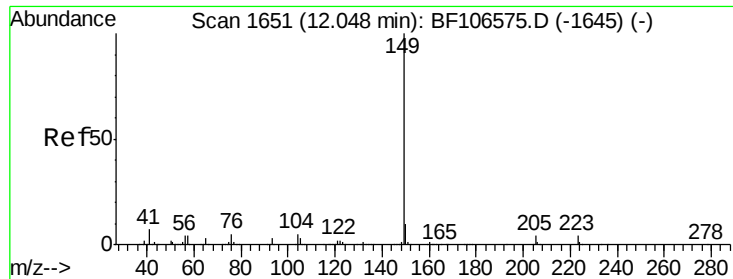

#73
Di-n-butylphthalate
Concen: 2.505 ng
RT: 12.04 min Scan# 1649
Delta R.T. -0.01 min
Lab File: BF107108.D
Acq: 4 Jul 2018 3:57




Instrument :
BNA_F
ClientSampleId :
161-TAN-BRICK


Tot Ion:149 Resp: 23353
Ion Ratio Lower Upper
149 100
150 9.1 7.8 11.6
104 5.0 3.8 5.8

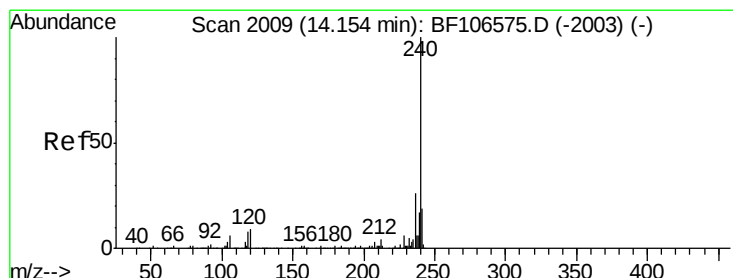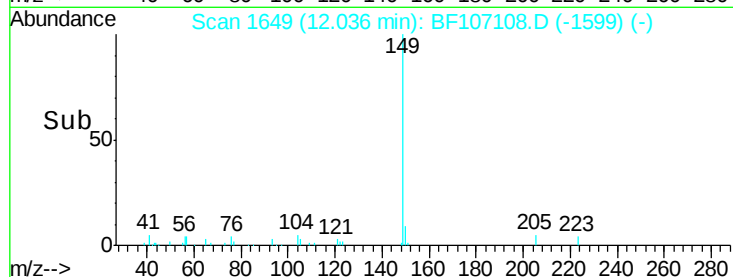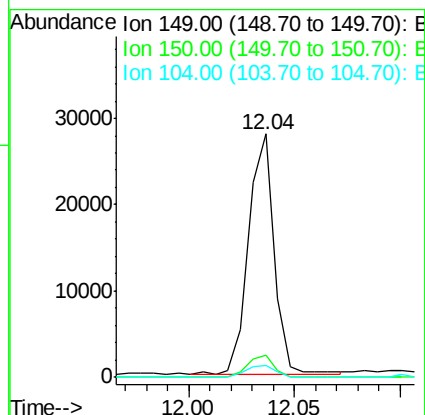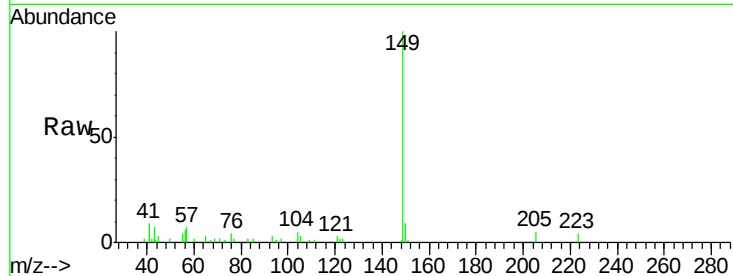

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.15 min Scan# 2008
Delta R.T. -0.02 min
Lab File: BF107108.D
Acq: 4 Jul 2018 3:57

Tgt Ion:240 Resp: 138053
Ion Ratio Lower Upper
240 100
120 8.9 9.5 14.3#
236 25.2 20.7 31.1


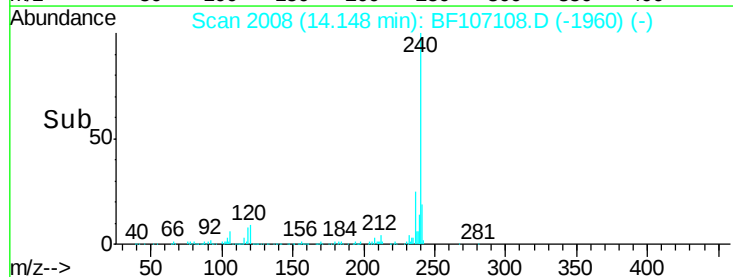
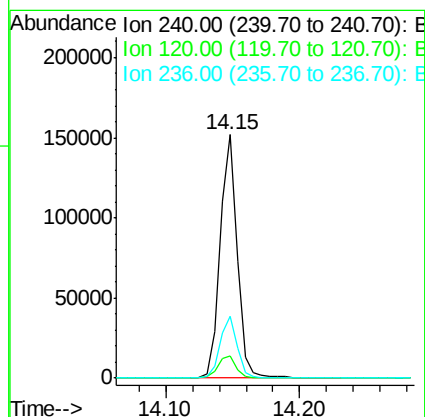
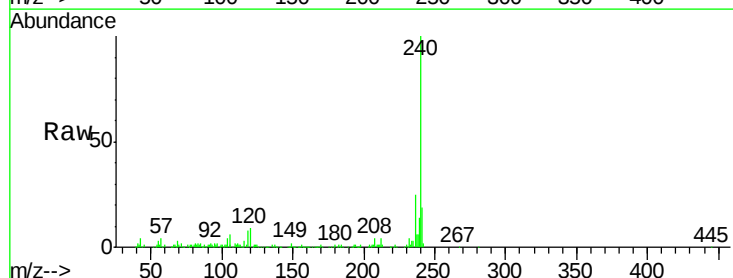


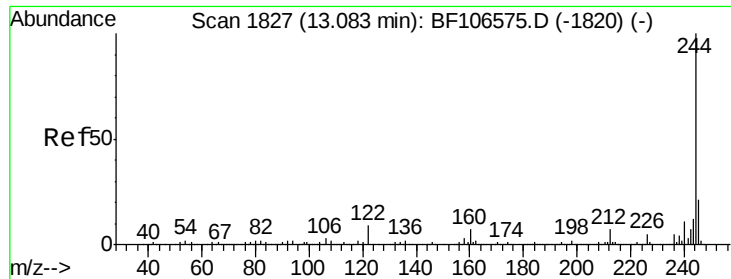

#78
 Terphenyl-d14
 Concen: 92.200 ng
 RT: 13.08 min Scan# 1826
 Delta R.T. -0.01 min
 Lab File: BF107108.D
 Acq: 4 Jul 2018 3:57

Instrument :
 BNA_F
 ClientSampleId :
 161-TAN-BRICK

Tot Ion:244 Resp: 525473
 Ion Ratio Lower Upper
 244 100
 212 6.5 5.4 8.0
 122 8.7 11.0 16.4#

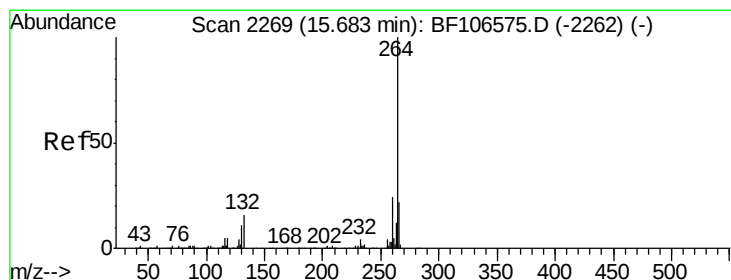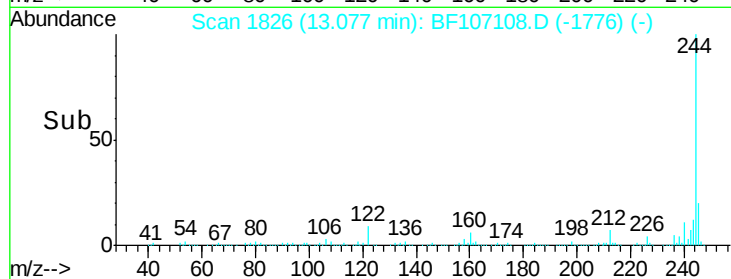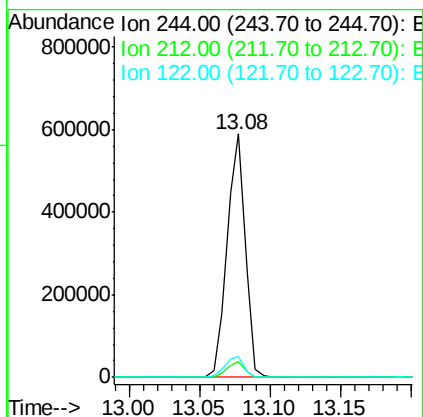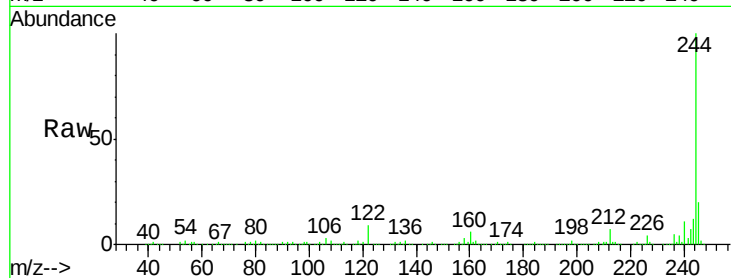

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.69 min Scan# 2270
 Delta R.T. -0.03 min
 Lab File: BF107108.D
 Acq: 4 Jul 2018 3:57

Tgt Ion:264 Resp: 97188
 Ion Ratio Lower Upper
 264 100
 260 23.2 19.2 28.8
 265 21.8 17.5 26.3

