

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070318\
 Data File : BF107079.D
 Acq On : 3 Jul 2018 13:51
 Operator : JU/SJ
 Sample : J3629-13
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 A0C14-01

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.178	480	483	493	rBB	14830	16727	3.54%	0.410%
2	5.601	551	555	569	rBV	177541	209026	44.19%	5.121%
3	6.601	722	725	740	rBV	158149	212488	44.92%	5.205%
4	6.731	744	747	759	rVB	233273	229684	48.56%	5.627%
5	6.954	782	785	789	rBV	385413	312739	66.12%	7.661%
6	7.107	808	811	824	rVB	197202	188005	39.75%	4.606%
7	7.519	878	881	891	rBV	120461	124891	26.40%	3.060%
8	8.242	1000	1004	1020	rBV	369546	384185	81.22%	9.412%
9	9.313	1182	1186	1195	rBV	224250	243543	51.49%	5.966%
10	9.707	1249	1253	1259	rVB	18654	20267	4.28%	0.496%
11	10.001	1299	1303	1314	rVB	374664	375552	79.40%	9.200%
12	10.795	1435	1438	1445	rBV	121219	114609	24.23%	2.808%
13	11.495	1553	1557	1560	rBV	440580	380132	80.37%	9.312%
14	11.966	1633	1637	1639	rBV5	3984	6841	1.45%	0.168%
15	12.083	1653	1657	1658	rBV3	6038	7799	1.65%	0.191%
16	12.495	1725	1727	1730	rBV3	9045	9932	2.10%	0.243%
17	12.713	1761	1764	1769	rVB	55822	54993	11.63%	1.347%
18	12.848	1785	1787	1788	rBV	10304	6835	1.45%	0.167%
19	12.871	1788	1791	1795	rVV	52384	47015	9.94%	1.152%
20	12.924	1797	1800	1801	rBV2	17247	17391	3.68%	0.426%
21	12.948	1801	1804	1808	rVB	63104	59805	12.64%	1.465%
22	13.071	1822	1825	1833	rVB	312267	309287	65.39%	7.577%
23	13.154	1838	1839	1842	rBV3	11589	7535	1.59%	0.185%
24	13.577	1909	1911	1915	rBV	34909	35378	7.48%	0.867%
25	14.148	2004	2008	2012	rBV	439761	472997	100.00%	11.587%
26	15.695	2268	2271	2275	rVB2	190674	234383	49.55%	5.742%


Sum of corrected areas: 4082039

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070318\
Data File : BF107079.D
Acq On : 3 Jul 2018 13:51
Operator : JU/SJ
Sample : J3629-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
A0C14-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

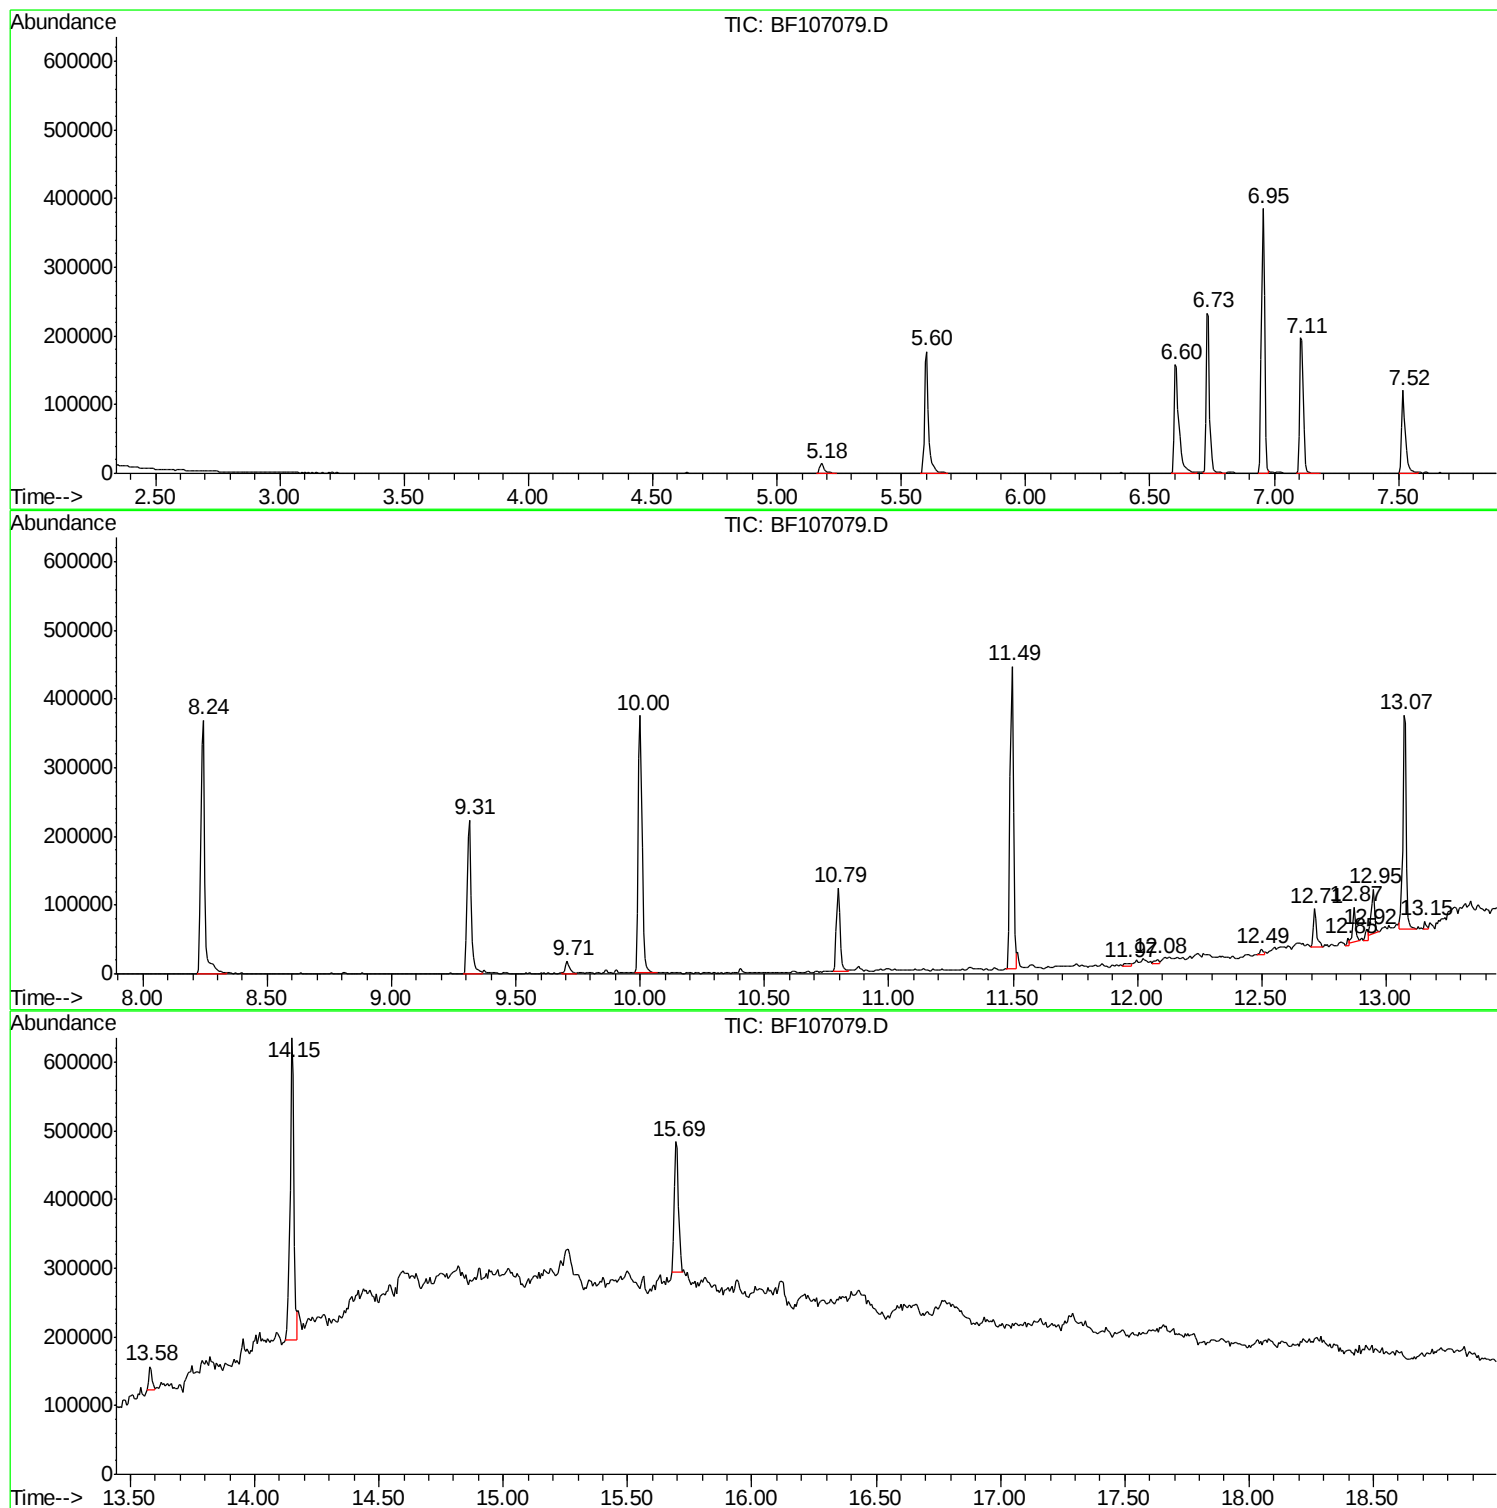

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF070318\
Data File : BF107079.D
Acq On : 3 Jul 2018 13:51
Operator : JU/SJ
Sample : J3629-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A0C14-01










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.73 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.73	14.69 ng	229684	1,4-Dichlorobenzene-d4	6.95

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	12
3			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
4			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5			4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

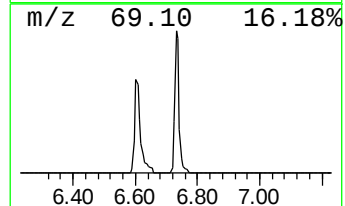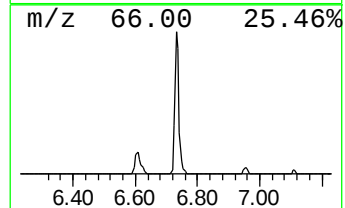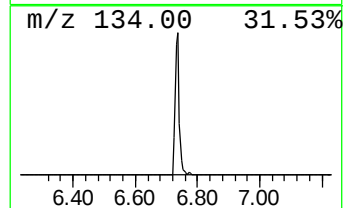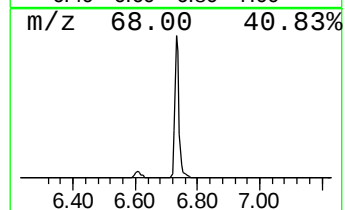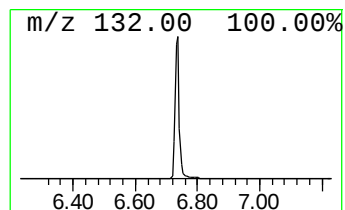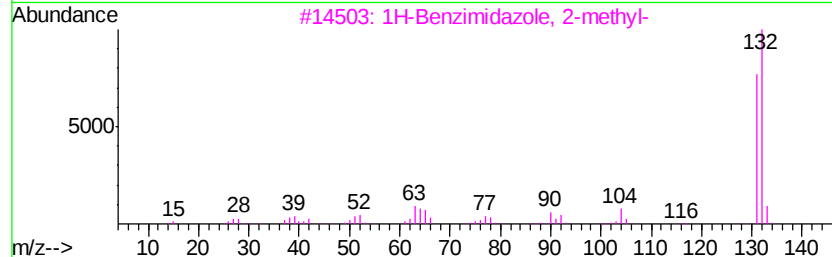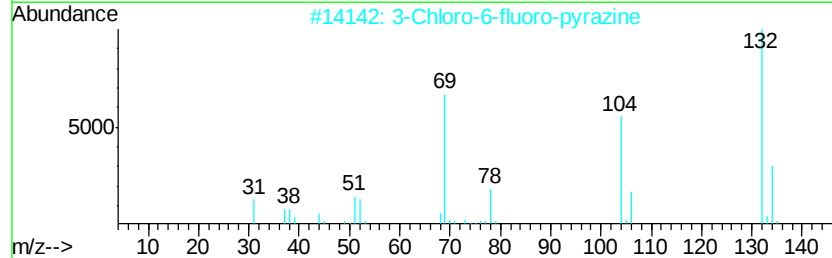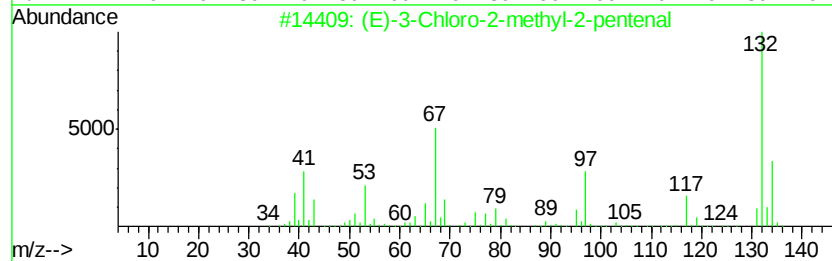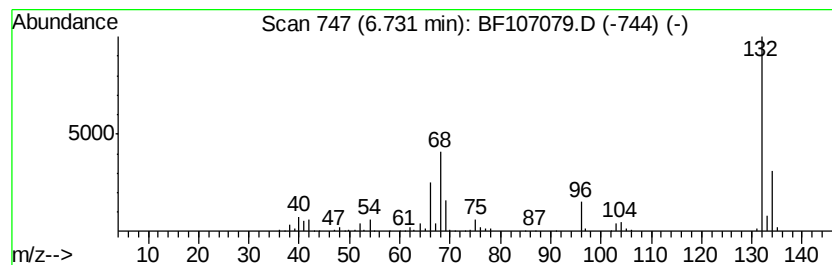

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070318\
Data File : BF107079.D
Acq On : 3 Jul 2018 13:51
Operator : JU/SJ
Sample : J3629-13
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A0C14-01

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.73	6.73	14.7	ng	229684	1	6.95	312739	20.0