


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070318\
 Data File : BF107070.D
 Acq On : 3 Jul 2018 9:14
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 29 14:38:29 2018

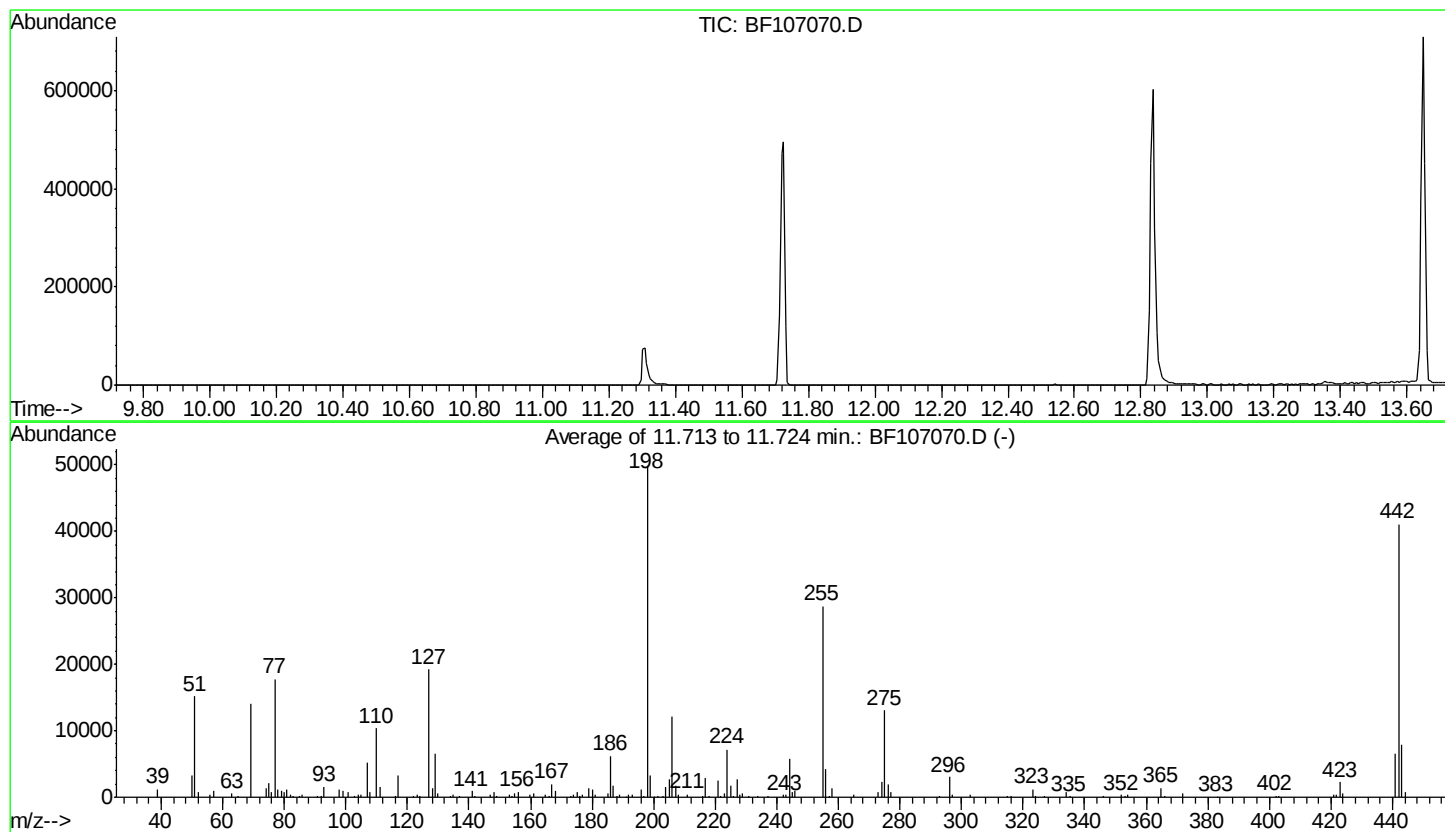

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	15134	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.1	14018	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.5	19198	PASS
197	198	0.00	2	0.5	258	PASS
198	198	100	100	100.0	49896	PASS
199	198	5	9	6.5	3244	PASS
275	198	10	60	26.2	13073	PASS
365	198	1	100	2.7	1370	PASS
441	198	0.01	100	13.1	6517	PASS
442	198	50	100	82.2	41026	PASS
443	442	15	24	19.1	7849	PASS