


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070318\
Data File : BF107096.D
Acq On : 3 Jul 2018 22:34
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 29 14:38:29 2018

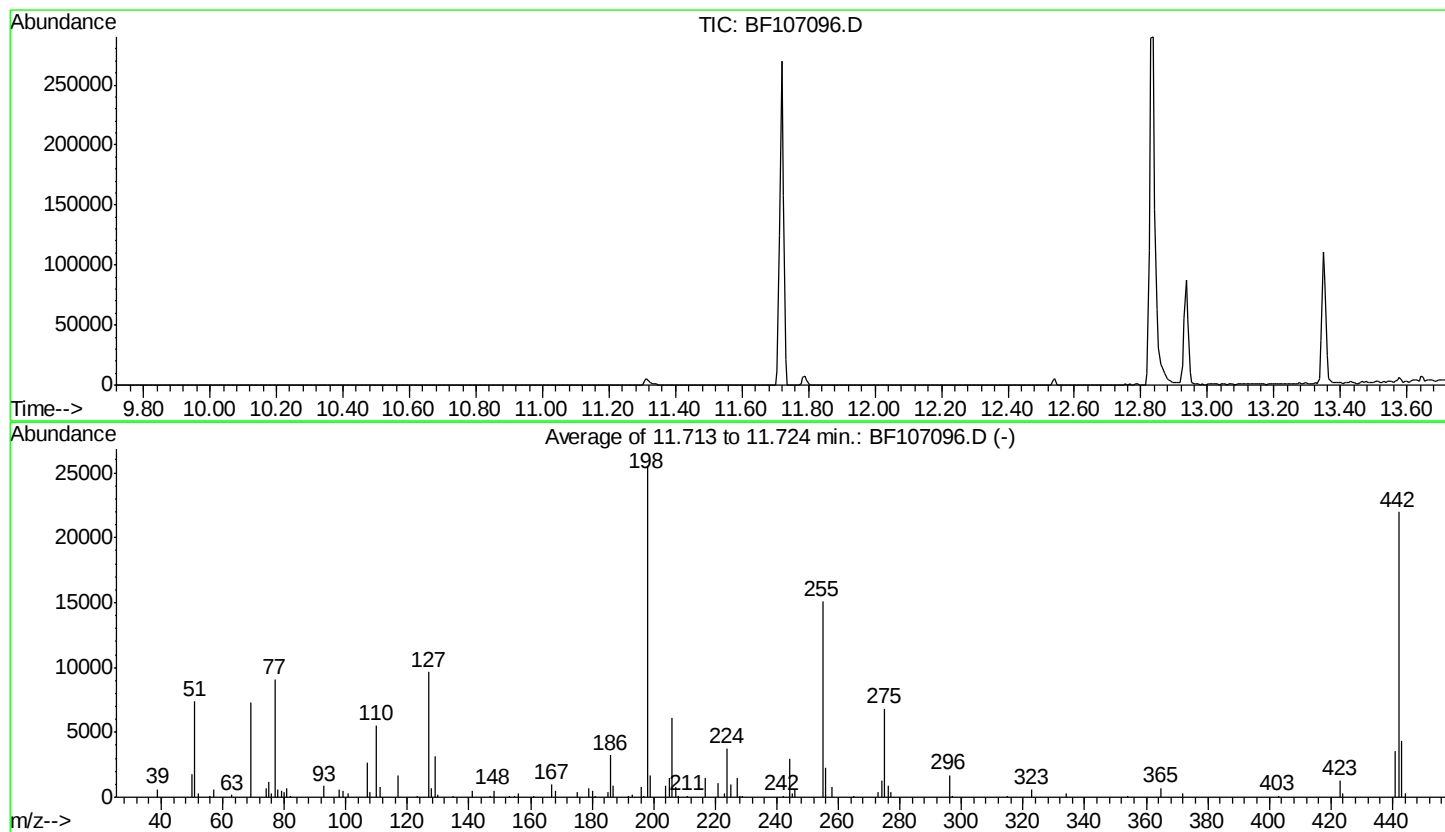

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.8	7372	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	28.7	7341	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.7	9628	PASS
197	198	0.00	2	0.4	111	PASS
198	198	100	100	100.0	25554	PASS
199	198	5	9	6.6	1699	PASS
275	198	10	60	26.7	6831	PASS
365	198	1	100	2.9	741	PASS
441	198	0.01	100	13.8	3517	PASS
442	198	50	100	86.0	21974	PASS
443	442	15	24	19.7	4335	PASS