
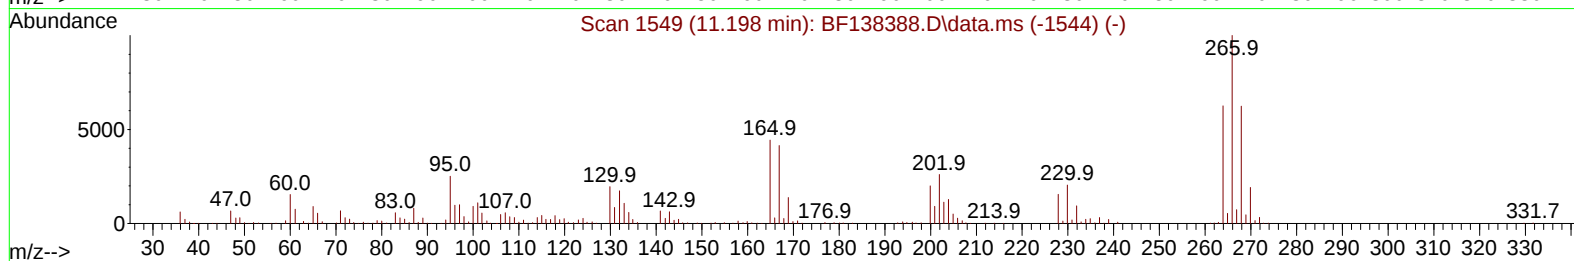
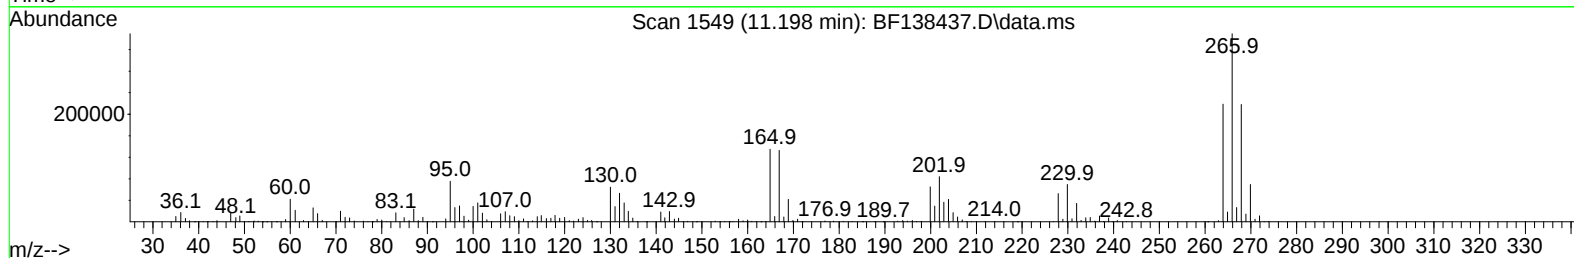


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF070324\  
Data File : BF138437.D  
Acq On : 03 Jul 2024 10:30  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 11:42:19 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF062824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jun 29 02:44:30 2024  
Response via : Initial Calibration

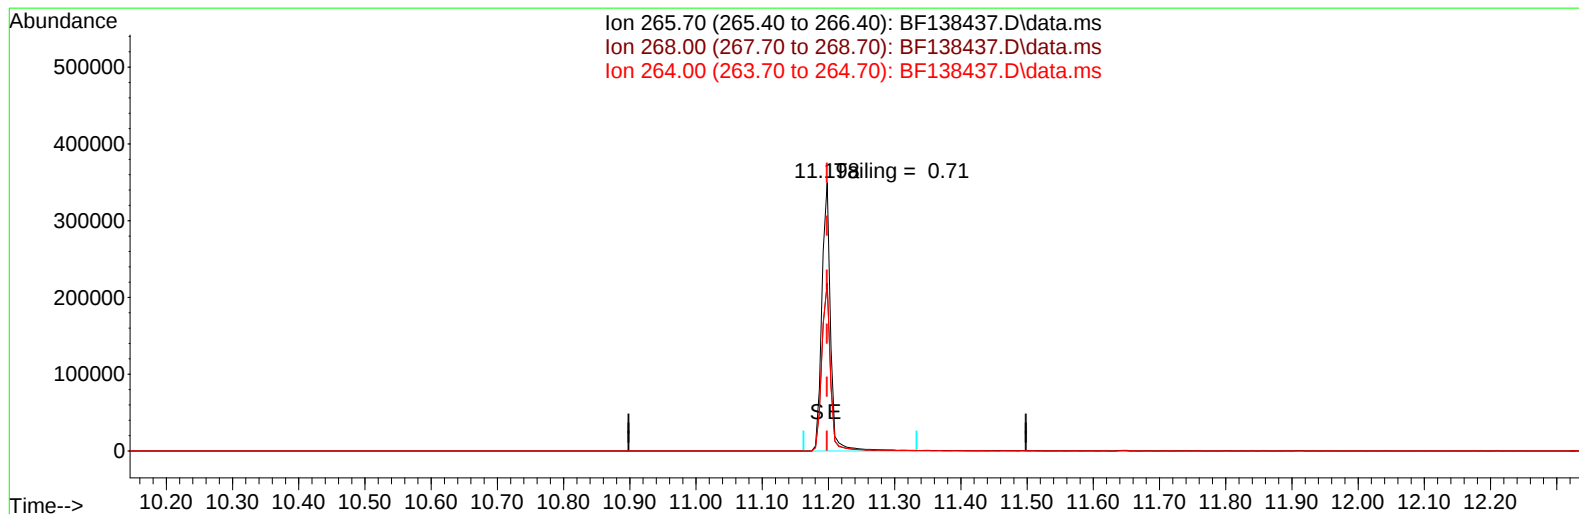

TIC: BF138437.D\data.ms

**(70) Pentachlorophenol (C)**




**11.198min (+ 0.000) 916547.31 ng**

**response 319651**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.40  | 62.38  |
| 264.00 | 62.50  | 62.58  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF070324\  
Data File : BF138437.D  
Acq On : 03 Jul 2024 10:30  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 03 11:42:19 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF062824.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Jun 29 02:44:30 2024  
Response via : Initial Calibration

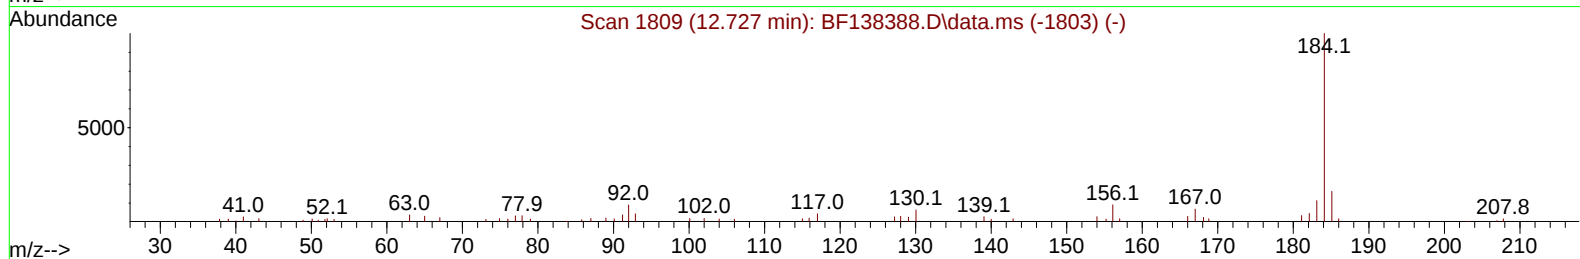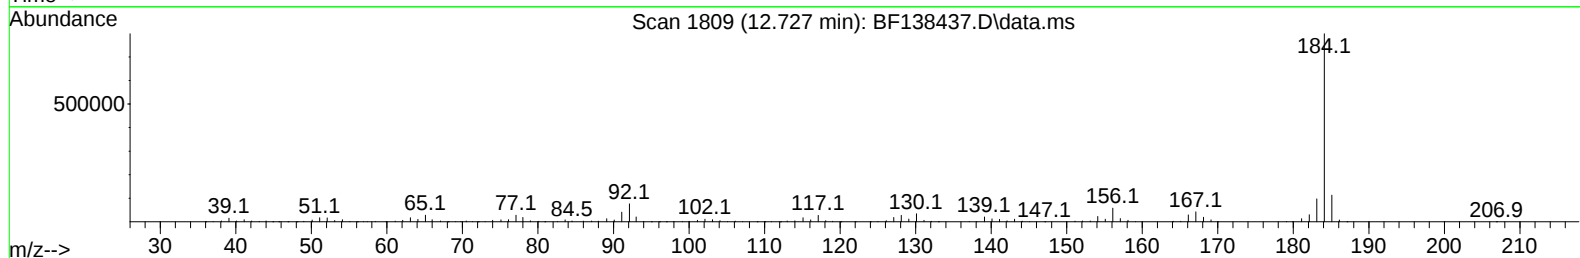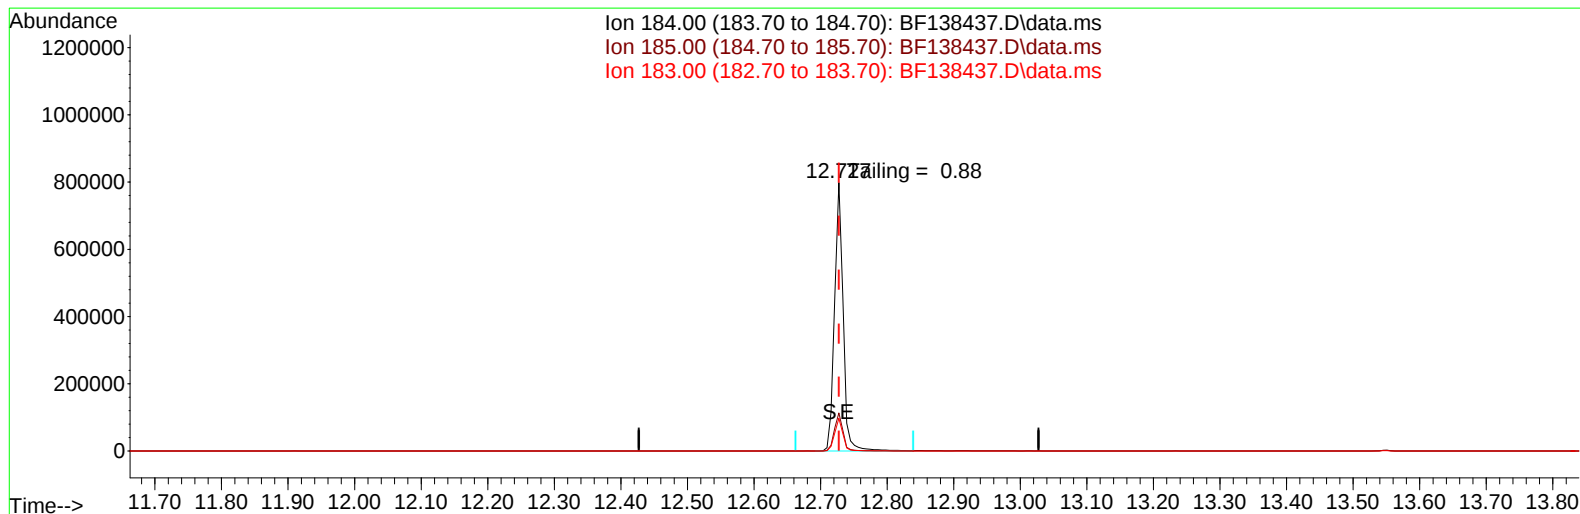

TIC: BF138437.D\data.ms

**(77) Benzidine**

**12.727min (+ 0.000) 425917.42 ng**

**response 722030**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 16.20  | 14.19  |
| 183.00 | 11.30  | 12.17  |
| 0.00   | 0.00   | 0.00   |