


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070324\
Data File : BF138437.D
Acq On : 03 Jul 2024 10:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jun 29 02:44:30 2024

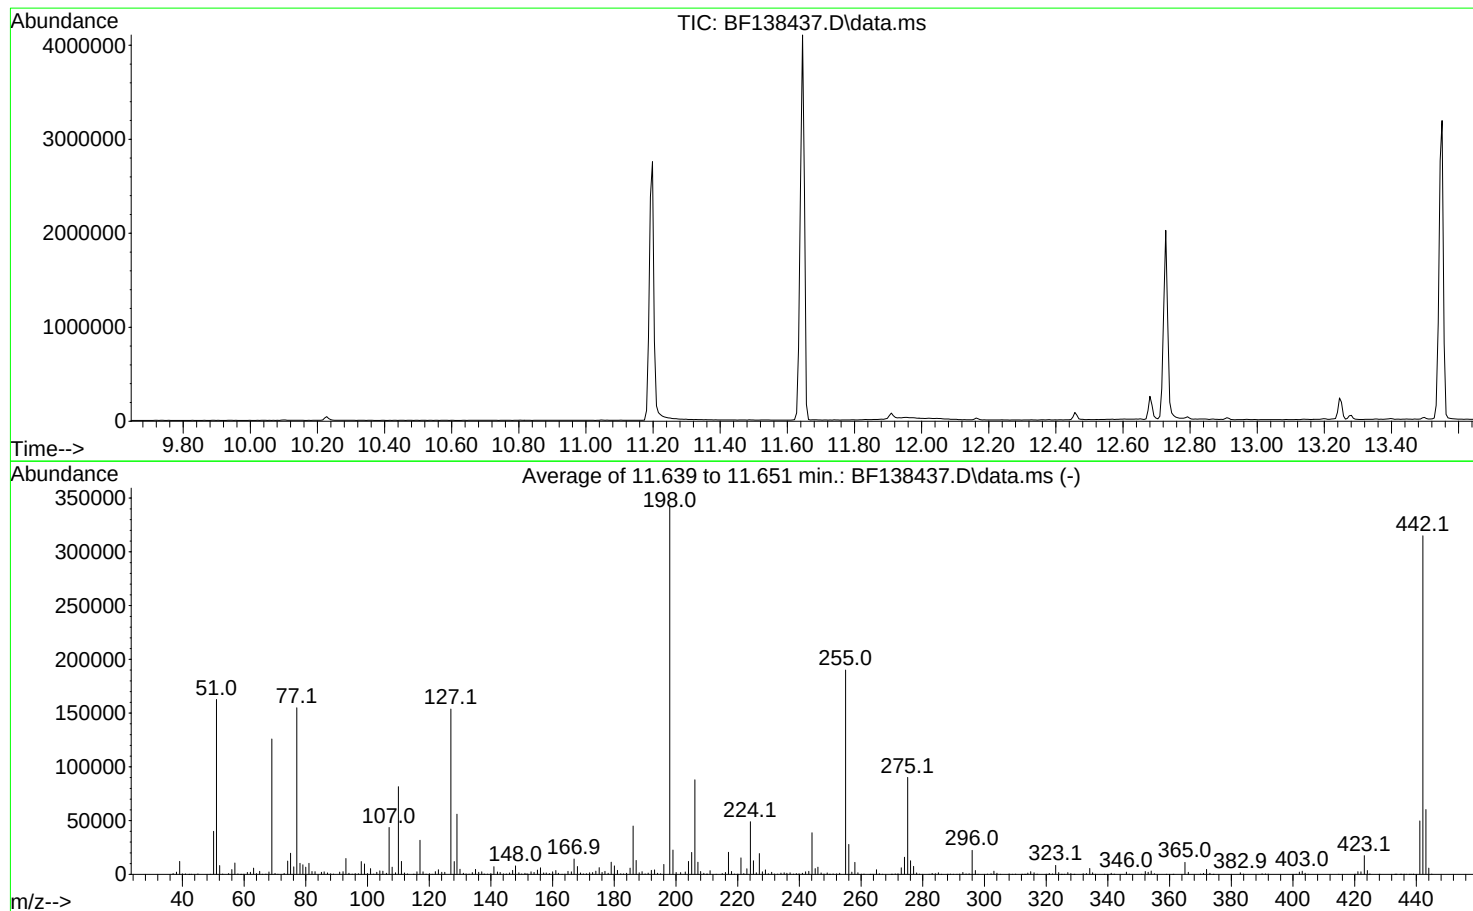

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	47.6	162724	PASS
68	69	0.00	2	1.7	2176	PASS
69	198	0.00	100	36.8	125875	PASS
70	69	0.00	2	0.7	846	PASS
127	198	10	80	44.9	153701	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	342187	PASS
199	198	5	9	6.6	22565	PASS
275	198	10	60	26.3	90165	PASS
365	198	1	100	3.3	11223	PASS
441	198	0.01	100	14.5	49731	PASS
442	442	50	100	100.0	314880	PASS
443	442	15	24	19.2	60304	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/3/2024	BNA_F	<u>BF138437.D</u>
Compound Name	Response	Retention Time
DDT	534449	13.551
DDD	44914	13.245
DDE	2075	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
46989	581438	8.08

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070324\
Data File : BF138437.D
Acq On : 03 Jul 2024 10:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 03 11:42:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

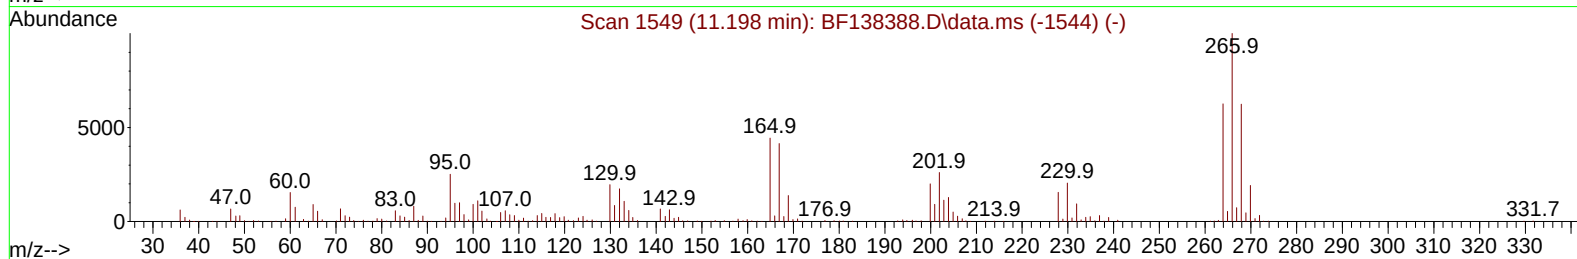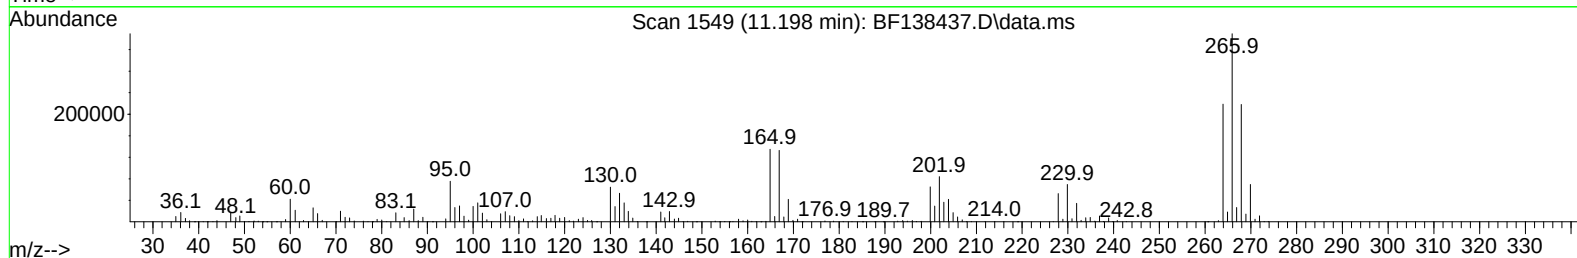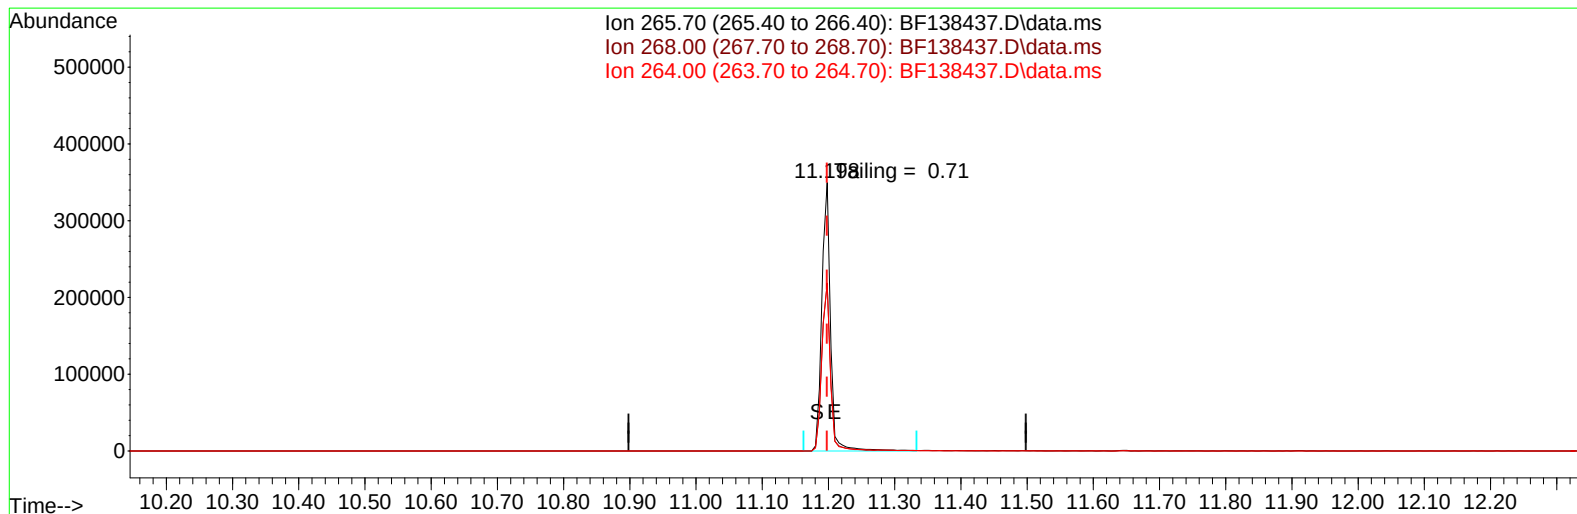

TIC: BF138437.D\data.ms

(70) Pentachlorophenol (C)

11.198min (+ 0.000) 916547.31 ng




response 319651

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.38
264.00	62.50	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070324\
Data File : BF138437.D
Acq On : 03 Jul 2024 10:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 03 11:42:19 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 29 02:44:30 2024
Response via : Initial Calibration

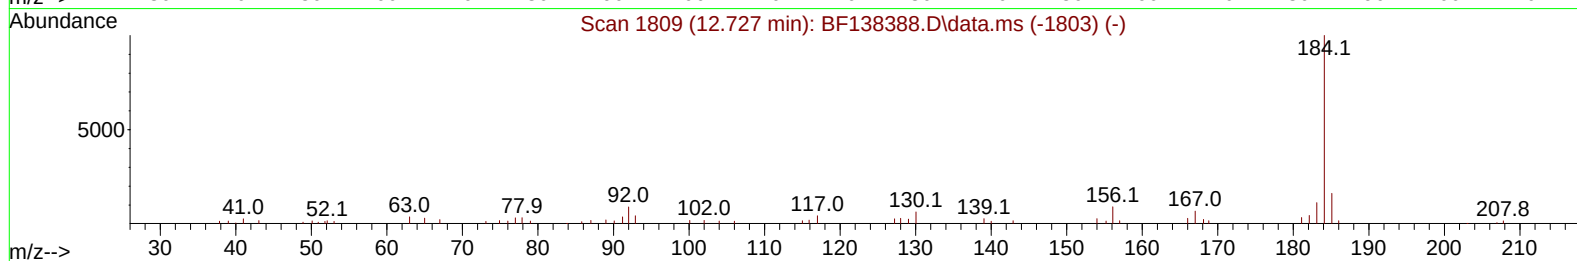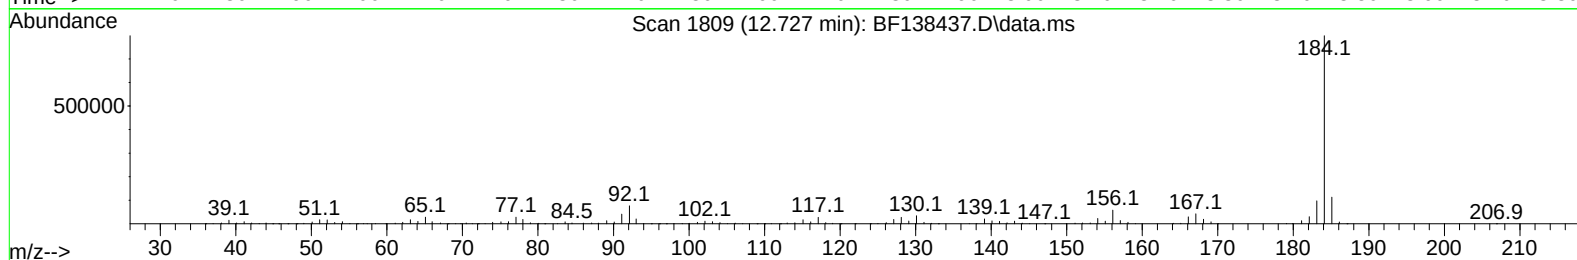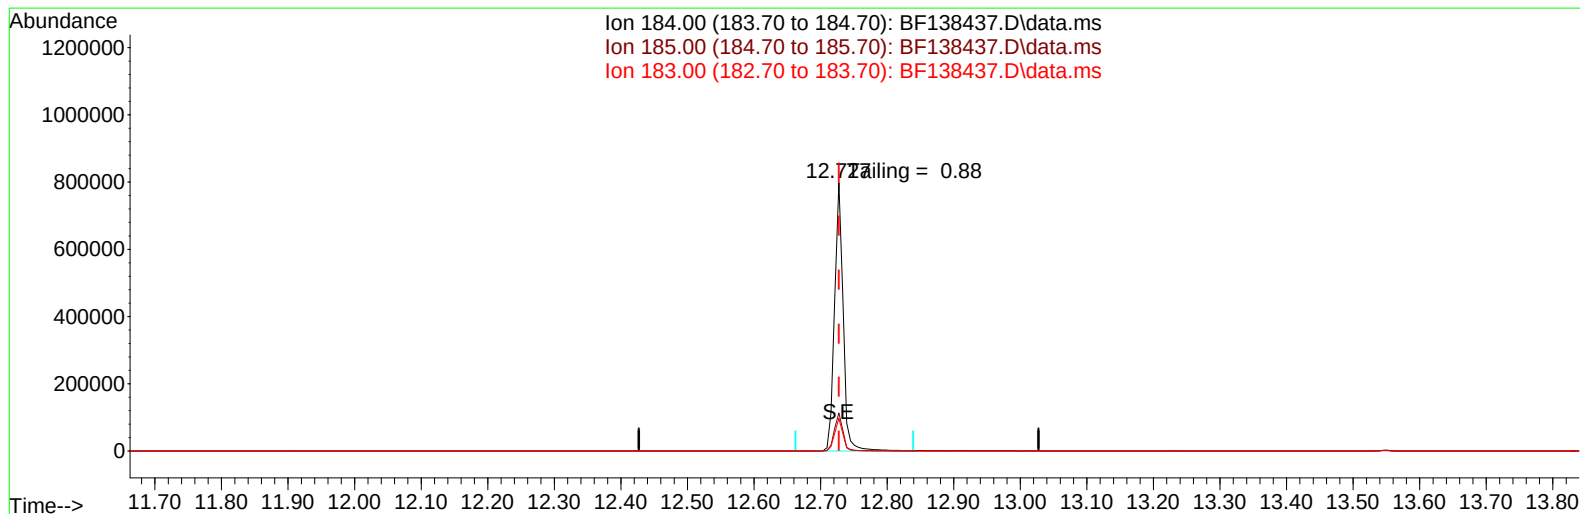

TIC: BF138437.D\data.ms

(77) Benzidine

12.727min (+ 0.000) 425917.42 ng

response 722030

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.20	14.19
183.00	11.30	12.17
0.00	0.00	0.00