


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070523\
 Data File : BF134072.D
 Acq On : 05 Jul 2023 17:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 30 18:35:29 2023

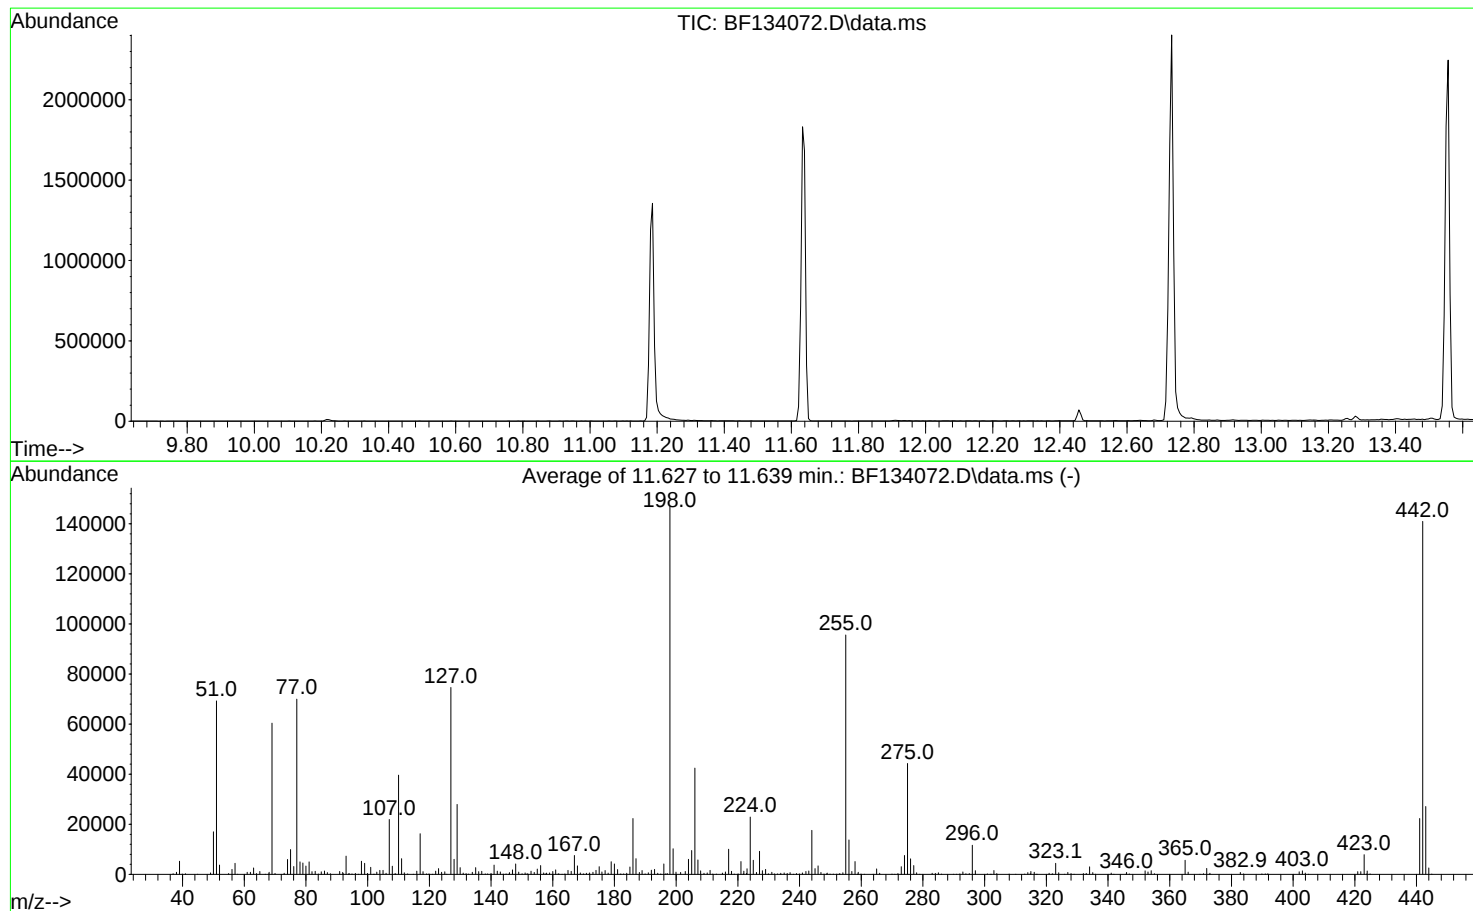

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	69283	PASS
68	69	0.00	2	1.3	815	PASS
69	198	0.00	100	41.1	60376	PASS
70	69	0.00	2	0.6	376	PASS
127	198	10	80	50.8	74661	PASS
197	198	0.00	2	0.3	420	PASS
198	198	100	100	100.0	146917	PASS
199	198	5	9	7.0	10228	PASS
275	198	10	60	30.2	44299	PASS
365	198	1	100	3.8	5607	PASS
441	198	0.01	100	15.2	22330	PASS
442	442	50	100	100.0	140944	PASS
443	442	15	24	19.2	27097	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/5/2023	BNA_F	<u>BF134072.D</u>
Compound Name	Response	Retention Time
DDT	393254	13.557
DDD	6215	13.28
DDE	453	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6668	399922	1.67

Instrument :
BNA_F
ClientSampleId :
DFTPP

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070523\  
Data File : BF134072.D  
Acq On    : 05 Jul 2023 17:55  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 06 05:10:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

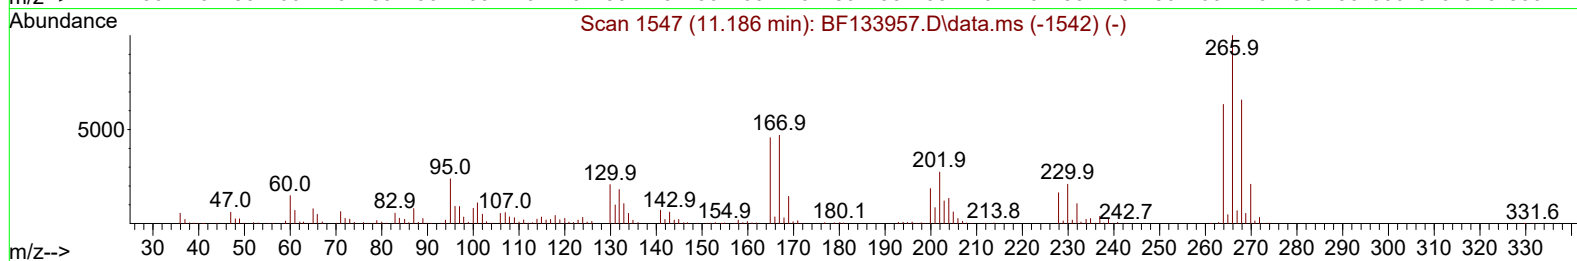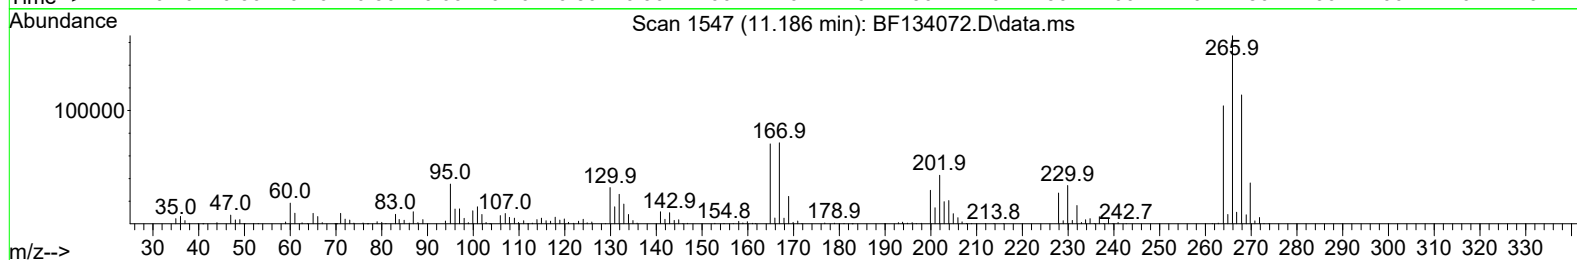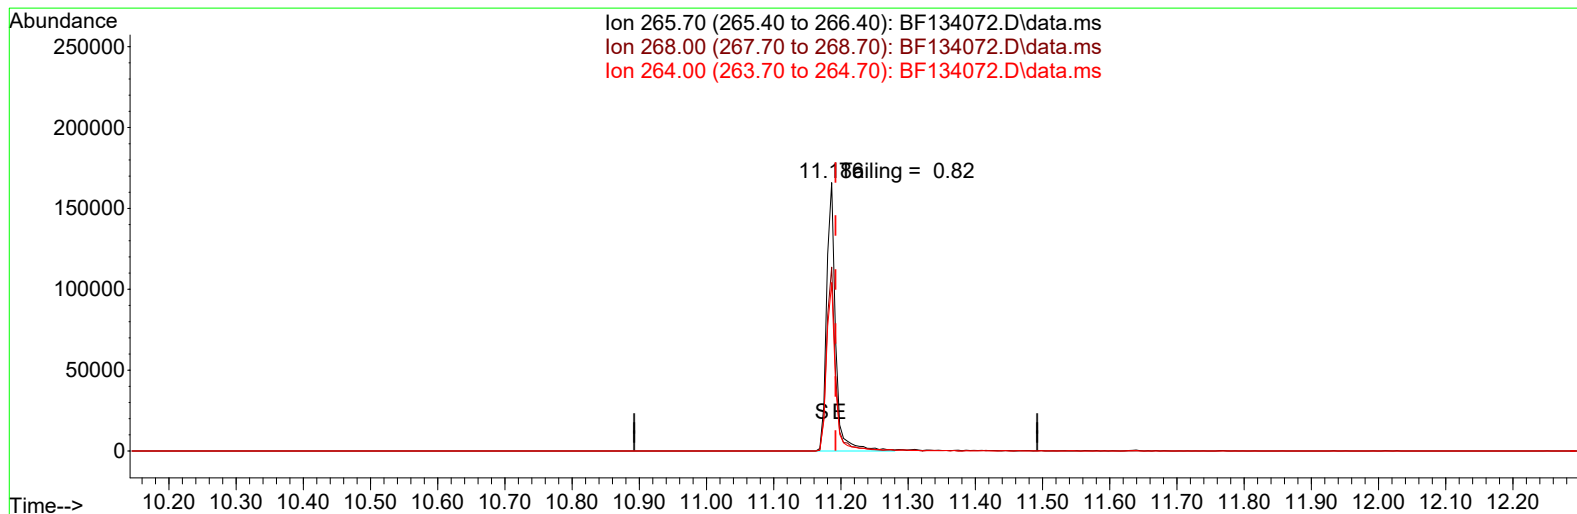

TIC: BF134072.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 29176.48 ng




response **155333**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	68.53
264.00	63.30	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070523\
Data File : BF134072.D
Acq On : 05 Jul 2023 17:55
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 06 05:10:58 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

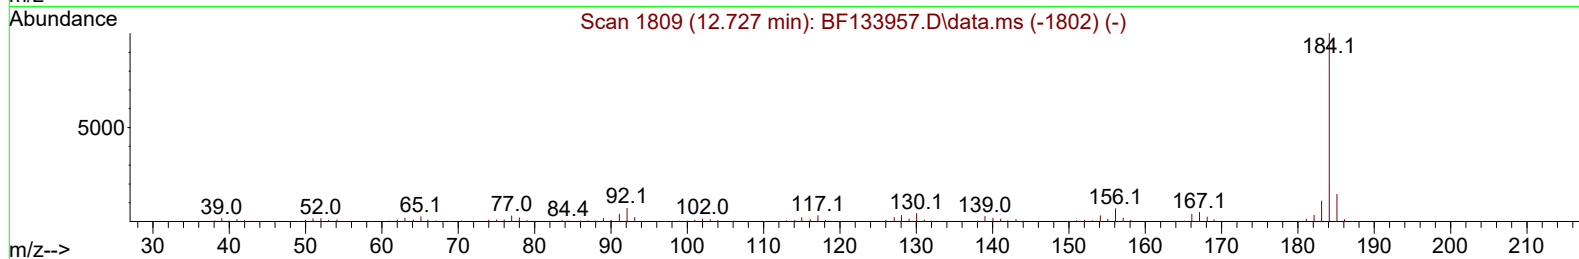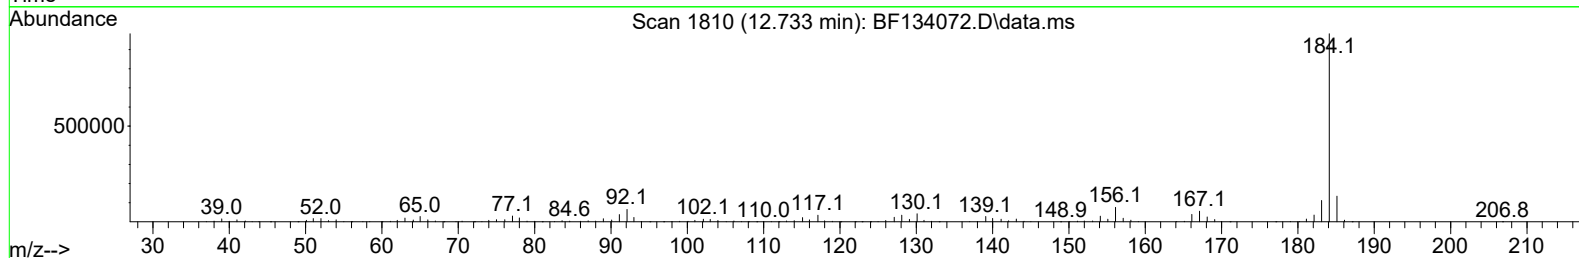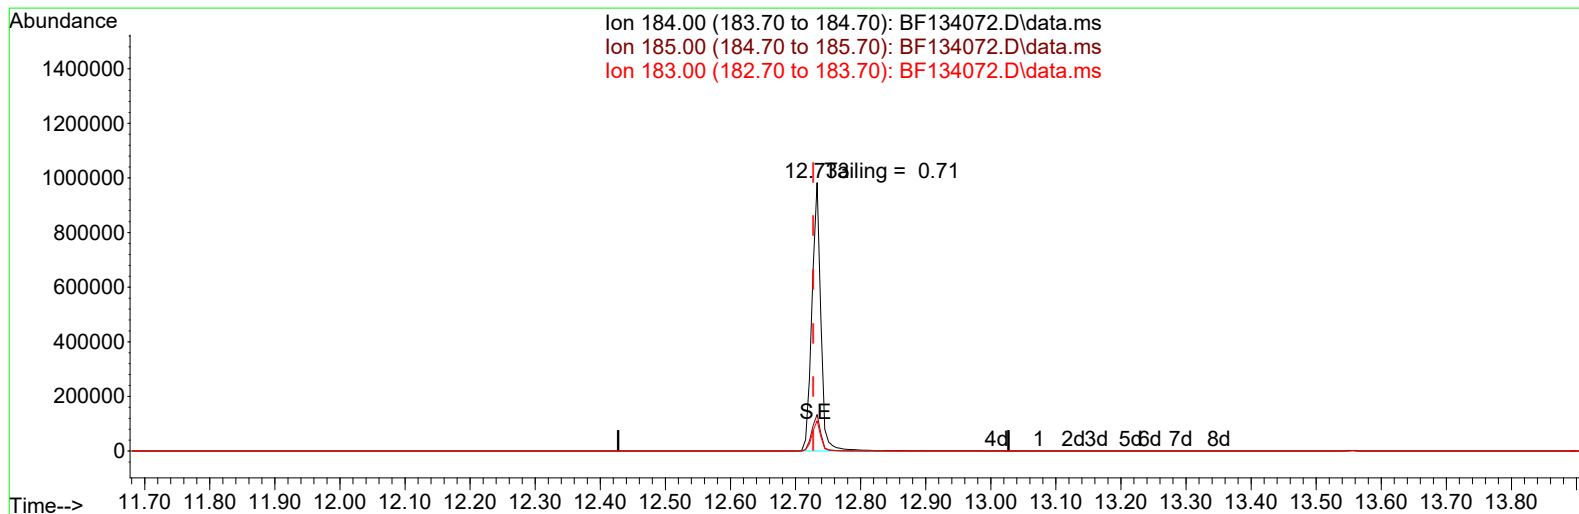

TIC: BF134072.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 679415.48 ng m

response 937642

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.63
183.00	11.00	11.30
0.00	0.00	0.00