
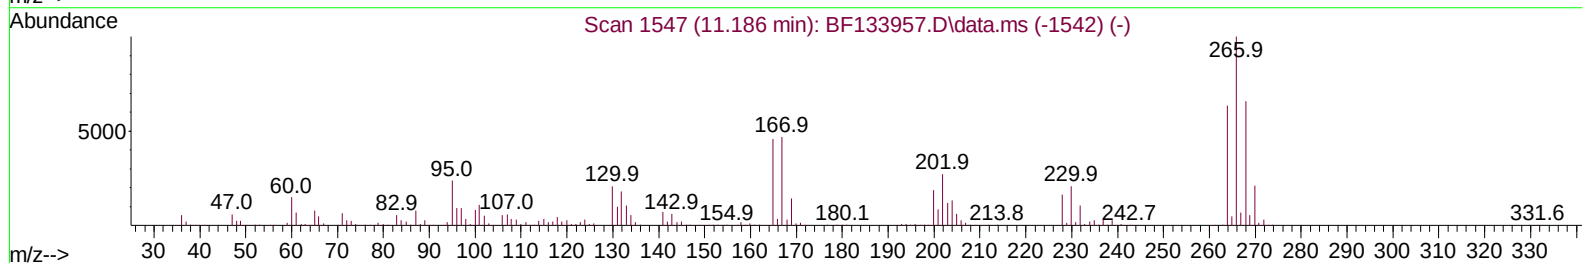
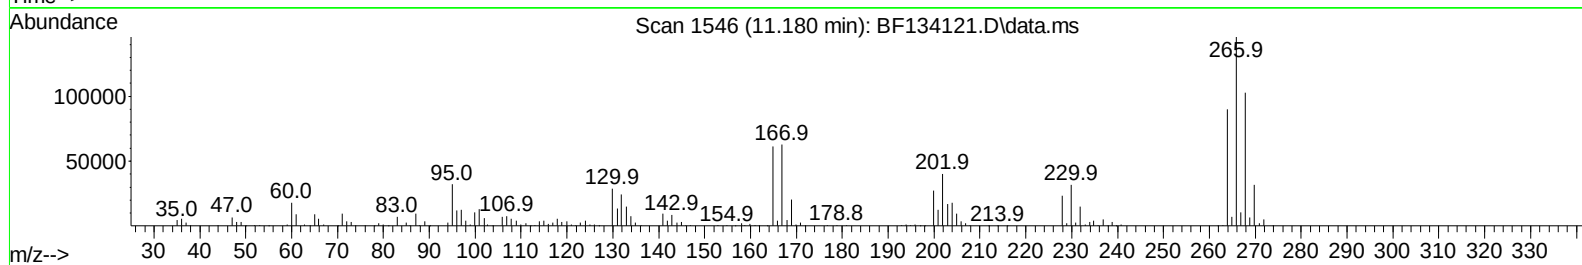


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
 Data File : BF134121.D
 Acq On : 07 Jul 2023 05:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 05:42:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 30 18:35:29 2023
 Response via : Initial Calibration

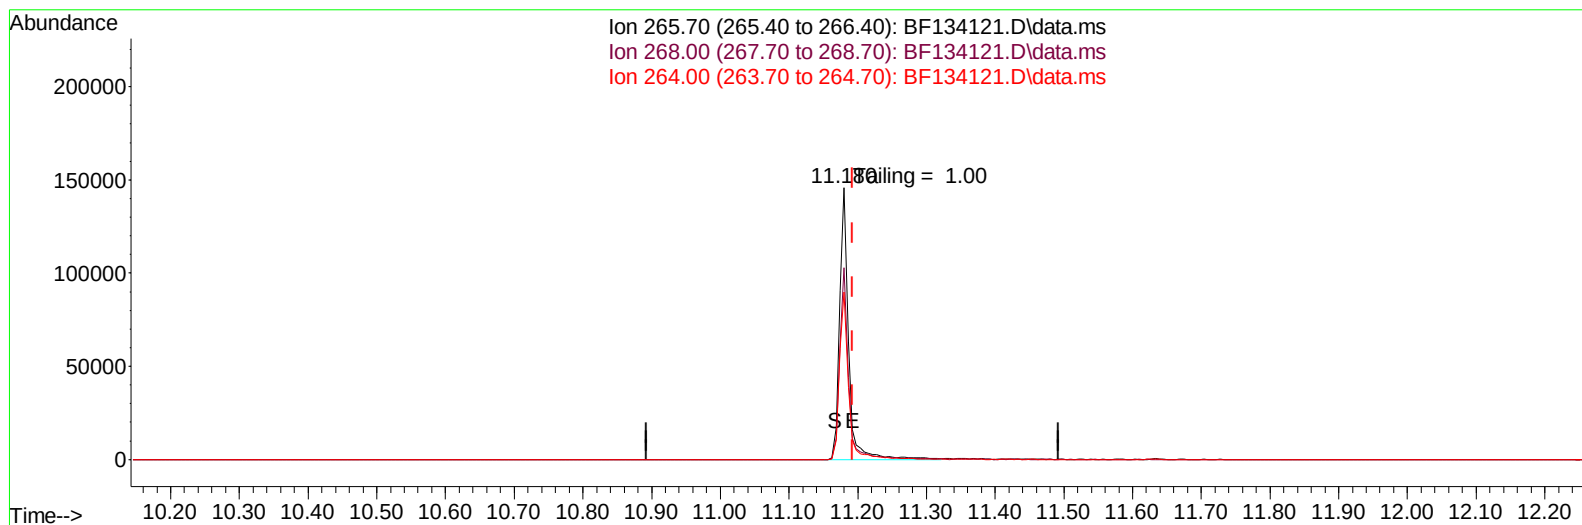




TIC: BF134121.D\data.ms

(70) Pentachlorophenol (C)**11.180min (-0.012) 149903.62 ng****response 129472**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	70.51
264.00	63.30	61.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
Data File : BF134121.D
Acq On : 07 Jul 2023 05:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 07 05:42:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

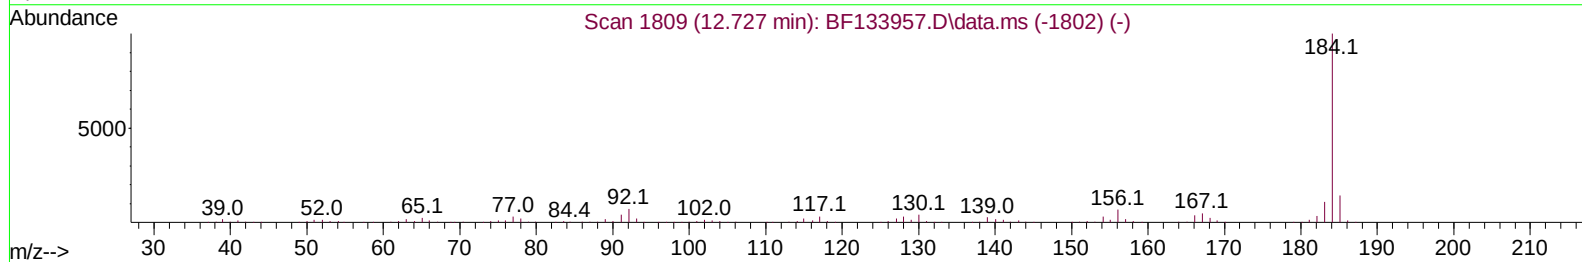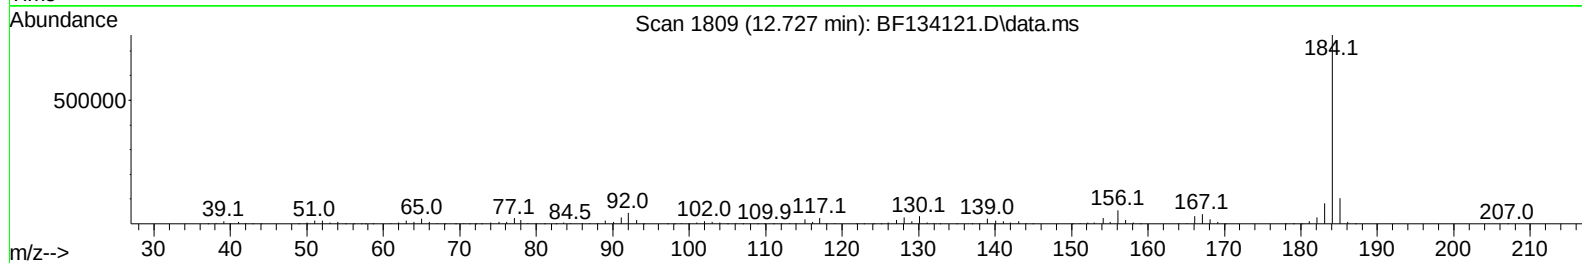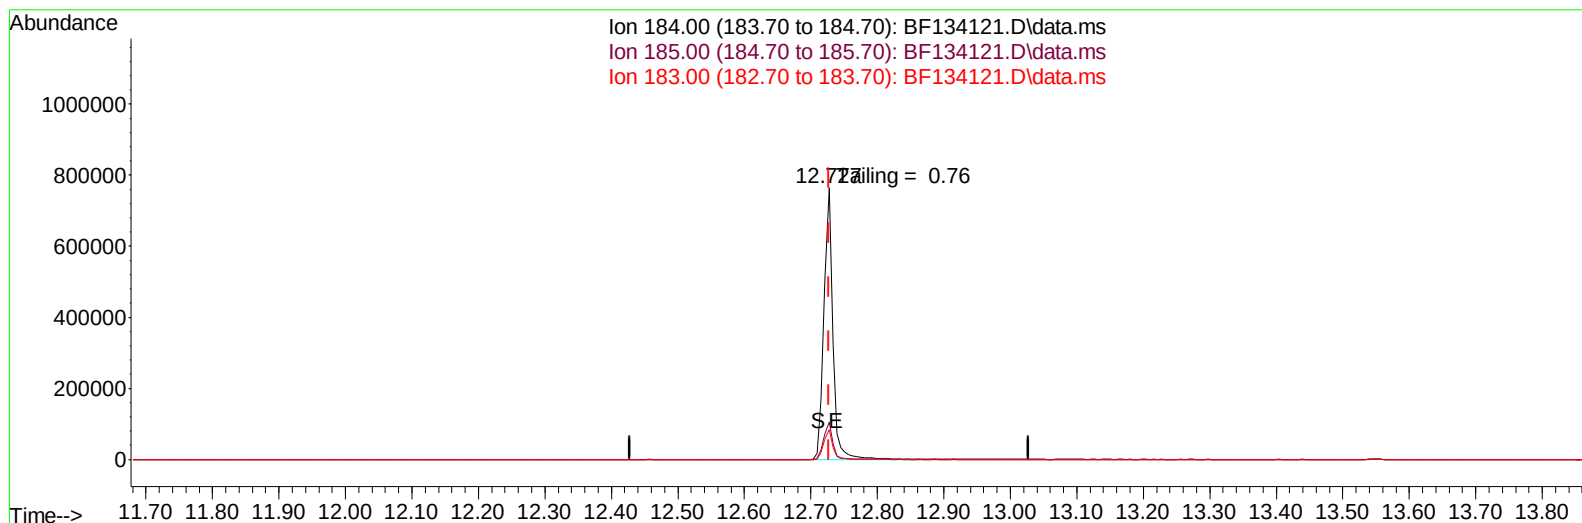

TIC: BF134121.D\data.ms

(77) Benzidine

12.727min (-0.000) 232610.69 ng

response 697387

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.74
183.00	11.00	10.97
0.00	0.00	0.00