

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
 Data File : BF134115.D
 Acq On : 07 Jul 2023 01:21
 Operator : CG\JU
 Sample : 03375-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-3(8-10)

Quant Time: Jul 07 04:10:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 30 18:35:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.845	152	100622	20.000	ng	0.00
21) Naphthalene-d8	8.122	136	395440	20.000	ng	-0.01
39) Acenaphthene-d10	9.881	164	194702	20.000	ng	-0.01
64) Phenanthrene-d10	11.375	188	387501	20.000	ng	-0.01
76) Chrysene-d12	14.033	240	248689	20.000	ng	-0.02
86) Perylene-d12	15.533	264	207364	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.481	112	573979	95.420	ng	0.00
7) Phenol-d6	6.481	99	709628	95.926	ng	-0.01
23) Nitrobenzene-d5	7.404	82	476905	65.010	ng	-0.02
42) 2,4,6-Tribromophenol	10.675	330	232134	95.091	ng	-0.01
45) 2-Fluorobiphenyl	9.204	172	857826	64.056	ng	0.00
79) Terphenyl-d14	12.974	244	940579	60.871	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
Data File : BF134115.D
Acq On : 07 Jul 2023 01:21
Operator : CG\JU
Sample : 03375-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3(8-10)

Quant Time: Jul 07 04:10:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration




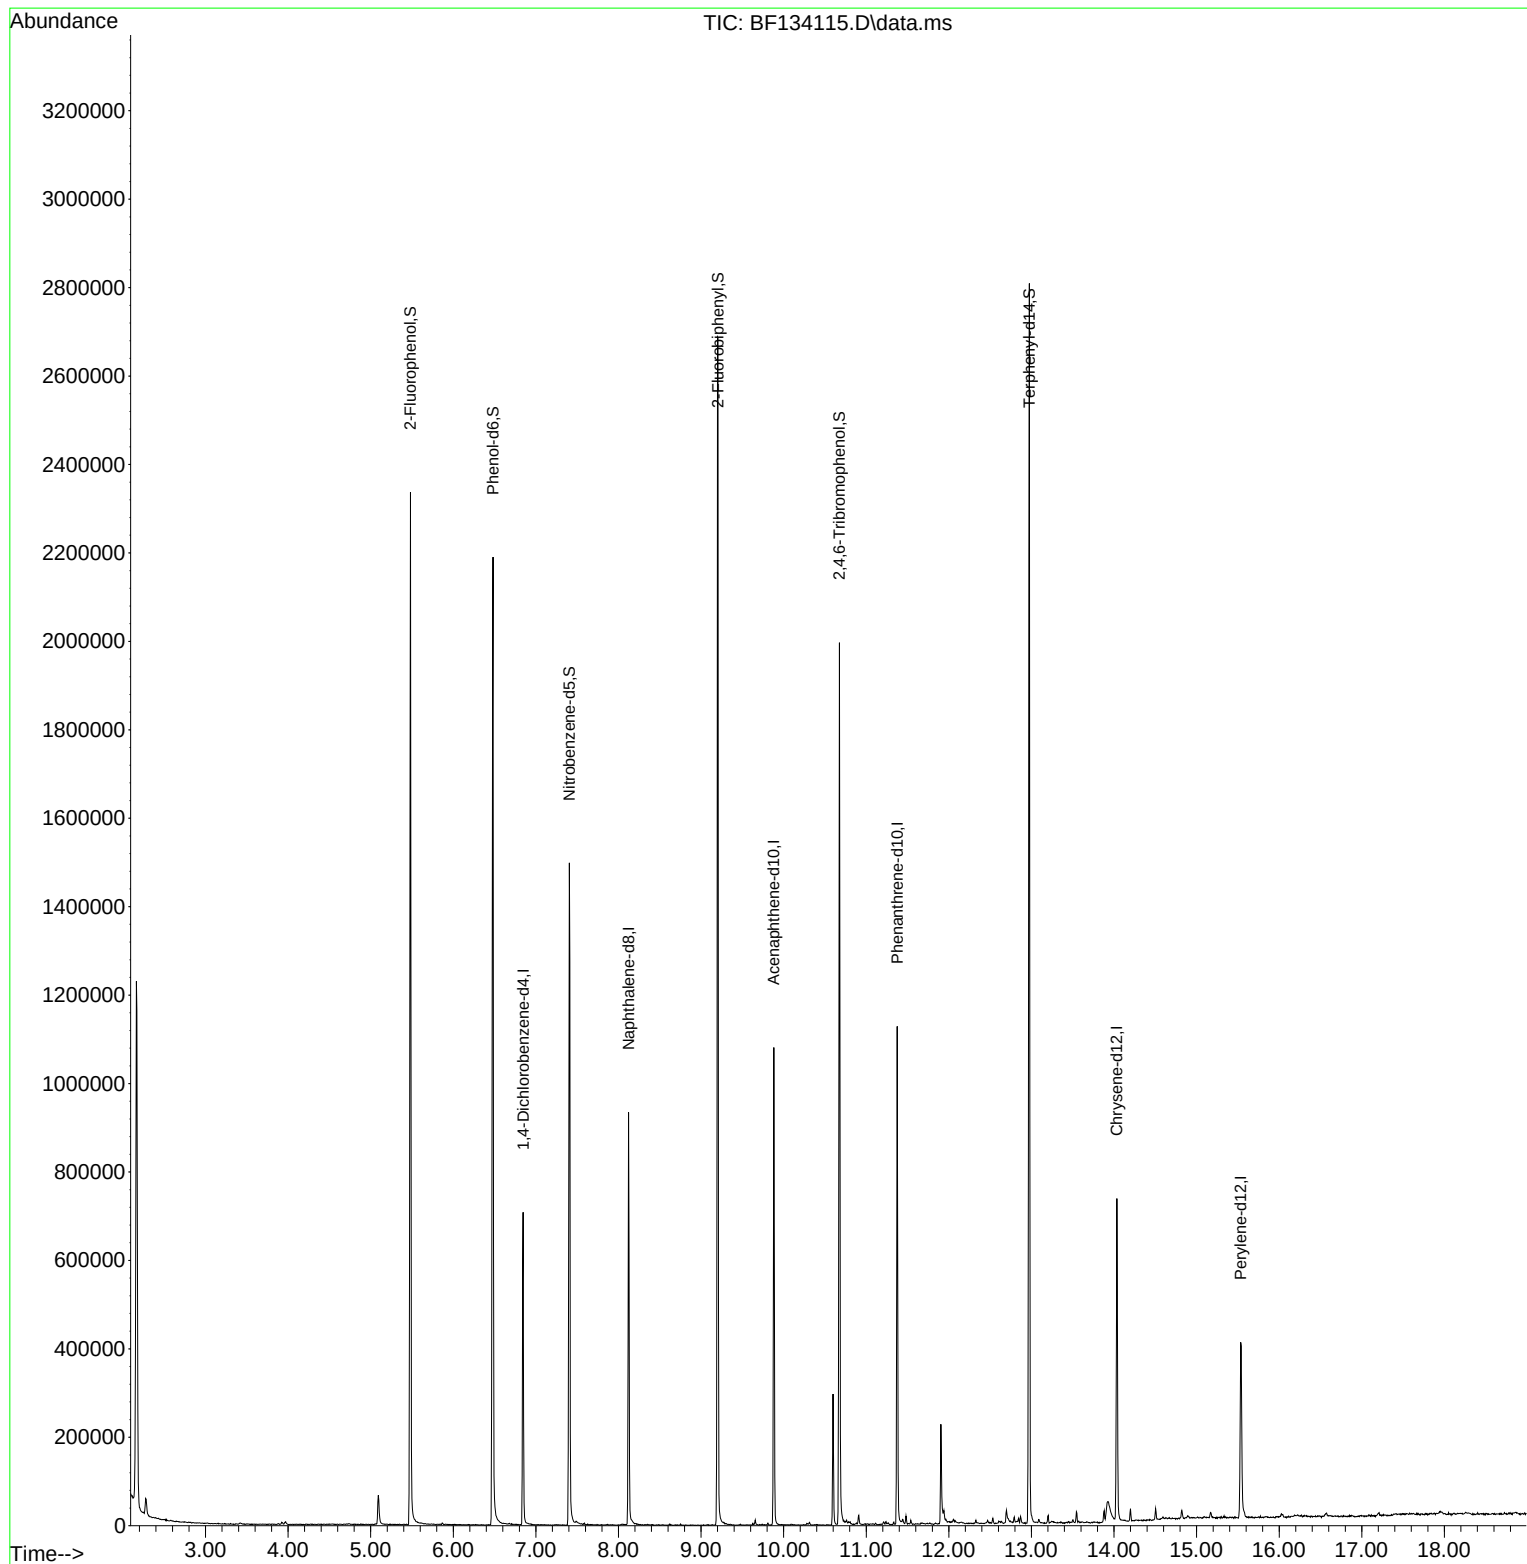


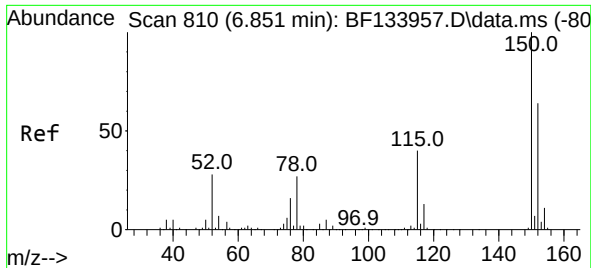

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.845 min Scan# 810
Delta R.T. -0.006 min
Lab File: BF134115.D
Acq: 07 Jul 2023 01:21




Instrument :
BNA_F
ClientSampleId :
SB-3(8-10)


Tgt Ion:152 Resp: 100622
Ion Ratio Lower Upper
152 100
150 157.9 124.5 186.7
115 61.1 50.2 75.2

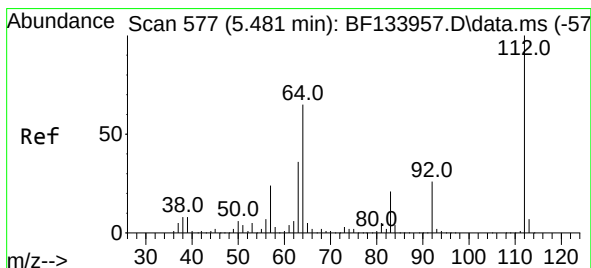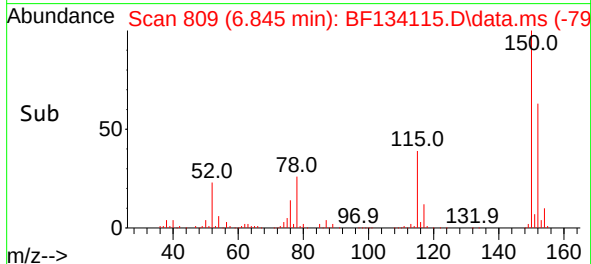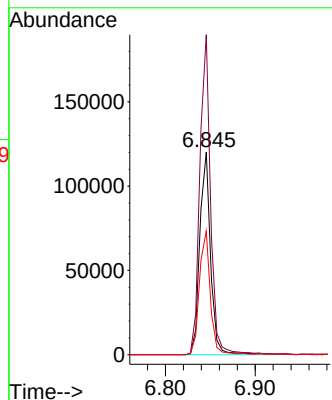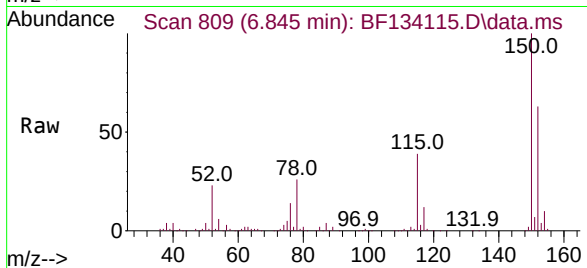

#5
2-Fluorophenol
Concen: 95.420 ng
RT: 5.481 min Scan# 577
Delta R.T. -0.006 min
Lab File: BF134115.D
Acq: 07 Jul 2023 01:21


Tgt Ion:112 Resp: 573979
Ion Ratio Lower Upper
112 100
64 63.6 52.1 78.1
63 36.5 28.6 42.8

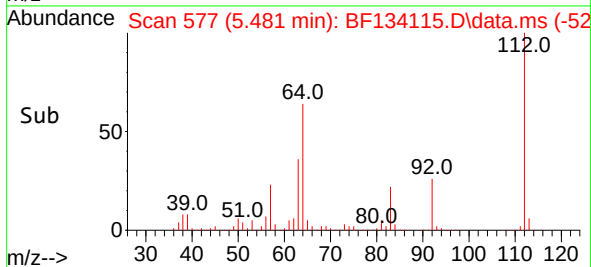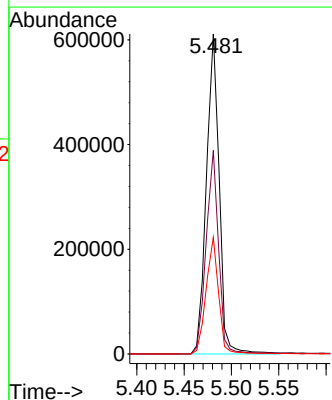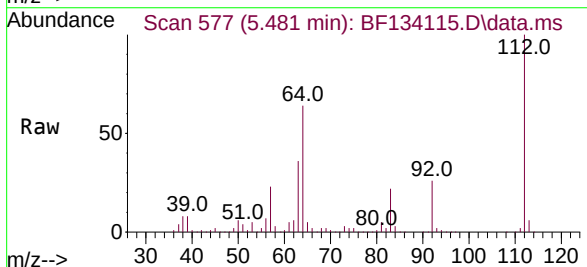

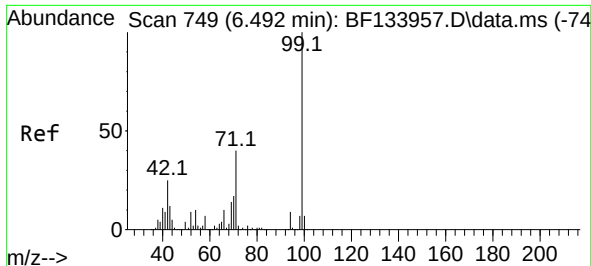




#7
Phenol-d6
Concen: 95.926 ng
RT: 6.481 min Scan# 749
Delta R.T. -0.012 min
Lab File: BF134115.D
Acq: 07 Jul 2023 01:21

Instrument :
BNA_F
ClientSampleId :
SB-3(8-10)

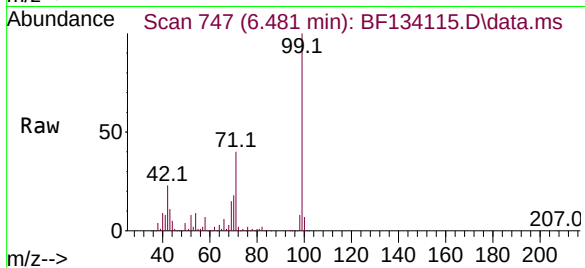

Tgt Ion: 99 Resp: 709628




Ion	Ratio	Lower	Upper
99	100		
42	23.4	19.8	29.6
71	40.4	31.9	47.9

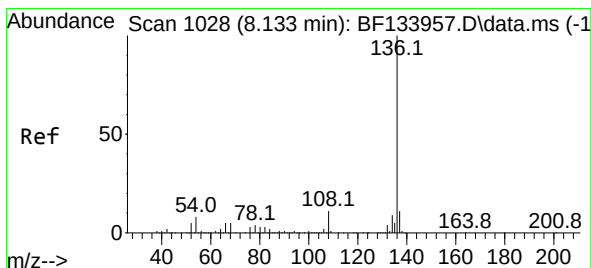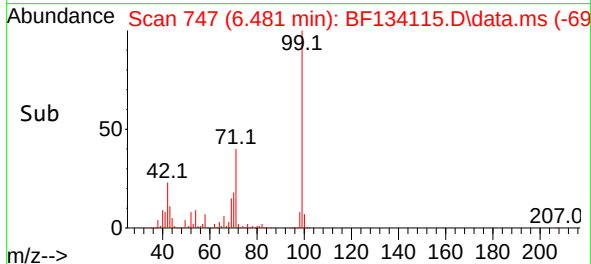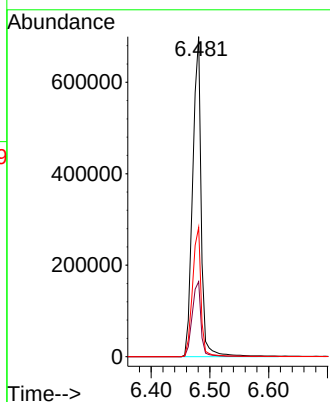


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.122 min Scan# 1026
Delta R.T. -0.012 min
Lab File: BF134115.D
Acq: 07 Jul 2023 01:21

Tgt Ion: 136 Resp: 395440

Ion	Ratio	Lower	Upper
136	100		
137	11.3	8.6	12.8
54	8.7	6.5	9.7
68	5.1	4.2	6.2

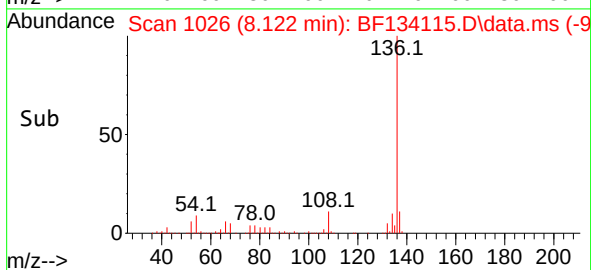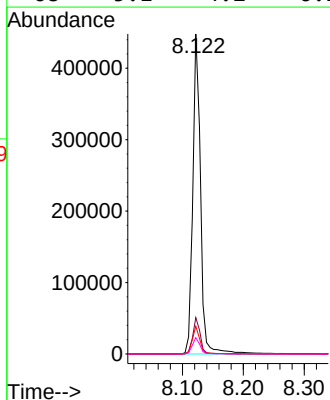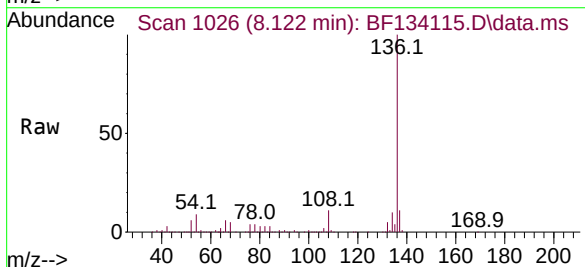

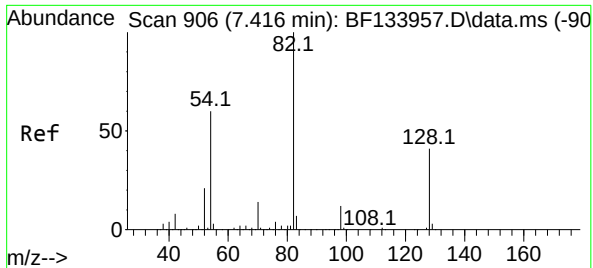

#23

Nitrobenzene-d5

Concen: 65.010 ng

RT: 7.404 min Scan# 906

Delta R.T. -0.018 min

Lab File: BF134115.D

Acq: 07 Jul 2023 01:21

Instrument :

BNA_F

ClientSampleId :

SB-3(8-10)





Tgt Ion: 82 Resp: 476905

Ion Ratio Lower Upper

82 100

128 39.7 32.5 48.7

54 59.2 48.2 72.2

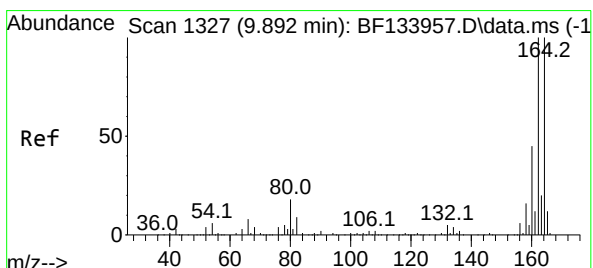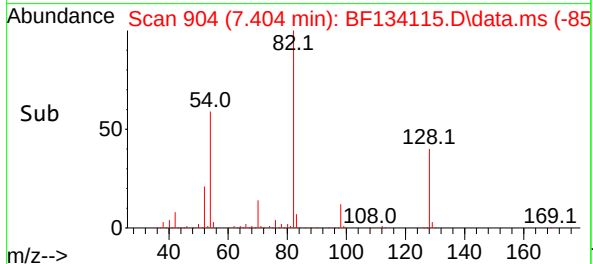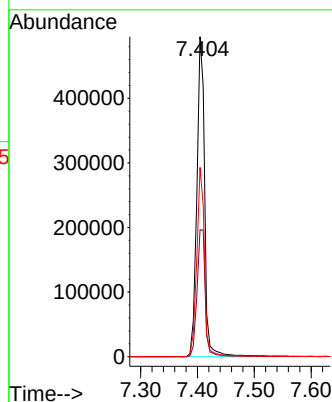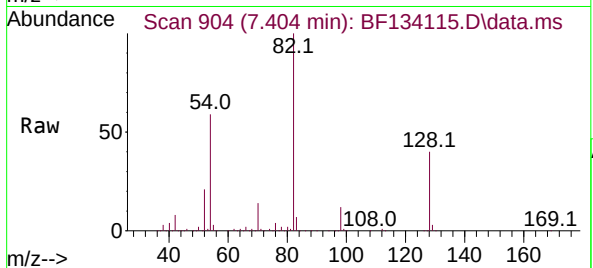

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.881 min Scan# 1325

Delta R.T. -0.012 min

Lab File: BF134115.D

Acq: 07 Jul 2023 01:21




Tgt Ion: 164 Resp: 194702


Ion Ratio Lower Upper

164 100

162 101.6 80.0 120.0

160 47.4 35.9 53.9


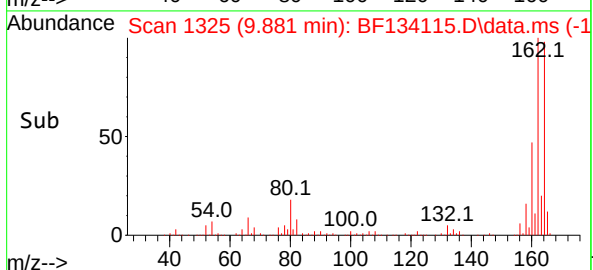
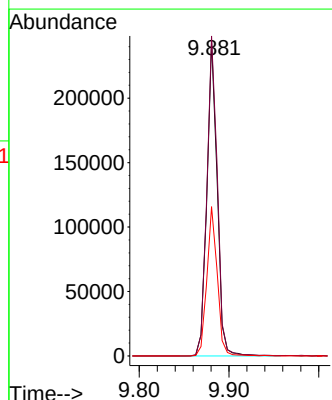
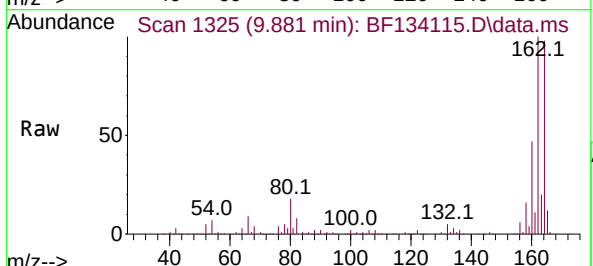


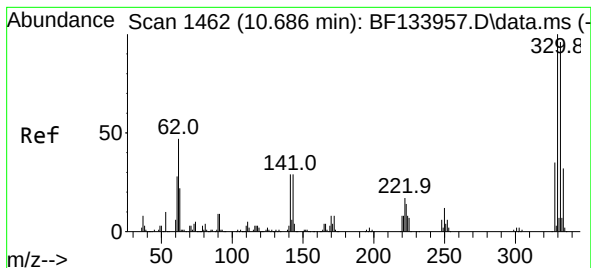

#42
2,4,6-Tribromophenol
Concen: 95.091 ng
RT: 10.675 min Scan# 1460
Delta R.T. -0.012 min
Lab File: BF134115.D
Acq: 07 Jul 2023 01:21




Instrument :
BNA_F
ClientSampleId :
SB-3(8-10)


Tgt Ion: 330 Resp: 232134
Ion Ratio Lower Upper
330 100
332 97.3 77.0 115.6
141 33.4 26.3 39.5

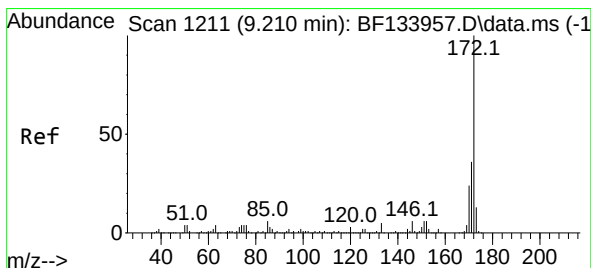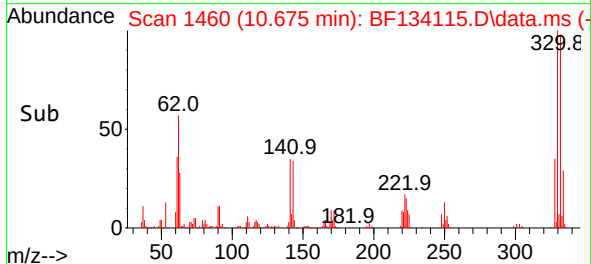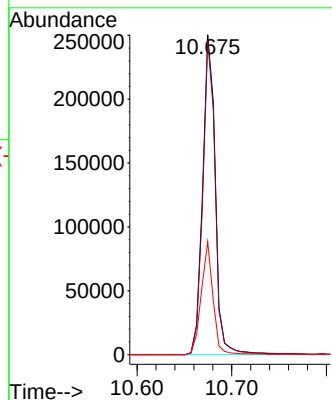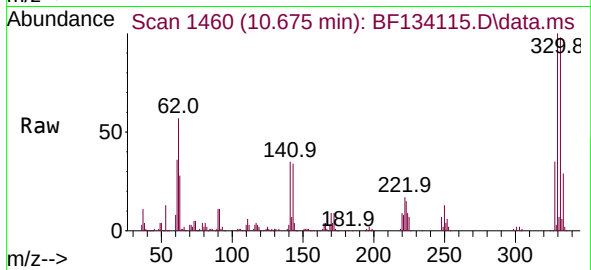

#45
2-Fluorobiphenyl
Concen: 64.056 ng
RT: 9.204 min Scan# 1210
Delta R.T. -0.006 min
Lab File: BF134115.D
Acq: 07 Jul 2023 01:21

Tgt Ion: 172 Resp: 857826
Ion Ratio Lower Upper
172 100
171 36.3 28.6 43.0
170 24.0 19.4 29.0


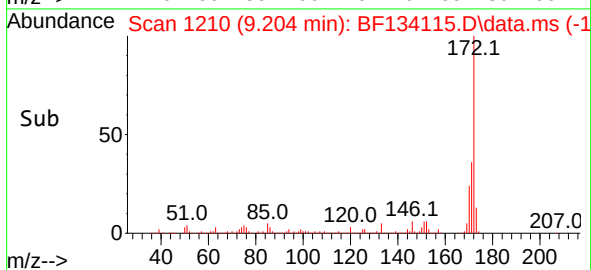
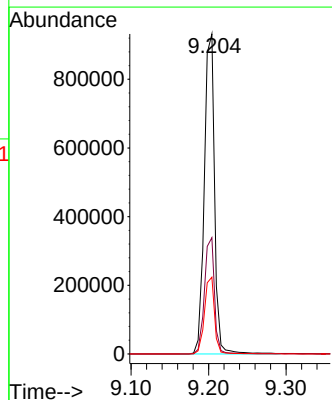
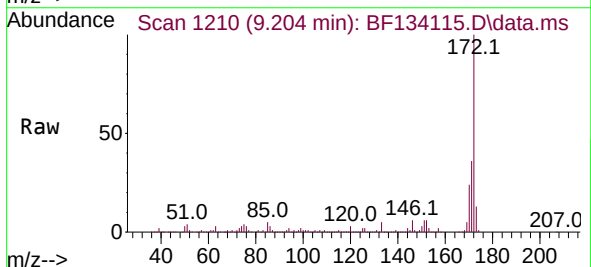


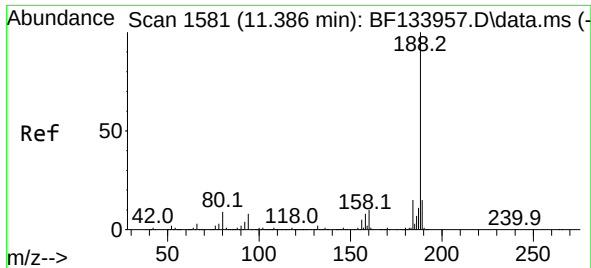

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.375 min Scan# 11
Delta R.T. -0.012 min
Lab File: BF134115.D
Acq: 07 Jul 2023 01:21




Instrument :
BNA_F
ClientSampleId :
SB-3(8-10)


Tgt Ion:188 Resp: 387501
Ion Ratio Lower Upper
188 100
94 8.0 6.4 9.6
80 9.5 7.3 10.9

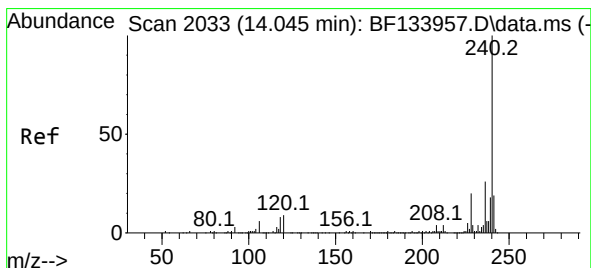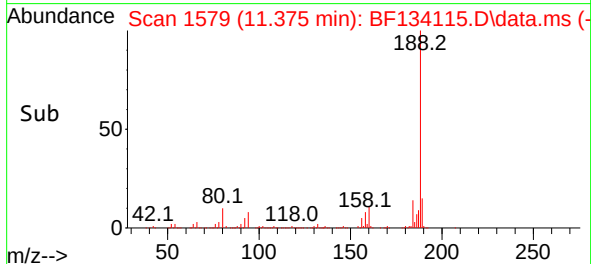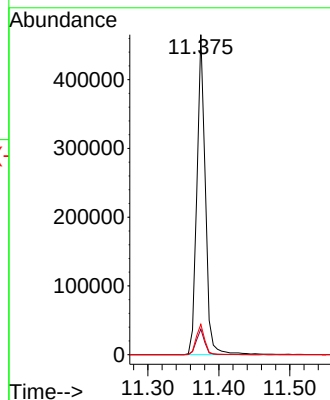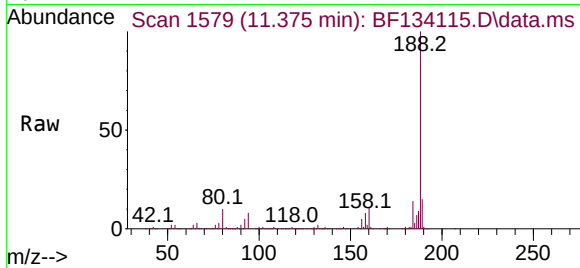

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.033 min Scan# 2031
Delta R.T. -0.018 min
Lab File: BF134115.D
Acq: 07 Jul 2023 01:21

Tgt Ion:240 Resp: 248689
Ion Ratio Lower Upper
240 100
120 10.8 7.4 11.0
236 26.6 21.0 31.6


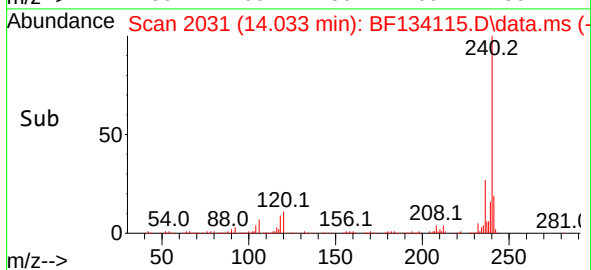
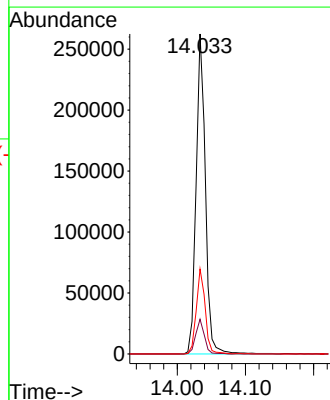
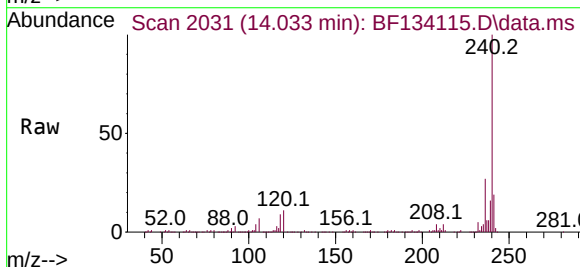


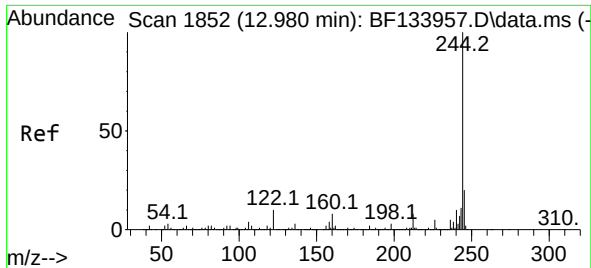

#79
 Terphenyl-d14
 Concen: 60.871 ng
 RT: 12.974 min Scan# 1851
 Delta R.T. -0.012 min
 Lab File: BF134115.D
 Acq: 07 Jul 2023 01:21

Instrument :
 BNA_F
 ClientSampleId :
 SB-3(8-10)

Tgt Ion:244 Resp: 940579
 Ion Ratio Lower Upper
 244 100
 212 7.3 6.0 9.0
 122 9.2 8.3 12.5

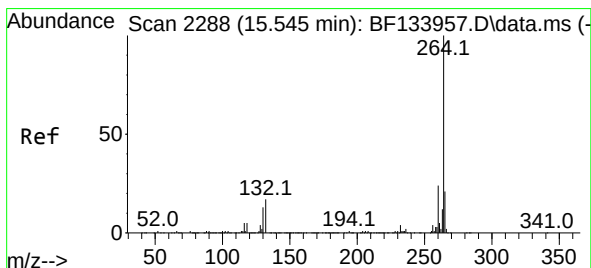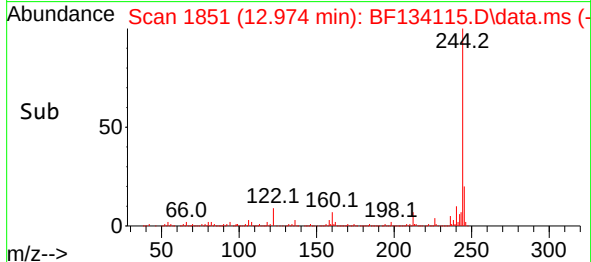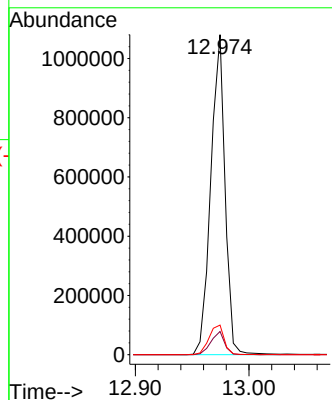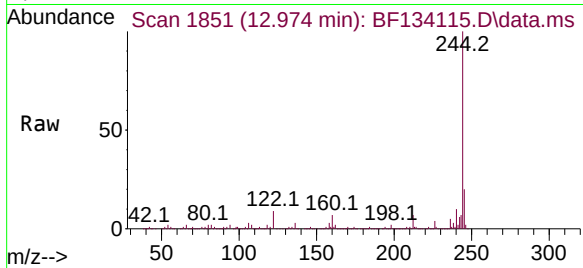

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.533 min Scan# 2286
 Delta R.T. -0.018 min
 Lab File: BF134115.D
 Acq: 07 Jul 2023 01:21

Tgt Ion:264 Resp: 207364
 Ion Ratio Lower Upper
 264 100
 260 24.2 19.5 29.3
 265 22.2 16.6 25.0

