

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
 Data File : BF134114.D
 Acq On : 07 Jul 2023 00:47
 Operator : CG\JU
 Sample : 03375-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB-5-062123

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.140	3	9	17	rVB	3257376	4435562	100.00%	25.243%
2	5.075	505	508	517	rVB	46962	49351	1.11%	0.281%
3	5.475	572	576	588	rBV	785197	803307	18.11%	4.572%
4	6.469	742	745	763	rBV	506376	496025	11.18%	2.823%
5	6.845	805	809	826	rBV	641986	580470	13.09%	3.303%
6	7.404	900	904	916	rBV	1362871	1259810	28.40%	7.170%
7	8.122	1023	1026	1044	rVB	887405	765047	17.25%	4.354%
8	9.198	1206	1209	1213	rBV	2450536	2223531	50.13%	12.654%
9	9.880	1321	1325	1338	rBV	1019807	834297	18.81%	4.748%
10	10.598	1444	1447	1452	rBV	62089	51302	1.16%	0.292%
11	10.675	1456	1460	1473	rBV	1724654	1527284	34.43%	8.692%
12	11.375	1575	1579	1589	rBV	1042460	874600	19.72%	4.977%
13	12.974	1846	1851	1854	rBV	2757649	2503178	56.43%	14.246%
14	14.033	2027	2031	2040	rVB	667109	641676	14.47%	3.652%
15	15.539	2281	2287	2299	rBV	382265	526245	11.86%	2.995%




Sum of corrected areas: 17571685

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
Data File : BF134114.D
Acq On : 07 Jul 2023 00:47
Operator : CG\JU
Sample : 03375-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-5-062123

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

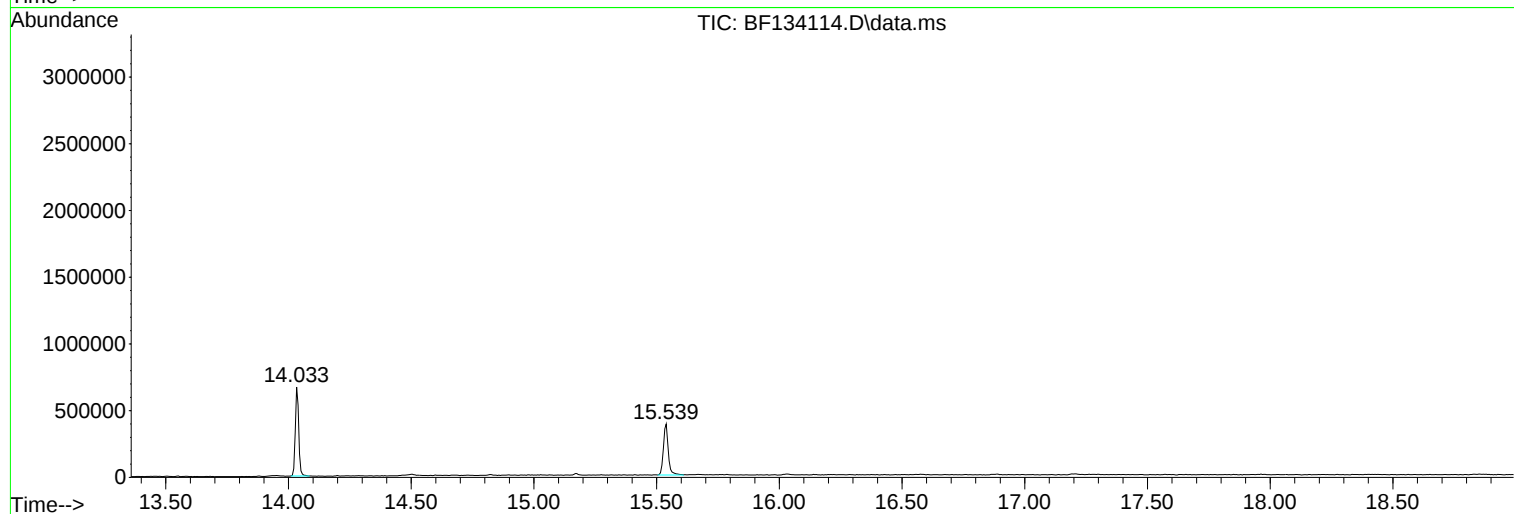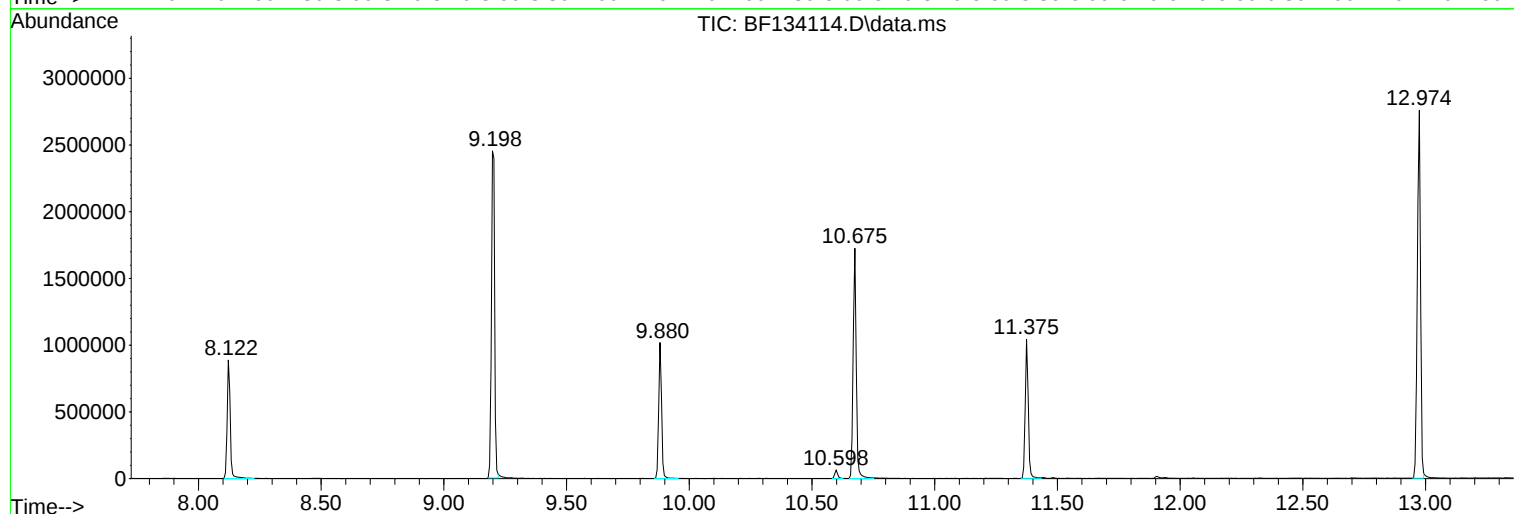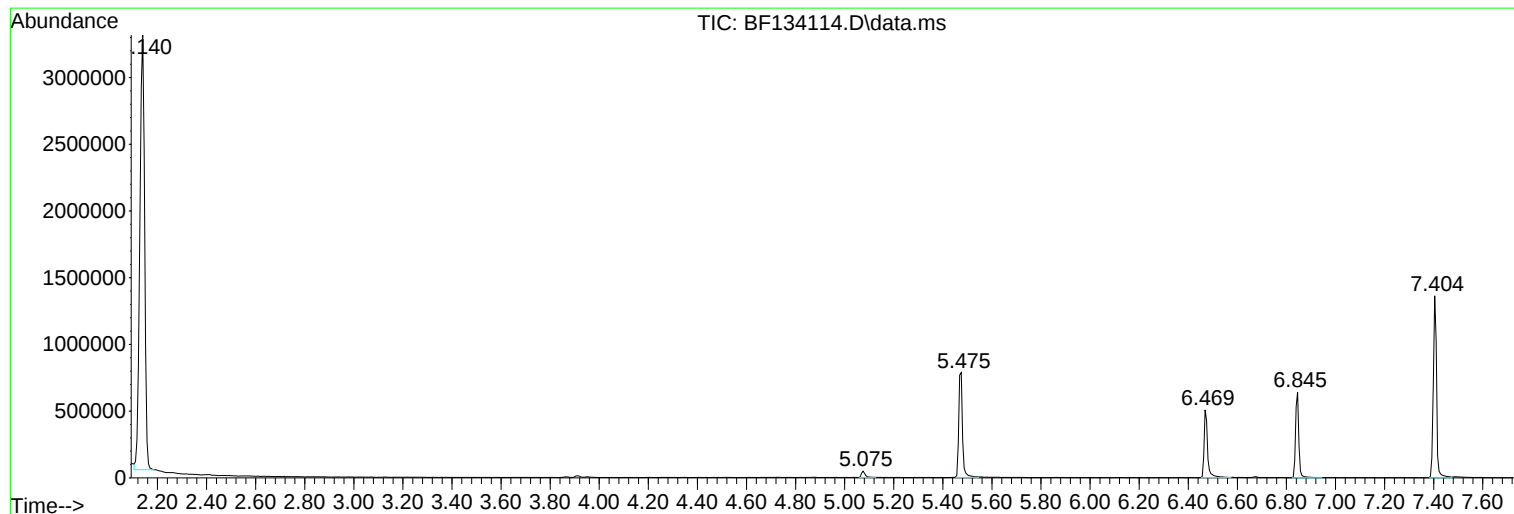

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
Data File : BF134114.D
Acq On : 07 Jul 2023 00:47
Operator : CG\JU
Sample : 03375-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-5-062123










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.140	152.83 ng	4435560	1,4-Dichlorobenzene-d4	6.845

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			Silane, tetramethyl-	88	C4H12Si	000075-76-3	38
4			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23
5			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12

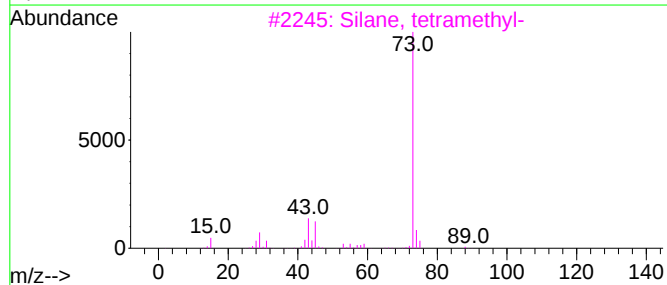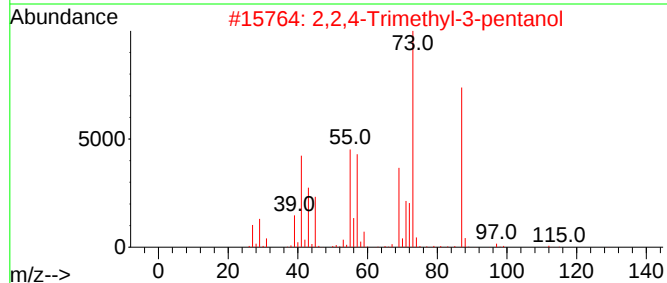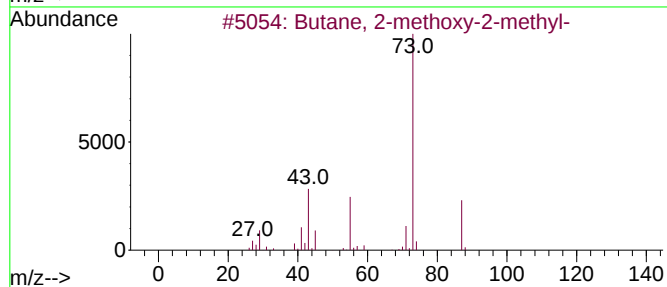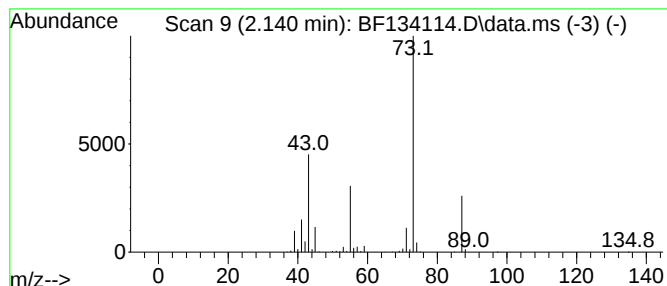

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
Data File : BF134114.D
Acq On : 07 Jul 2023 00:47
Operator : CG\JU
Sample : 03375-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-5-062123

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.140	152.8	ng	4435560	1	6.845	580470	20.0