

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
 Data File : BF134117.D
 Acq On : 07 Jul 2023 02:29
 Operator : CG\JU
 Sample : 03376-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TW-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134117.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.146	4	10	24	rVB	3673800	5139837	100.00%	21.144%
2	4.593	421	426	432	rBV	246742	280457	5.46%	1.154%
3	5.081	506	509	517	rBV	58311	68949	1.34%	0.284%
4	5.475	572	576	594	rBV	1706303	1533123	29.83%	6.307%
5	6.475	742	746	756	rBV	1074373	984358	19.15%	4.049%
6	6.845	805	809	822	rBV	736219	636979	12.39%	2.620%
7	7.410	900	905	908	rBV	2231312	1987613	38.67%	8.177%
8	8.122	1022	1026	1038	rBV	988374	822533	16.00%	3.384%
9	9.204	1205	1210	1213	rBV	4006024	3425764	66.65%	14.093%
10	9.880	1321	1325	1334	rBV	1112287	905288	17.61%	3.724%
11	10.598	1444	1447	1456	rBV	85371	79144	1.54%	0.326%
12	10.674	1456	1460	1473	rBV	2521892	2475594	48.16%	10.184%
13	11.374	1575	1579	1587	rBV	1087803	950729	18.50%	3.911%
14	12.974	1846	1851	1855	rBV	3811970	3725383	72.48%	15.326%
15	14.033	2027	2031	2040	rVB	743415	713530	13.88%	2.935%
16	15.539	2282	2287	2299	rBV	418624	579003	11.27%	2.382%




Sum of corrected areas: 24308284

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
Data File : BF134117.D
Acq On : 07 Jul 2023 02:29
Operator : CG\JU
Sample : 03376-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

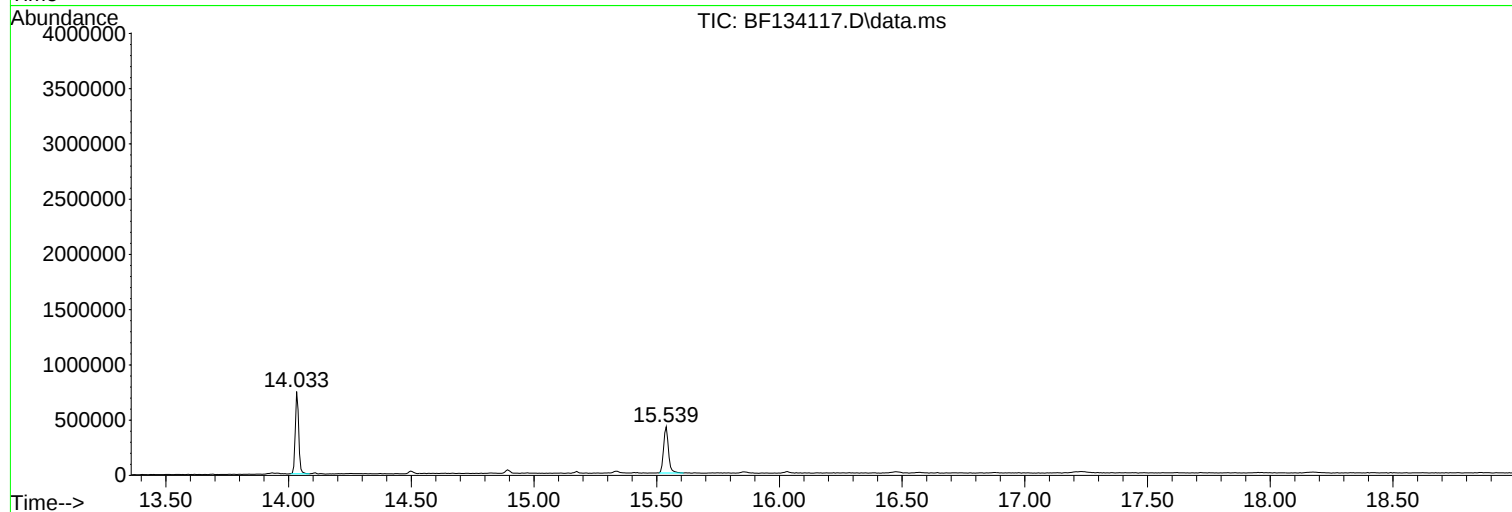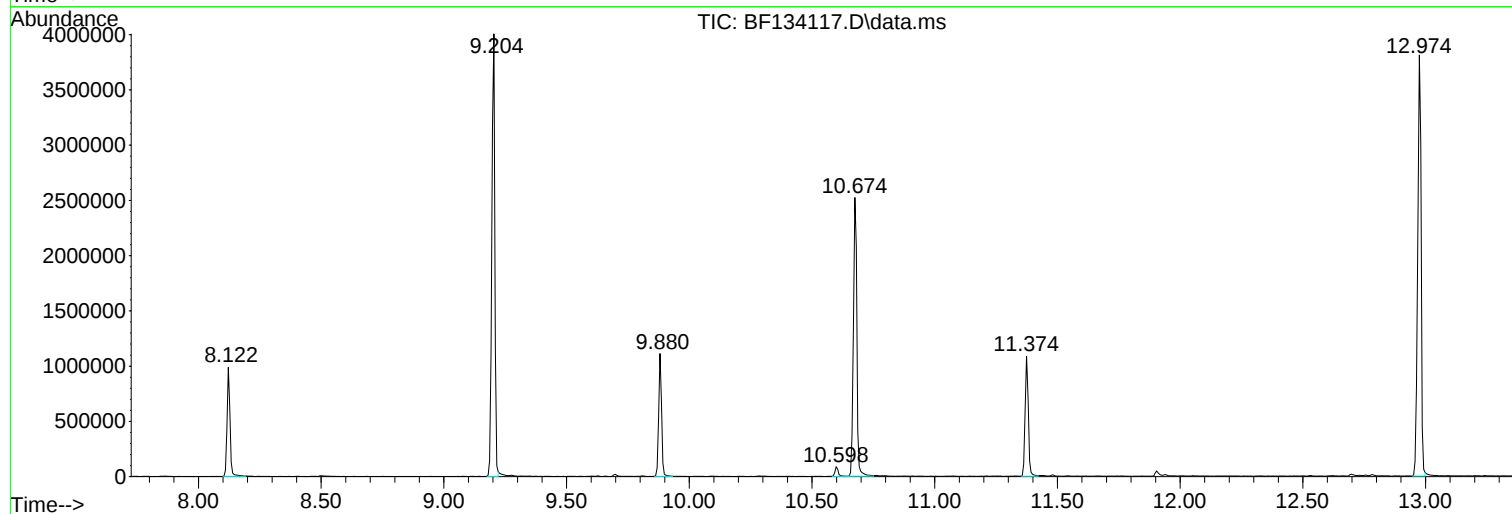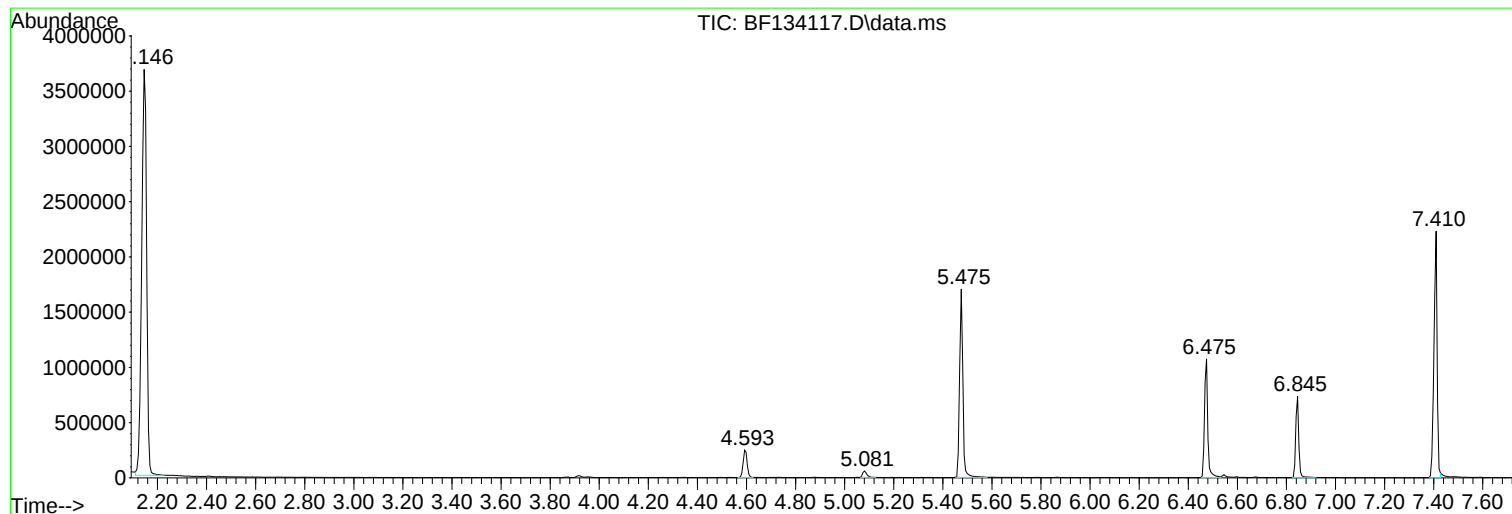

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
Data File : BF134117.D
Acq On : 07 Jul 2023 02:29
Operator : CG\JU
Sample : 03376-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.146	161.38 ng	5139840	1,4-Dichlorobenzene-d4	6.845

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

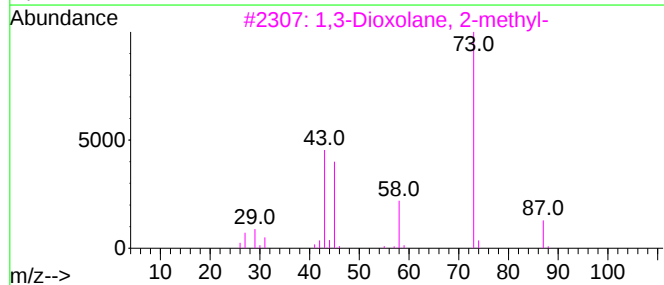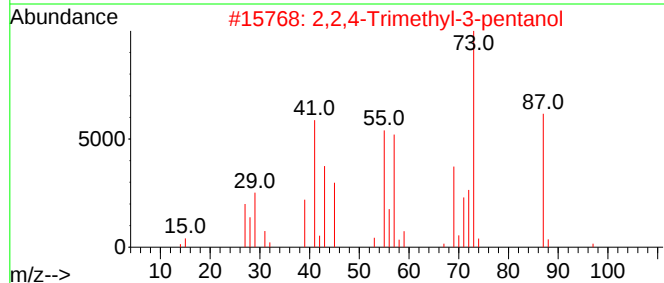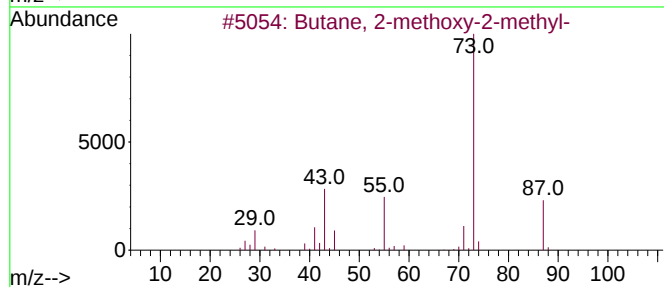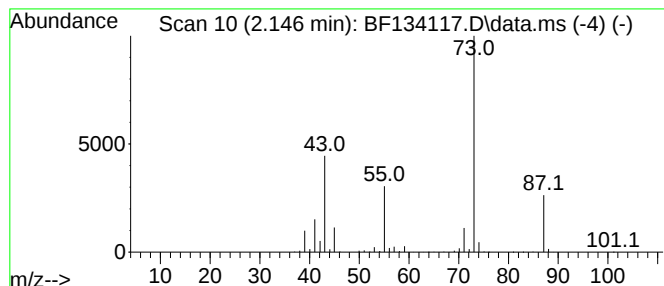

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
Data File : BF134117.D
Acq On : 07 Jul 2023 02:29
Operator : CG\JU
Sample : 03376-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-1










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.081	2.16 ng	68949	1,4-Dichlorobenzene-d4	6.845

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	3-Hydroxy-3-methyl-2-butanone	102	C5H10O2	000115-22-0	23		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	Diacetamide	101	C4H7NO2	000625-77-4	9		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		

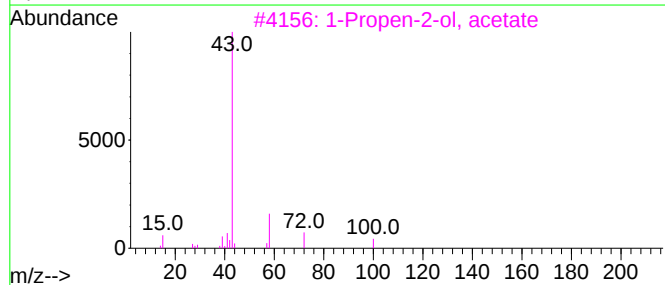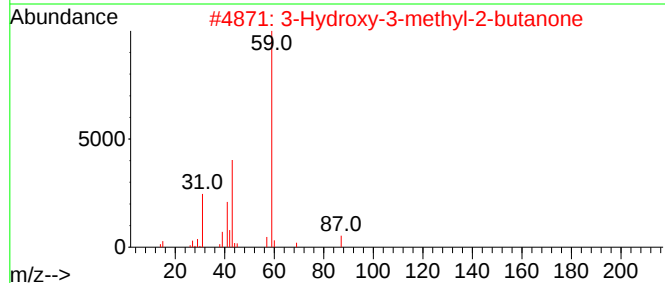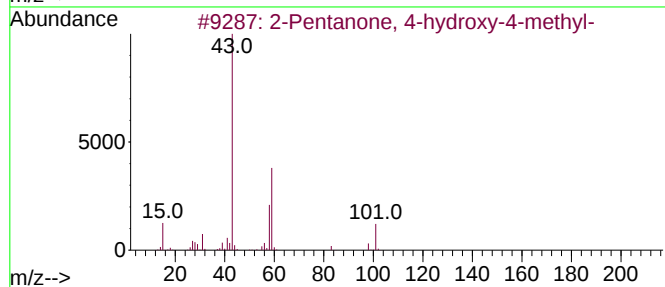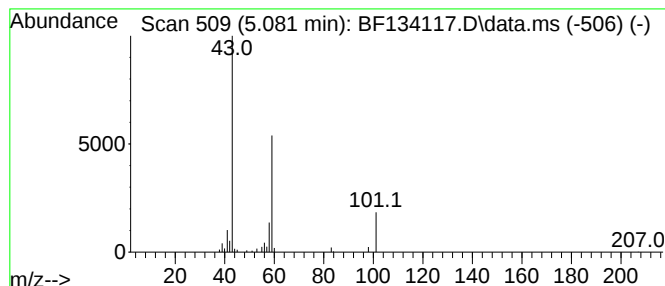

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
Data File : BF134117.D
Acq On : 07 Jul 2023 02:29
Operator : CG\JU
Sample : 03376-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.146	161.4	ng	5139840	1	6.845	636979	20.0
2-Pentanone, 4-...	5.081	2.2	ng	68949	1	6.845	636979	20.0