


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
Data File : BF134121.D
Acq On : 07 Jul 2023 05:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 30 18:35:29 2023

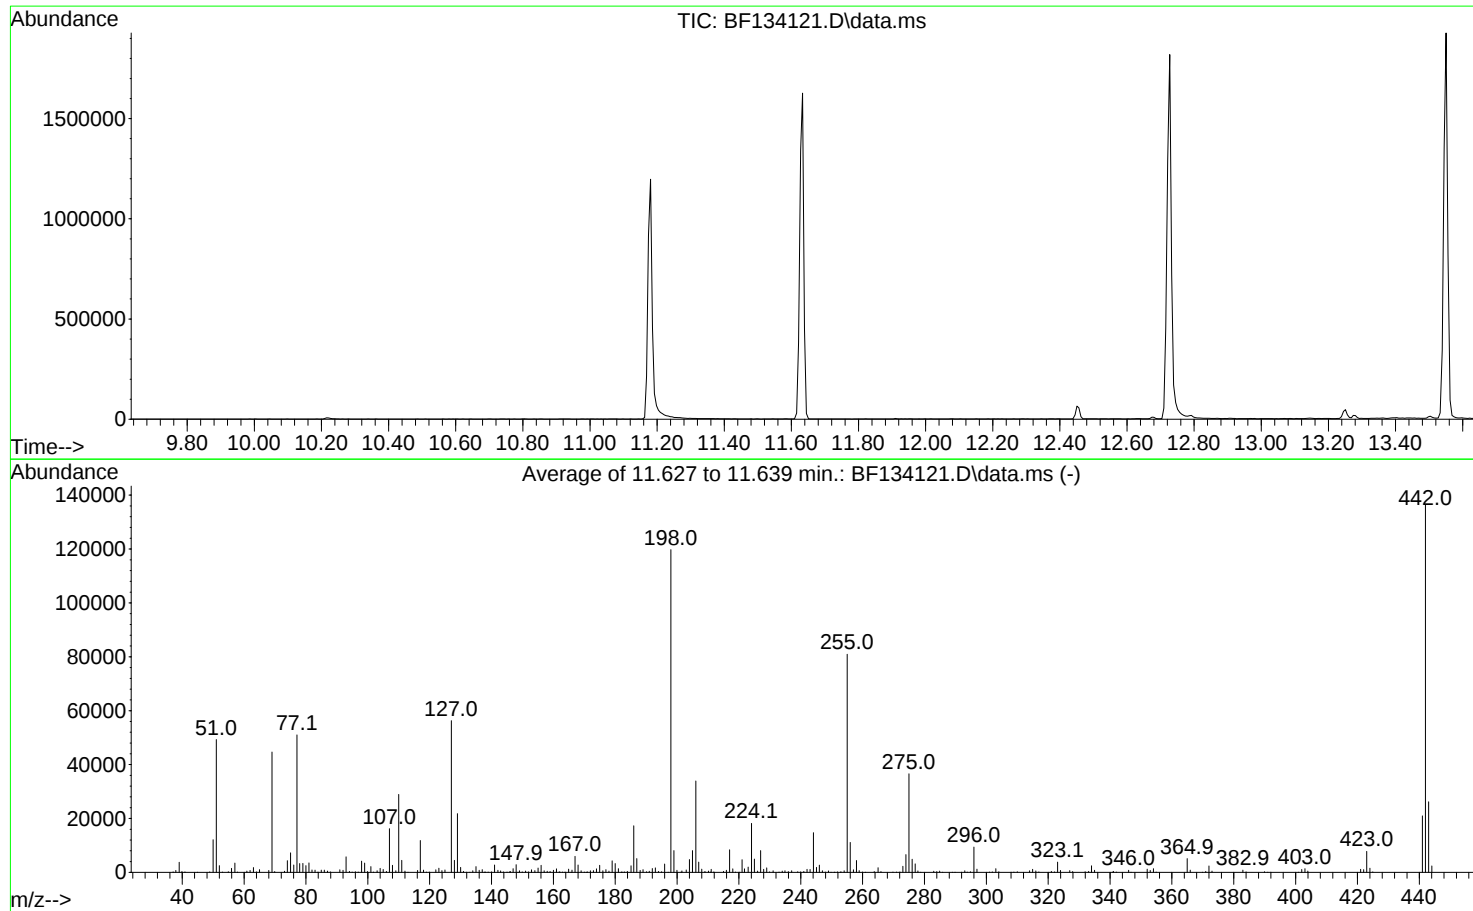




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	49268	PASS
68	69	0.00	2	1.6	720	PASS
69	198	0.00	100	37.3	44635	PASS
70	69	0.00	2	0.6	287	PASS
127	198	10	80	47.0	56290	PASS
197	198	0.00	2	0.1	91	PASS
198	198	100	100	100.0	119784	PASS
199	198	5	9	6.8	8107	PASS
275	198	10	60	30.5	36582	PASS
365	198	1	100	4.2	5080	PASS
441	198	0.01	100	17.5	20999	PASS
442	442	50	100	100.0	136525	PASS
443	442	15	24	19.2	26184	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
Data File : BF134121.D
Acq On : 07 Jul 2023 05:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 07 05:42:14 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

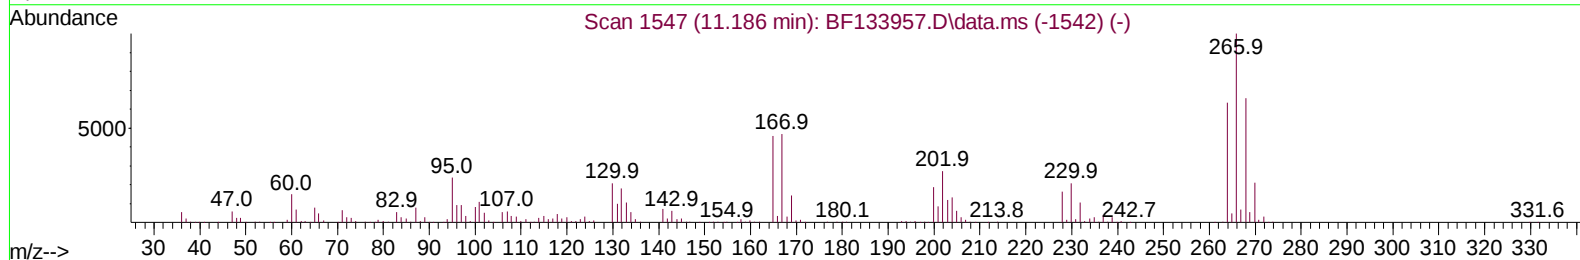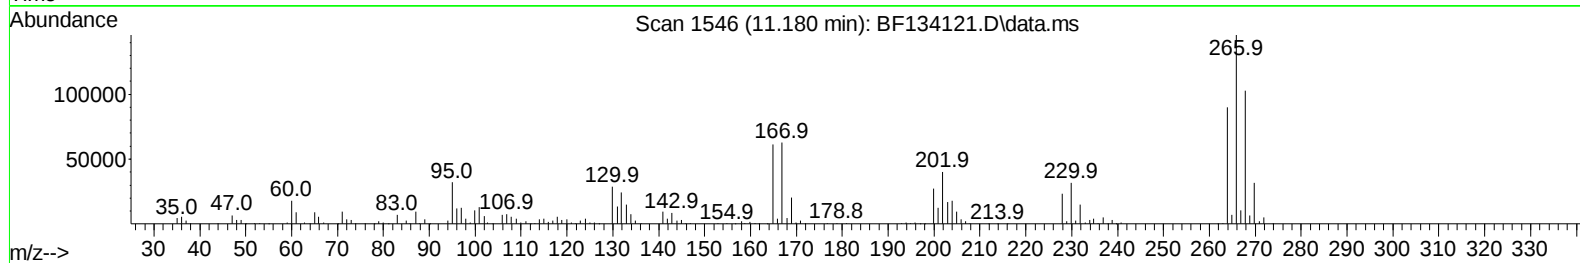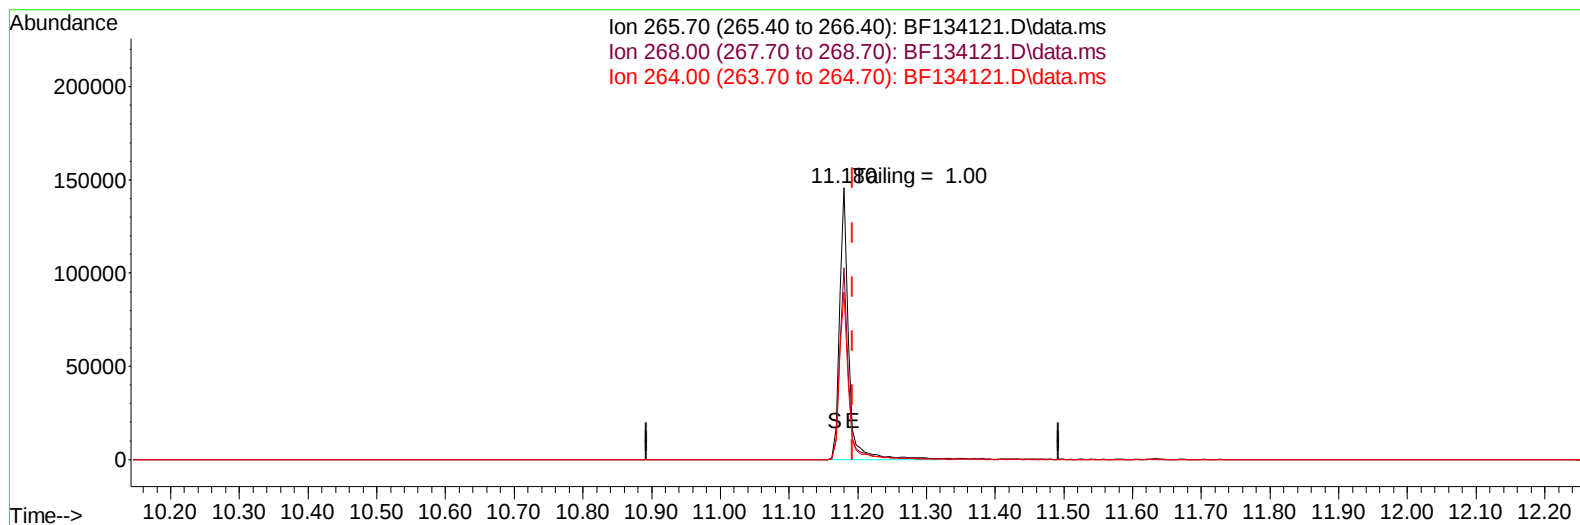

TIC: BF134121.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.012) 149903.62 ng




response 129472

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	70.51
264.00	63.30	61.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070623\
 Data File : BF134121.D
 Acq On : 07 Jul 2023 05:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 07 05:42:14 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 30 18:35:29 2023
 Response via : Initial Calibration

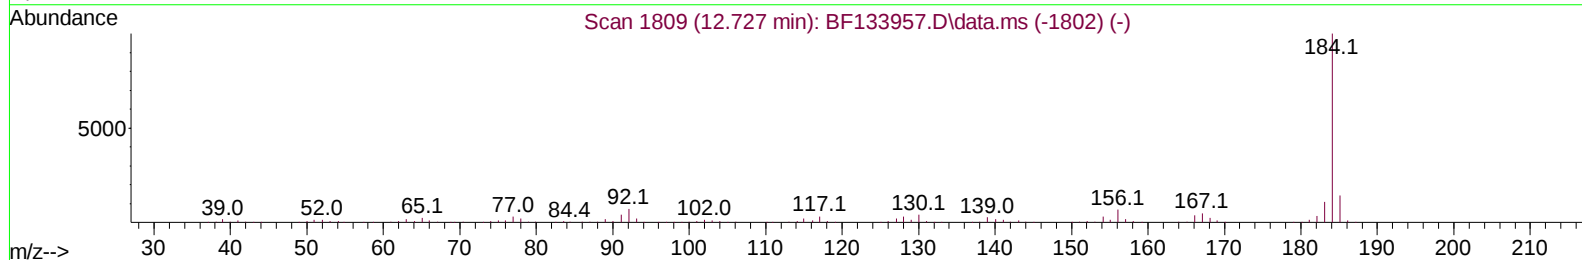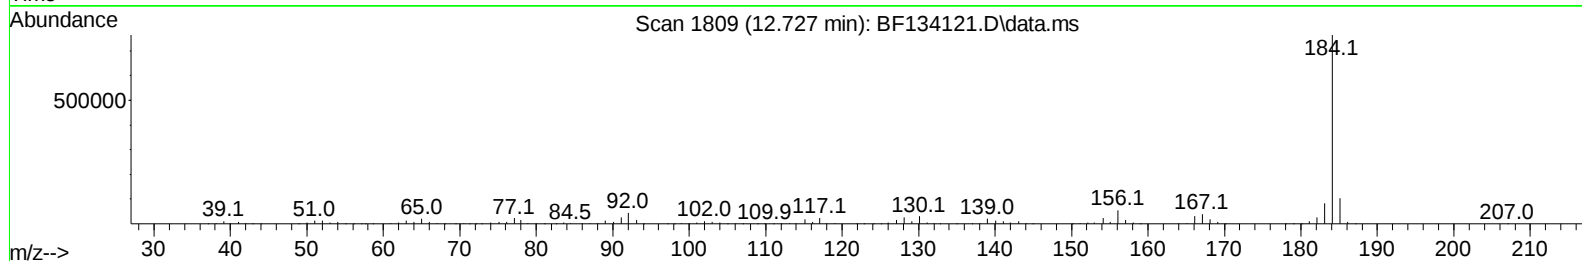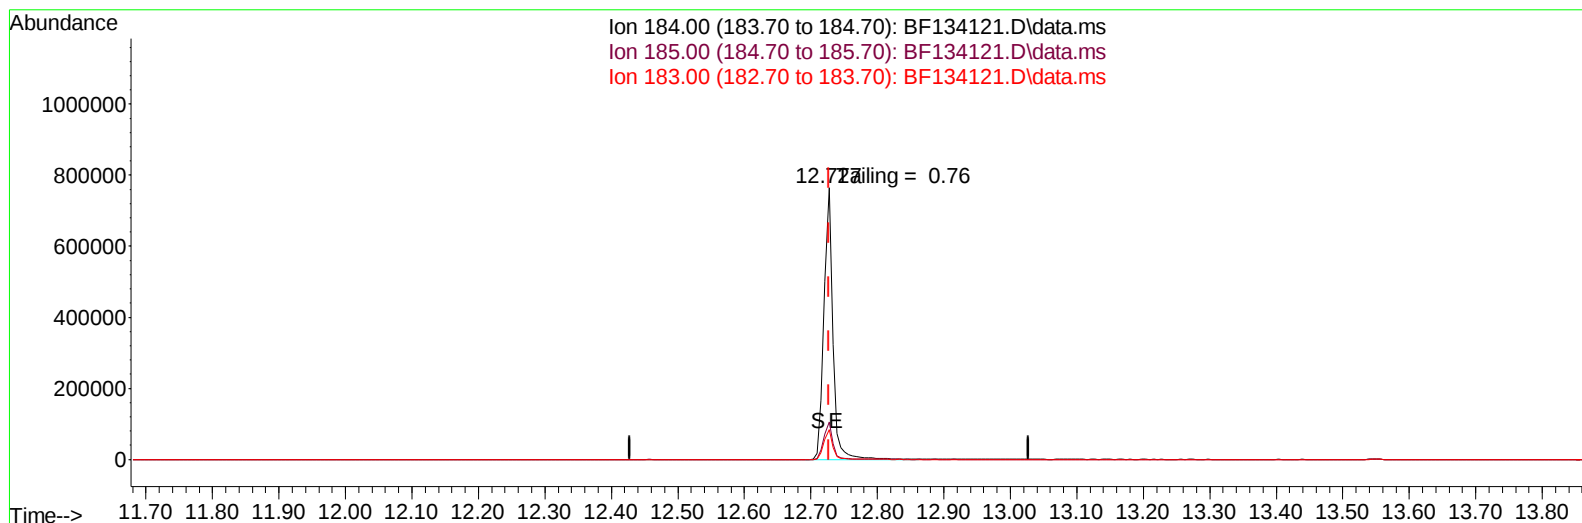

TIC: BF134121.D\data.ms

(77) Benzidine

12.727min (-0.000) 232610.69 ng

response 697387

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.74
183.00	11.00	10.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/6/2023	BNA_F	<u>BF134121.D</u>
Compound Name	Response	Retention Time
DDT	317678	13.551
DDD	12110	13.251
DDE	399	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12509	330187	3.79

Instrument :
BNA_F
ClientSampleId :
DFTPP