

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070718\
 Data File : BF107200.D
 Acq On : 7 Jul 2018 12:30
 Operator : JU/SJ
 Sample : J3791-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ZER-SB-03-11-72

Quant Time: Jul 09 02:11:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 29 14:38:29 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	59333	20.00	ng	-0.02
21) Naphthalene-d8	8.22	136	235177	20.00	ng	-0.02
38) Acenaphthene-d10	9.98	164	121530	20.00	ng	-0.02
63) Phenanthrene-d10	11.48	188	241484	20.00	ng	-0.02
75) Chrysene-d12	14.13	240	174733	20.00	ng	-0.04
86) Perylene-d12	15.67	264	172167	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.59	112	344902	98.43	ng	-0.01
7) Phenol-d6	6.59	99	436385	99.73	ng	-0.02
23) Nitrobenzene-d5	7.51	82	273669	64.67	ng	-0.02
41) 2,4,6-Tribromophenol	10.78	330	149086	105.84	ng	-0.02
44) 2-Fluorobiphenyl	9.30	172	476695	62.49	ng	-0.02
78) Terphenyl-d14	13.07	244	537014	74.45	ng	-0.02
Target Compounds						
9) Benzaldehyde	6.72	77	7452	2.033	ng	89
19) n-Nitroso-di-n-propylamine	7.51	70	35443	12.288	ng	# 72
25) Isophorone	7.51	82	273704	36.704	ng	# 64
49) Dimethylphthalate	9.70	163	93965	10.309	ng	# 98
56) 2,4-Dinitrotoluene	9.98	165	15497	6.151	ng	# 21
66) 4-Bromophenyl-phenylether	10.78	248	9109	3.161	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070718\
Data File : BF107200.D
Acq On : 7 Jul 2018 12:30
Operator : JU/SJ
Sample : J3791-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ZER-SB-03-11-72

Quant Time: Jul 09 02:11:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

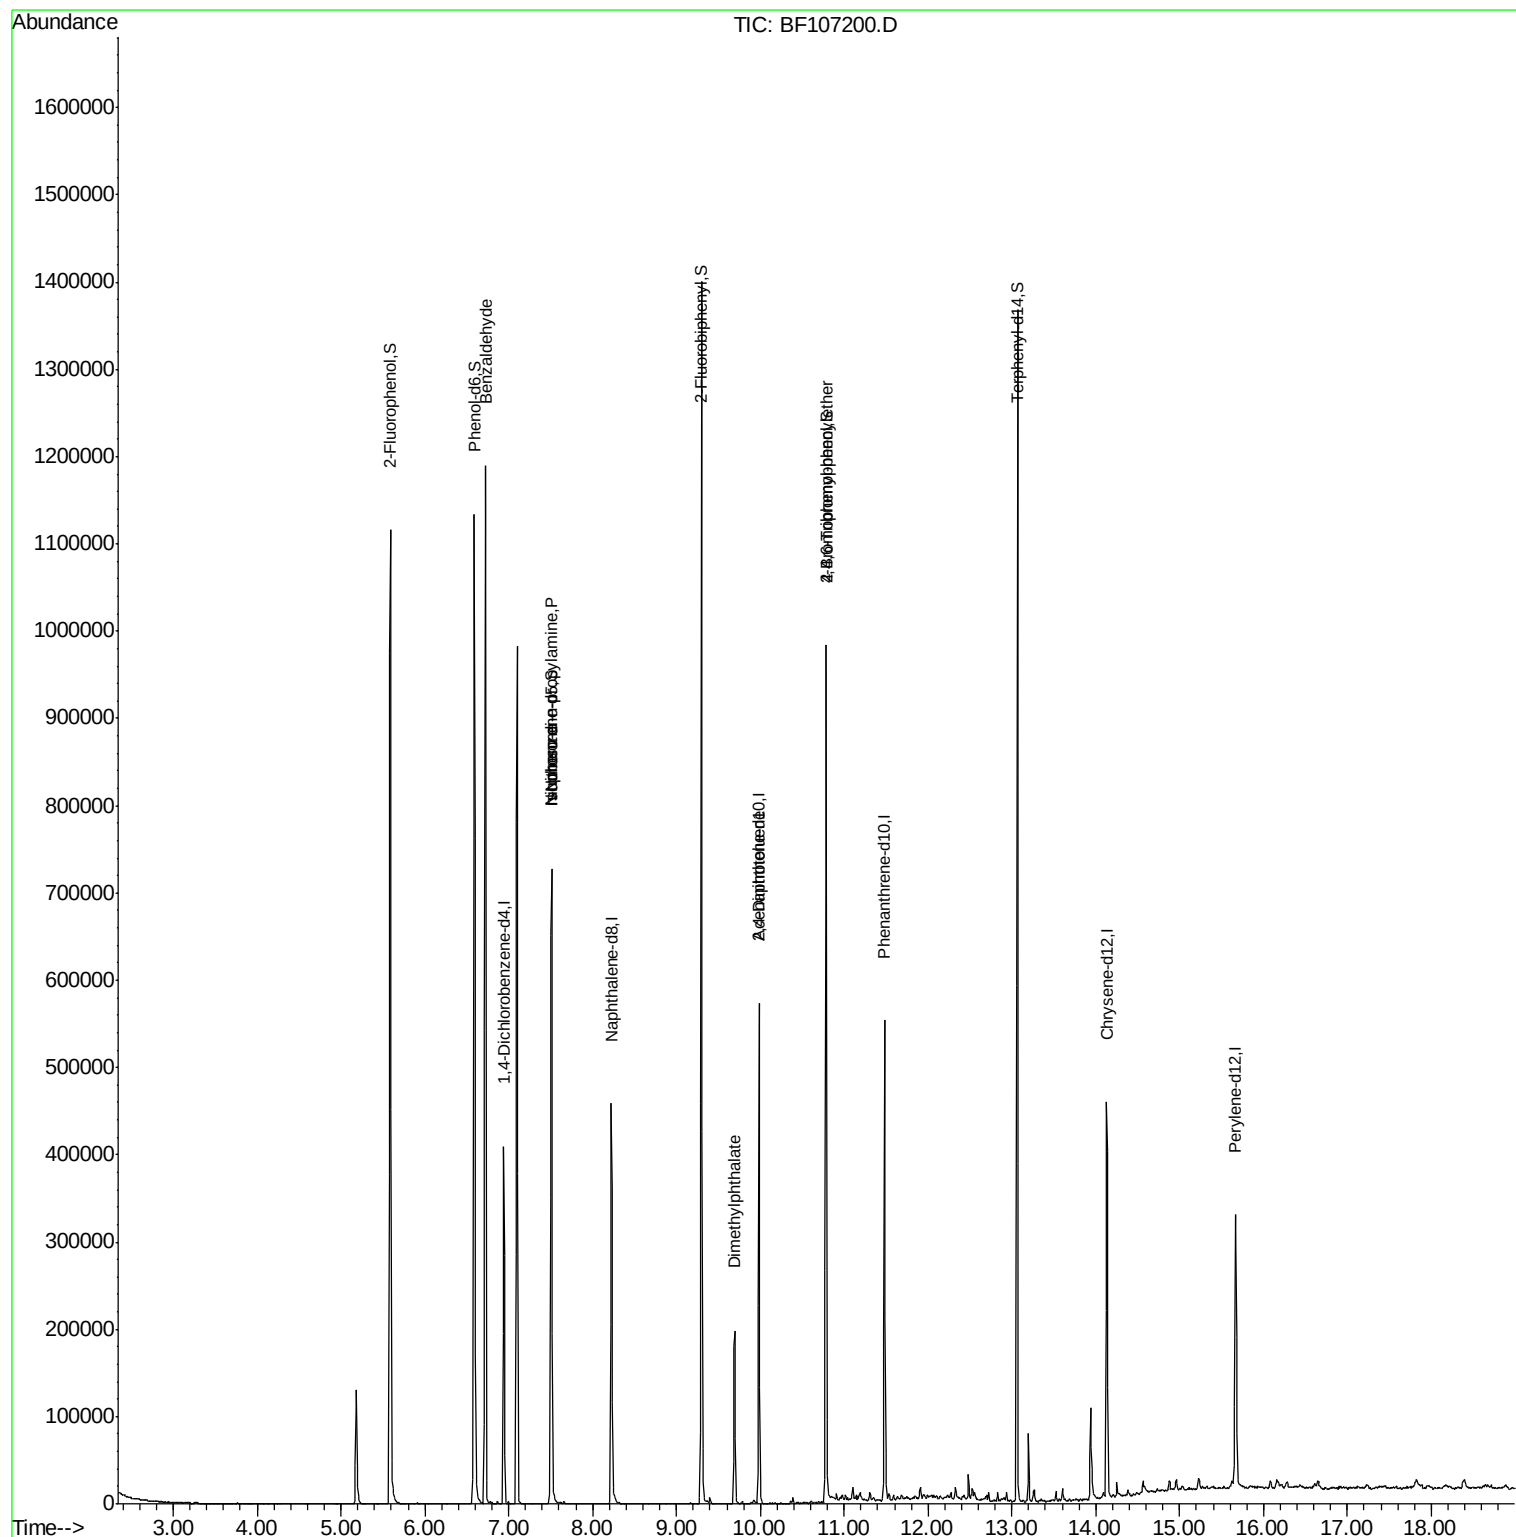

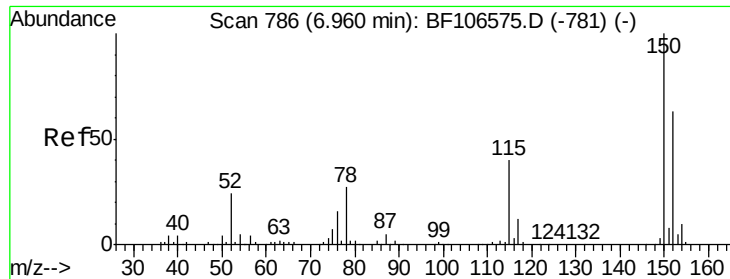


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.94 min Scan# 783
Delta R.T. -0.02 min
Lab File: BF107200.D
Acq: 7 Jul 2018 12:30

Instrument :
BNA_F
ClientSampleId :
ZER-SB-03-11-72

Tgt Ion:152 Resp: 59333
Ion Ratio Lower Upper
152 100
150 159.3 124.6 186.8
115 62.4 50.1 75.1

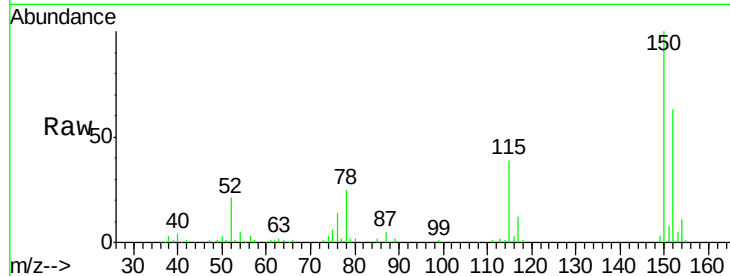


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

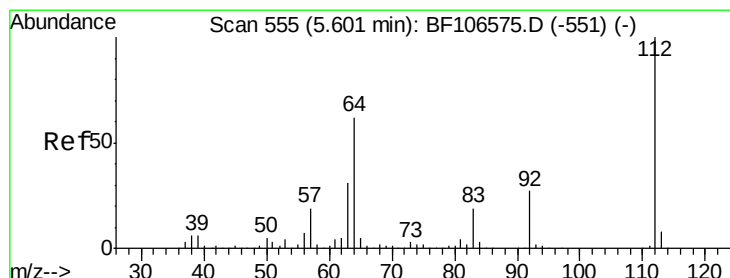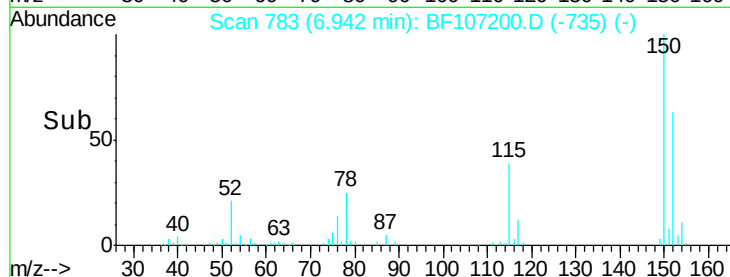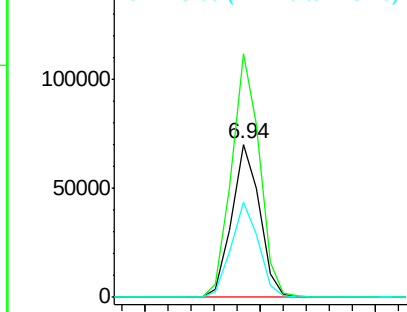



#5


2-Fluorophenol
Concen: 98.432 ng
RT: 5.59 min Scan# 553
Delta R.T. -0.01 min
Lab File: BF107200.D
Acq: 7 Jul 2018 12:30

Tgt Ion:112 Resp: 344902
Ion Ratio Lower Upper
112 100
64 56.8 47.9 71.9
63 28.0 23.7 35.5

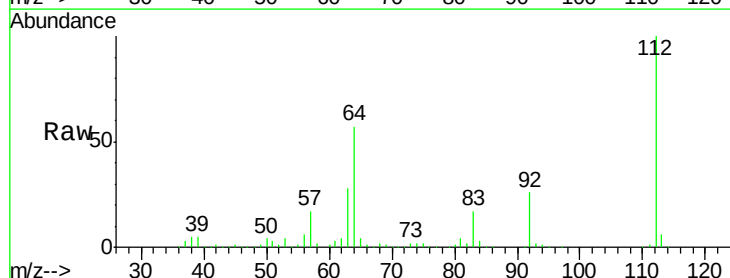

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

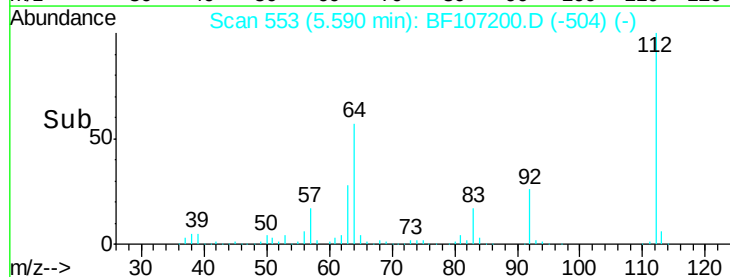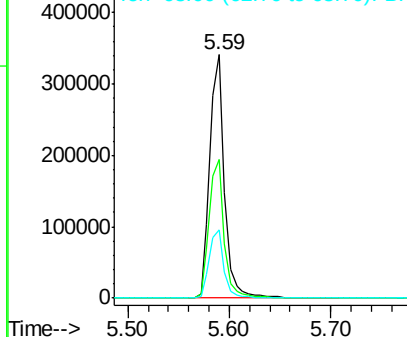

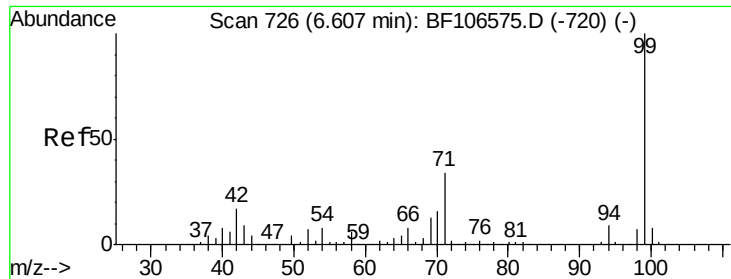

#7

Phenol-d6

Concen: 99.728 ng

RT: 6.59 min Scan# 723

Delta R.T. -0.02 min

Lab File: BF107200.D

Acq: 7 Jul 2018 12:30

Instrument :

BNA_F

ClientSampleId :

ZER-SB-03-11-72


Tgt Ion: 99 Resp: 436385

Ion Ratio Lower Upper

99 100

42 15.9 14.5 21.7




71 33.1 25.4 38.0

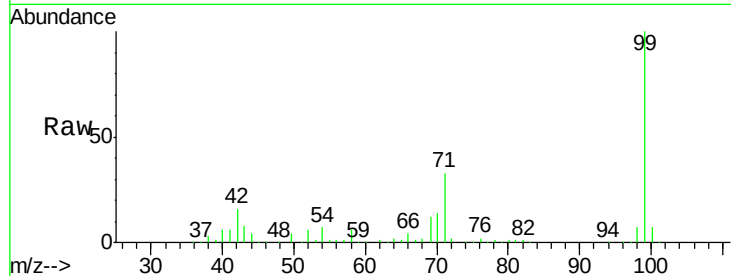

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

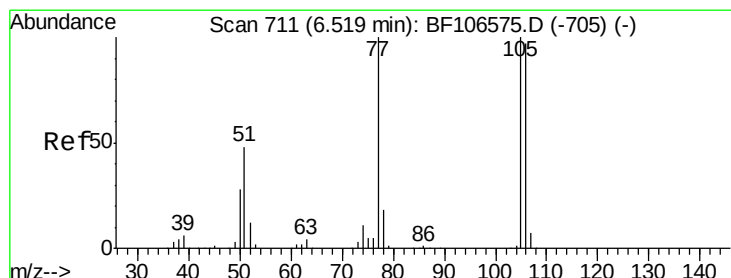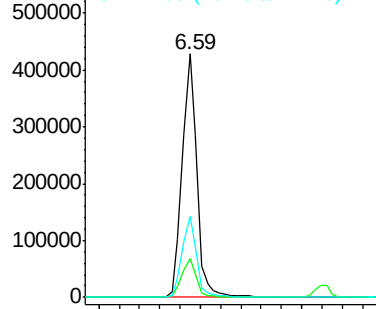

#9

Benzaldehyde

Concen: 2.033 ng

RT: 6.72 min Scan# 746

Delta R.T. 0.21 min

Lab File: BF107200.D

Acq: 7 Jul 2018 12:30


Tgt Ion: 77 Resp: 7452

Ion Ratio Lower Upper

77 100

105 92.3 81.1 121.1



106 82.2 74.5 114.5



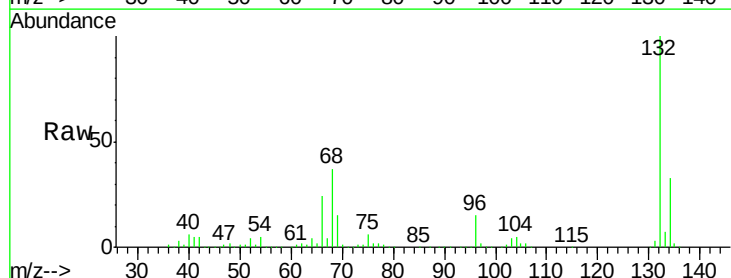


Abundance Ion 77.00 (76.70 to 77.70): BF1

Ion 105.00 (104.70 to 105.70): BF1

Ion 106.00 (105.70 to 106.70): BF1




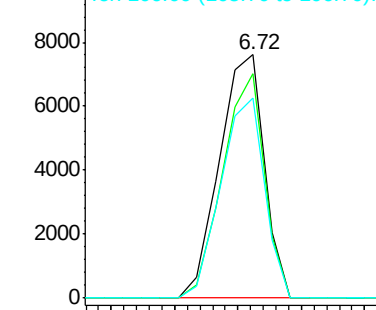


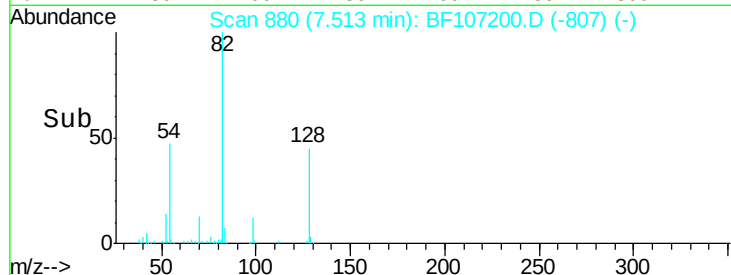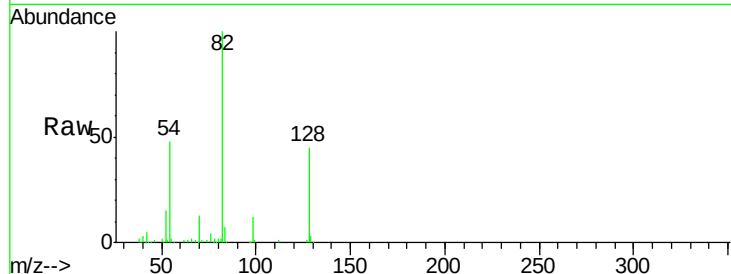

#19
n-Nitroso-di-n-propylamine
Concen: 12.288 ng
RT: 7.51 min Scan# 880
Delta R.T. 0.13 min
Lab File: BF107200.D
Acq: 7 Jul 2018 12:30


Instrument :
BNA_F
ClientSampleId :
ZER-SB-03-11-72


Tgt Ion: 70 Resp: 35443
Ion Ratio Lower Upper
70 100
42 41.2 47.5 71.3#
101 0.0 7.4 11.2#
130 2.0 16.6 25.0#

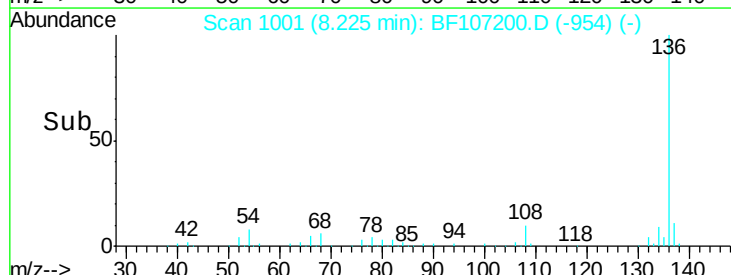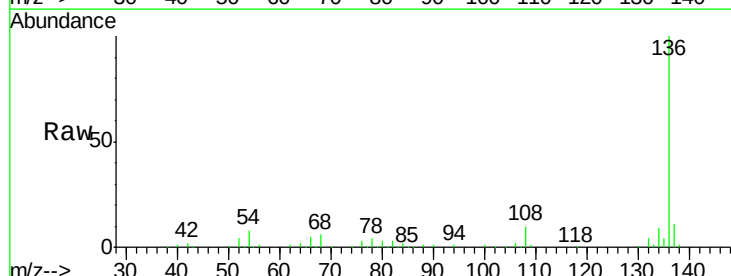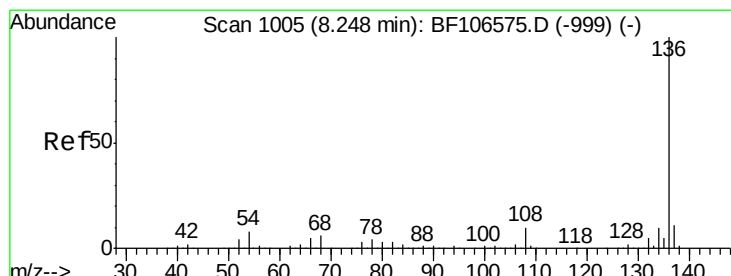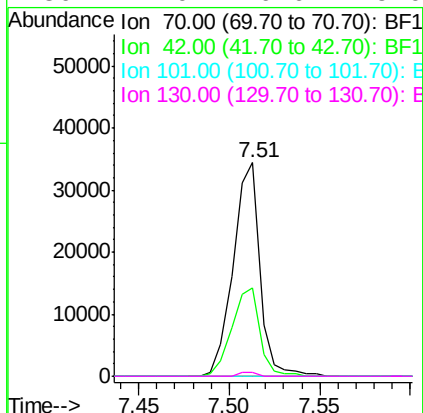

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.22 min Scan# 1001
Delta R.T. -0.02 min
Lab File: BF107200.D
Acq: 7 Jul 2018 12:30

Tgt Ion: 136 Resp: 235177
Ion Ratio Lower Upper
136 100
137 10.9 8.9 13.3
54 8.4 6.6 9.8
68 6.3 5.0 7.4




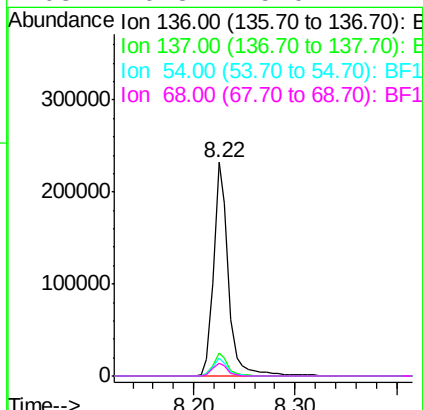




#23
 Nitrobenzene-d5
 Concen: 64.669 ng
 RT: 7.51 min Scan# 880
 Delta R.T. -0.02 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30




Instrument :
 BNA_F
 ClientSampleId :
 ZER-SB-03-11-72


Tgt Ion: 82 Resp: 273669
 Ion Ratio Lower Upper
 82 100
 128 45.4 36.1 54.1
 54 47.6 41.4 62.2

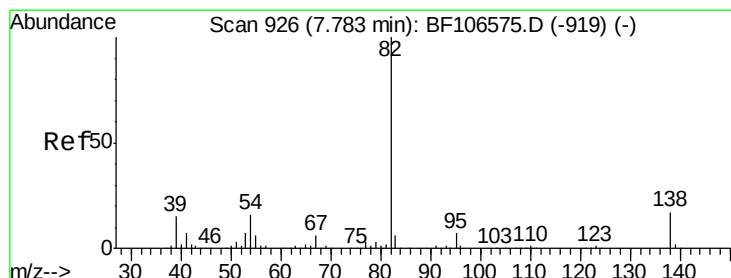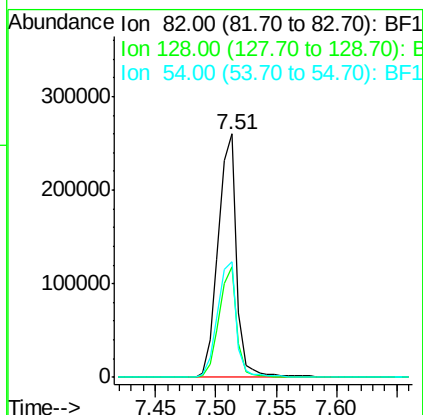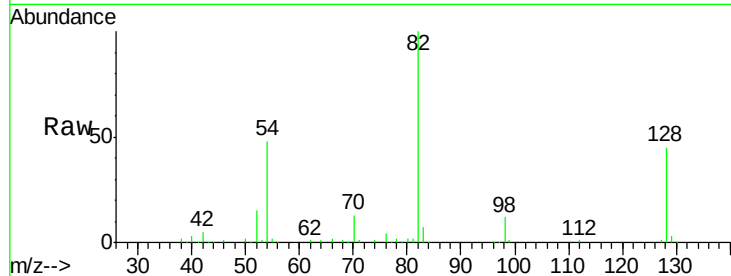

#25
 Isophorone
 Concen: 36.704 ng
 RT: 7.51 min Scan# 880
 Delta R.T. -0.28 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30

Tgt Ion: 82 Resp: 273704
 Ion Ratio Lower Upper
 82 100
 95 0.0 5.2 7.8#
 138 0.0 14.9 22.3#

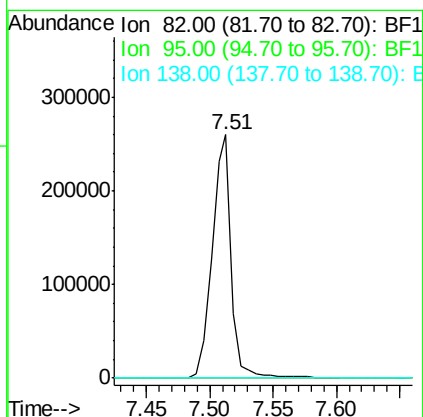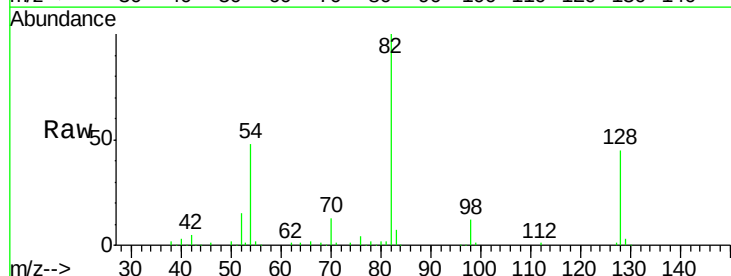


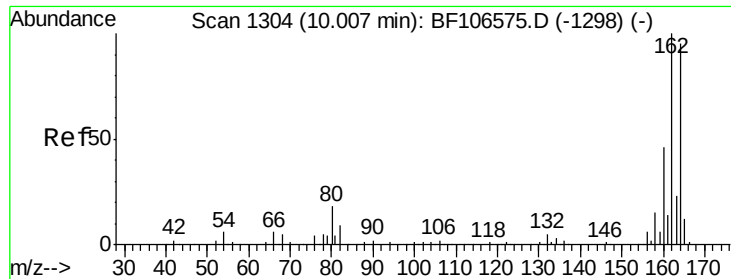




#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.98 min Scan# 1300
 Delta R.T. -0.02 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30

Instrument :
 BNA_F
 ClientSampleId :
 ZER-SB-03-11-72

Tgt Ion:164 Resp: 121530
 Ion Ratio Lower Upper
 164 100
 162 95.2 86.1 129.1
 160 42.3 38.3 57.5

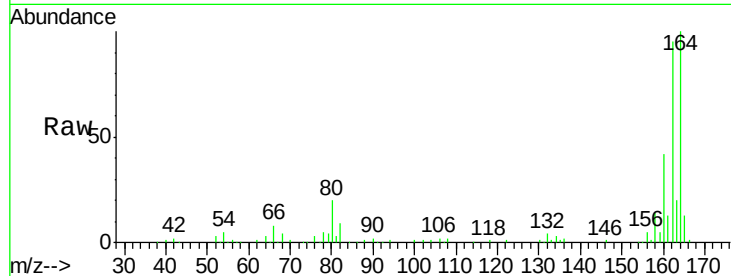


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

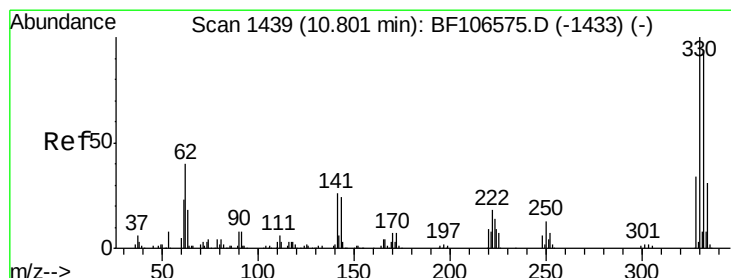
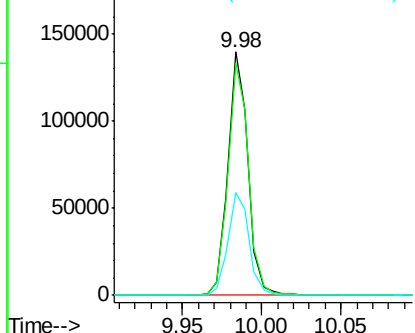



#41
 2,4,6-Tribromophenol
 Concen: 105.842 ng
 RT: 10.78 min Scan# 1436
 Delta R.T. -0.02 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30

Tgt Ion:330 Resp: 149086
 Ion Ratio Lower Upper
 330 100
 332 97.4 77.0 115.6
 141 22.7 29.9 44.9#

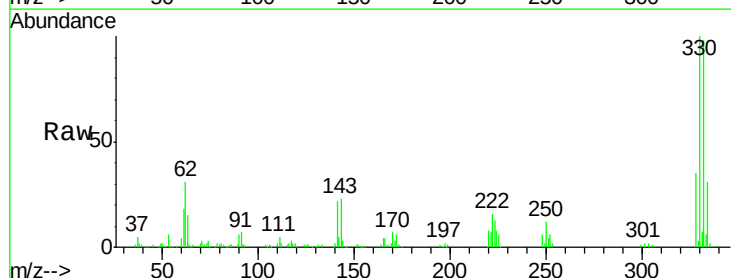

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E




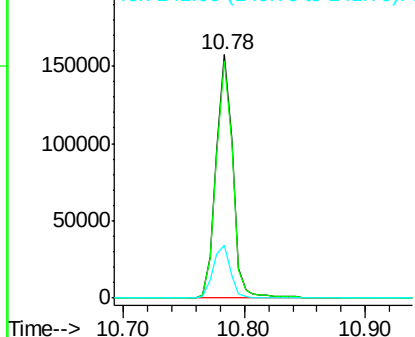


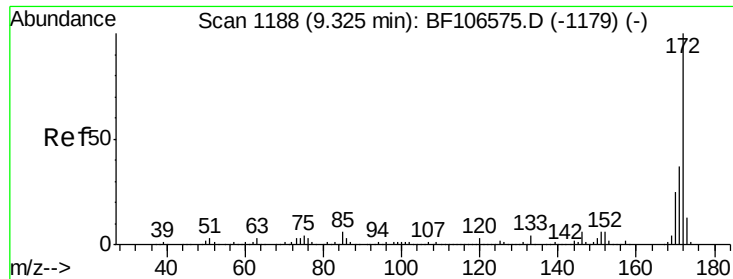

#44
 2-Fluorobiphenyl
 Concen: 62.485 ng
 RT: 9.30 min Scan# 1184
 Delta R.T. -0.02 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30




Instrument :
 BNA_F
 ClientSampleId :
 ZER-SB-03-11-72


Tgt Ion:172 Resp: 476695
 Ion Ratio Lower Upper
 172 100
 171 36.1 29.7 44.5
 170 24.3 19.6 29.4

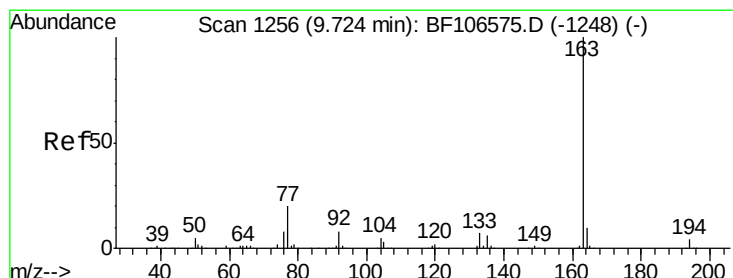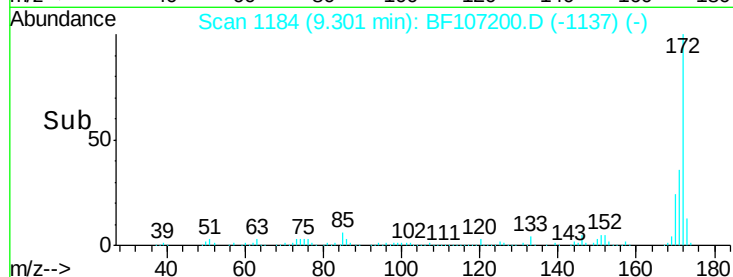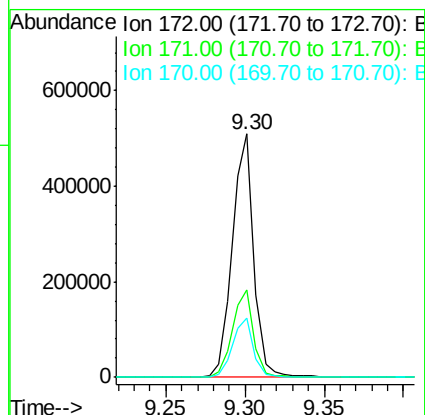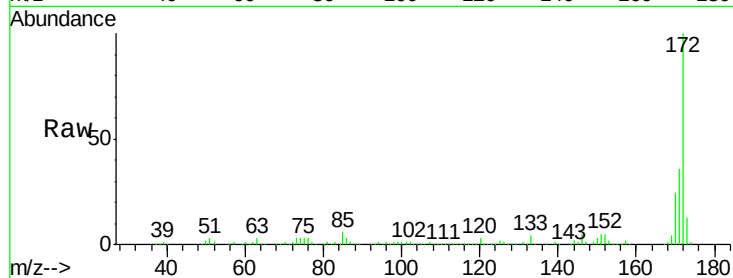

#49
 Dimethylphthalate
 Concen: 10.309 ng
 RT: 9.70 min Scan# 1251
 Delta R.T. -0.03 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30

Tgt Ion:163 Resp: 93965
 Ion Ratio Lower Upper
 163 100
 194 4.2 2.7 4.1#
 164 10.6 8.2 12.2


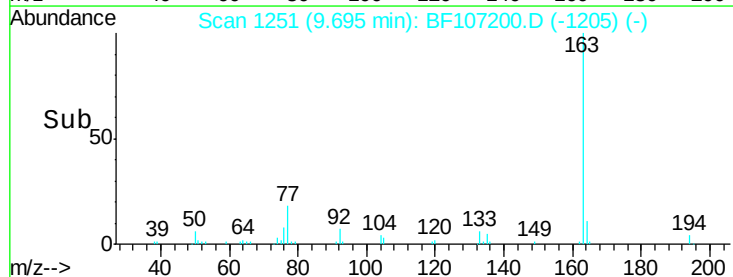
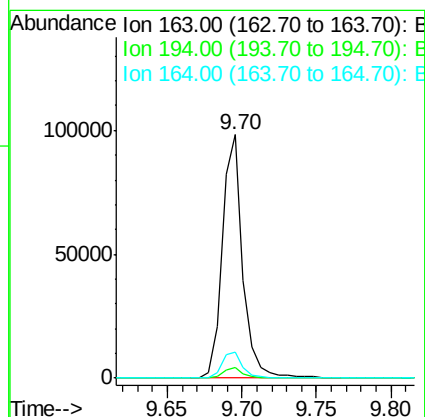
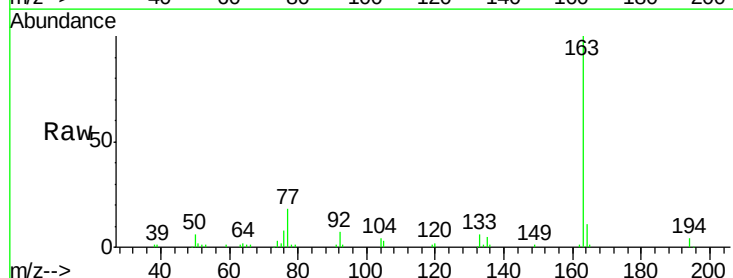


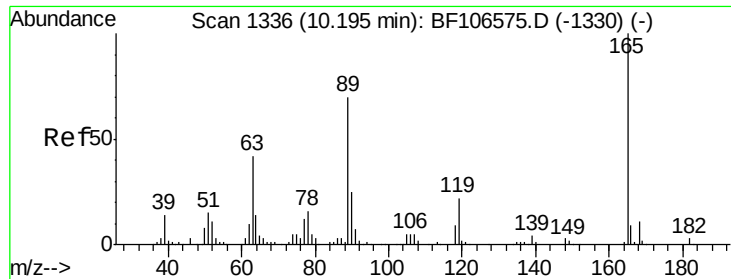

#56
 2,4-Dinitrotoluene
 Concen: 6.151 ng
 RT: 9.98 min Scan# 1300
 Delta R.T. -0.22 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30




Instrument :
 BNA_F
 ClientSampleId :
 ZER-SB-03-11-72


Tgt Ion:	165	Resp:	15497
Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.4	54.6#
89	0.0	57.8	86.6#
182	0.0	1.6	2.4#

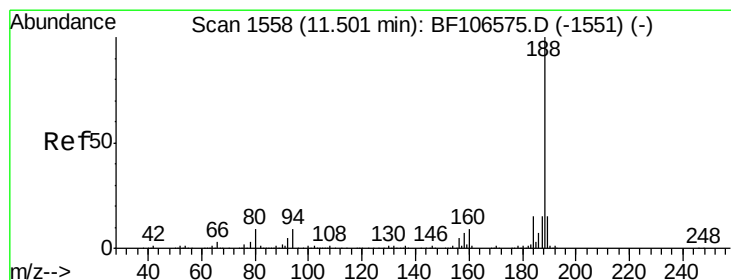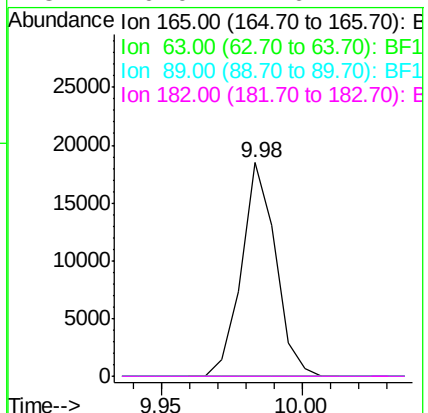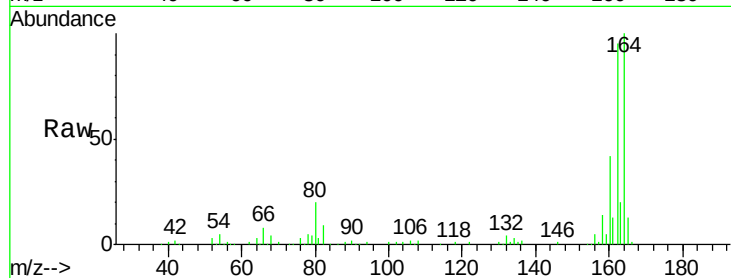

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.48 min Scan# 1555
 Delta R.T. -0.02 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30

Tgt Ion:	188	Resp:	241484
Ion	Ratio	Lower	Upper
188	100		
94	8.0	8.5	12.7#
80	8.4	9.2	13.8#

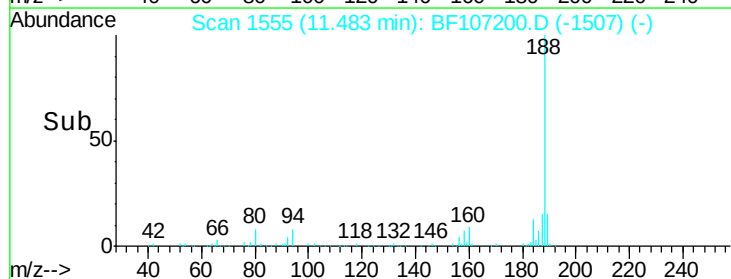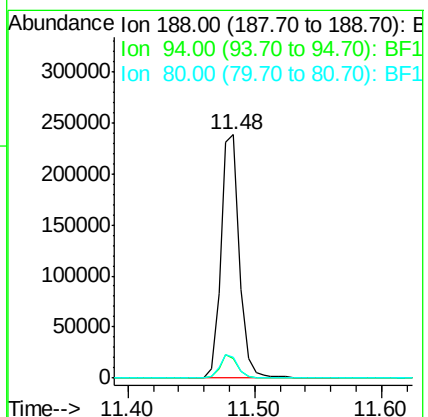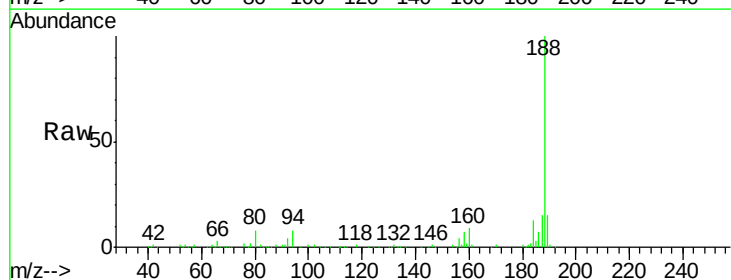


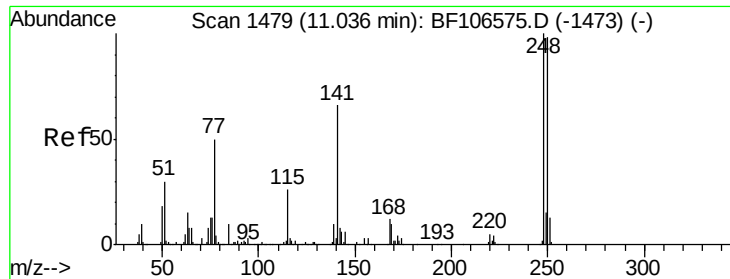




#66
 4-Bromophenyl-phenylether
 Concen: 3.161 ng
 RT: 10.78 min Scan# 1436
 Delta R.T. -0.25 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30

Instrument :
 BNA_F
 ClientSampleId :
 ZER-SB-03-11-72

Tgt Ion: 248 Resp: 9109
 Ion Ratio Lower Upper
 248 100
 250 199.6 76.9 115.3#
 141 348.0 74.4 111.6#

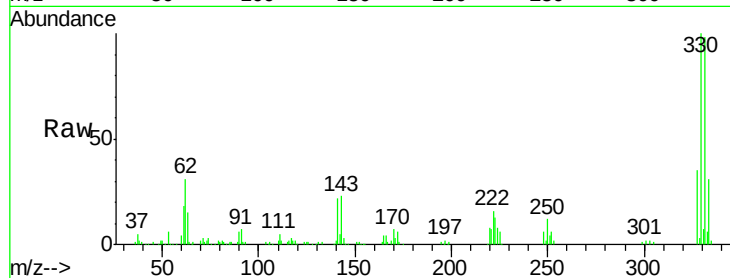


Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

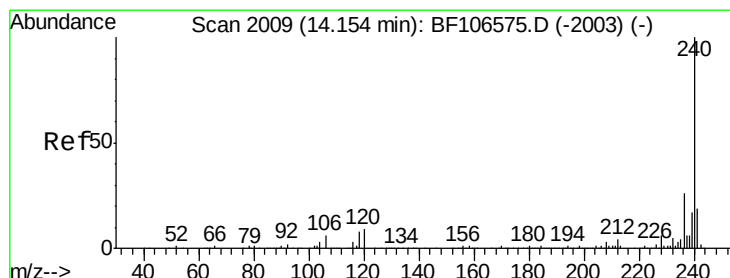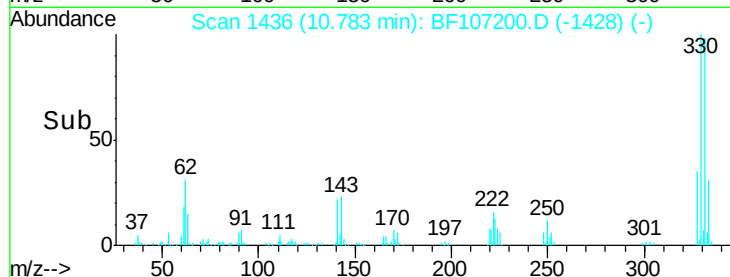
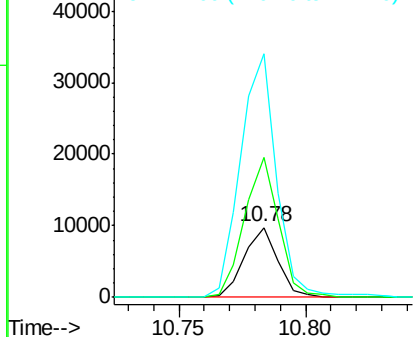



#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.13 min Scan# 2005
 Delta R.T. -0.04 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30

Tgt Ion: 240 Resp: 174733
 Ion Ratio Lower Upper
 240 100
 120 10.4 9.5 14.3
 236 25.8 20.7 31.1

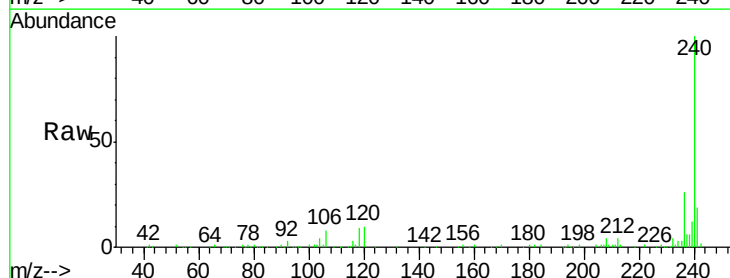

Abundance Ion 240.00 (239.70 to 240.70): E
 Ion 120.00 (119.70 to 120.70): E
 Ion 236.00 (235.70 to 236.70): E



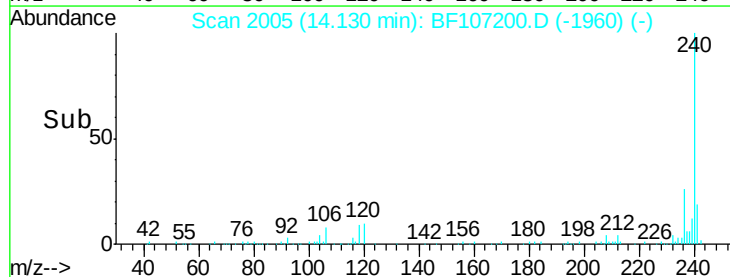
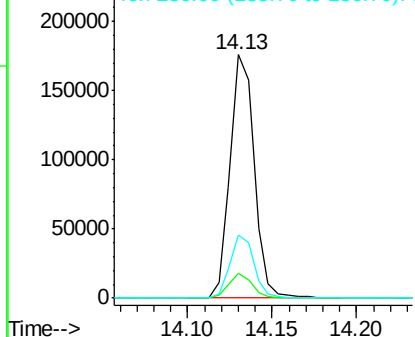


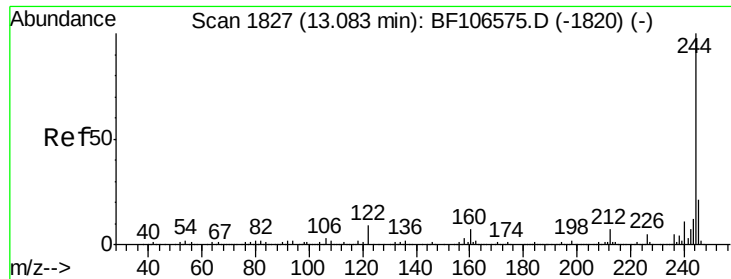

#78
 Terphenyl-d14
 Concen: 74.445 ng
 RT: 13.07 min Scan# 1824
 Delta R.T. -0.02 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30

Instrument :
 BNA_F
 ClientSampleId :
 ZER-SB-03-11-72

Tgt Ion: 244 Resp: 537014
 Ion Ratio Lower Upper
 244 100
 212 6.4 5.4 8.0
 122 8.2 11.0 16.4#

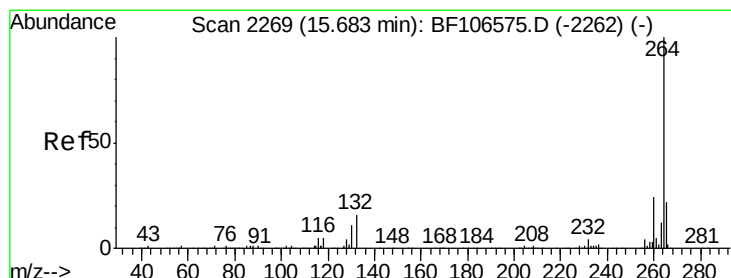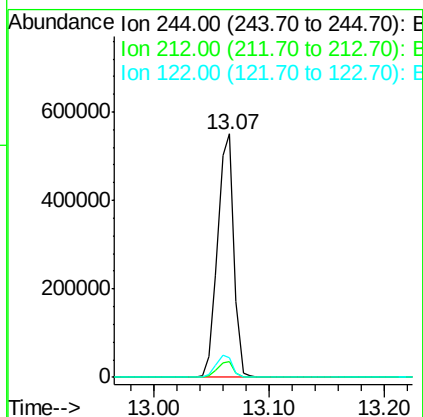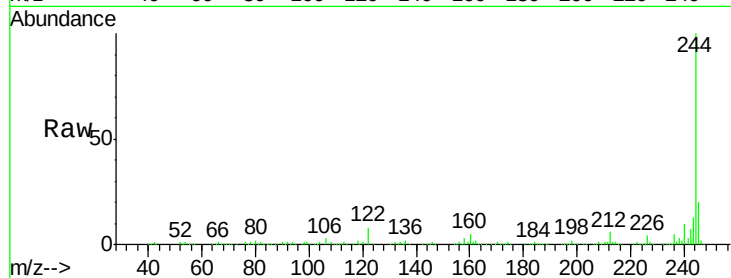

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.67 min Scan# 2266
 Delta R.T. -0.05 min
 Lab File: BF107200.D
 Acq: 7 Jul 2018 12:30

Tgt Ion: 264 Resp: 172167
 Ion Ratio Lower Upper
 264 100
 260 23.7 19.2 28.8
 265 21.8 17.5 26.3

