
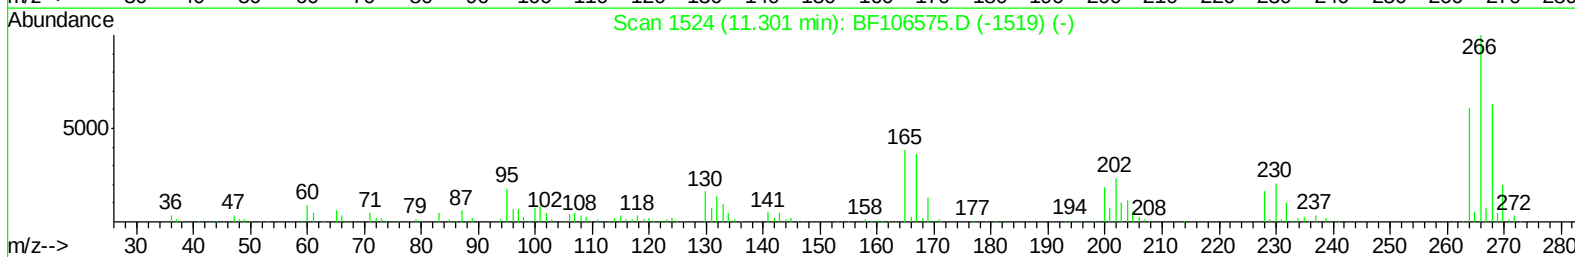
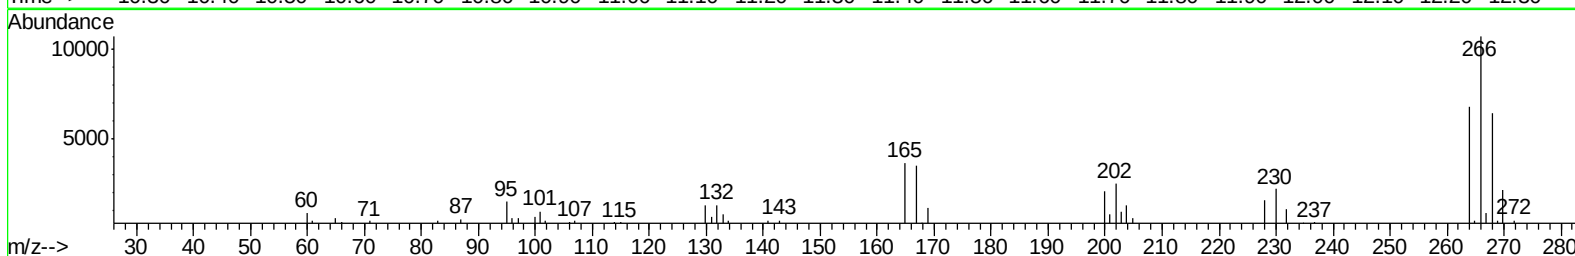


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070718\
Data File : BF107193.D
Acq On : 7 Jul 2018 9:21
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 09 07:18:41 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

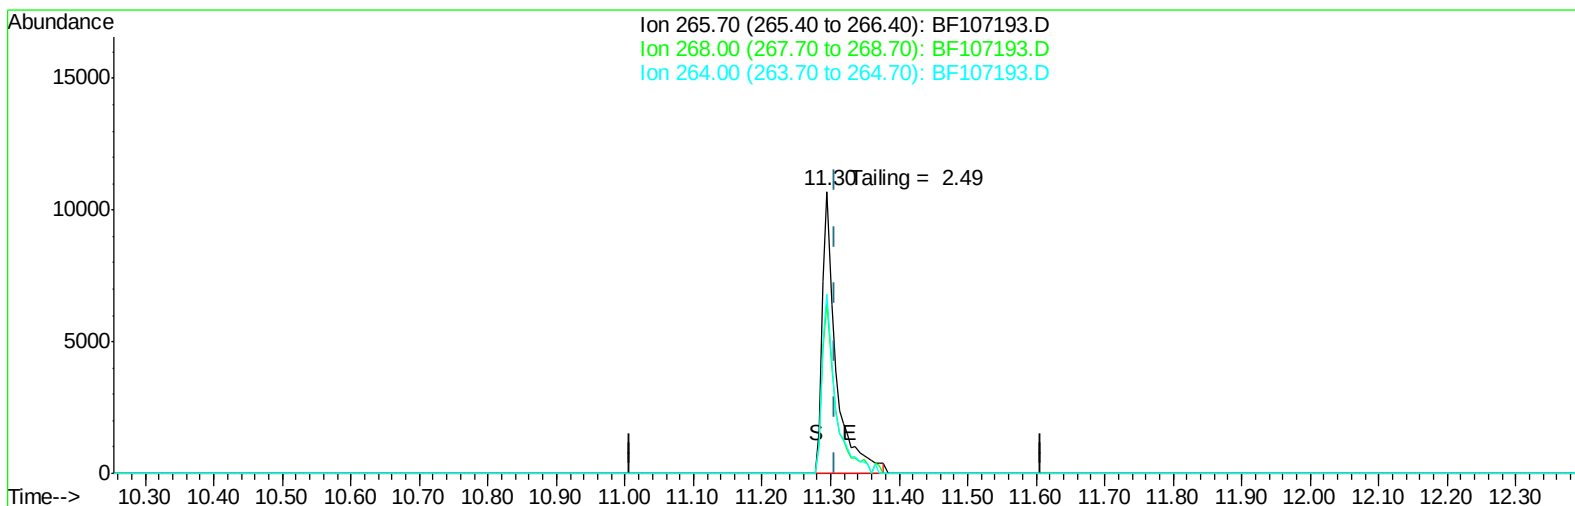

TIC: BF107193.D

(69) Pentachlorophenol (C)

11.295min (-0.012) 0.00ng

response 14634

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.30
264.00	61.90	63.71
0.00	0.00	0.00