


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070718\
 Data File : BF107193.D
 Acq On : 7 Jul 2018 9:21
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 29 14:38:29 2018

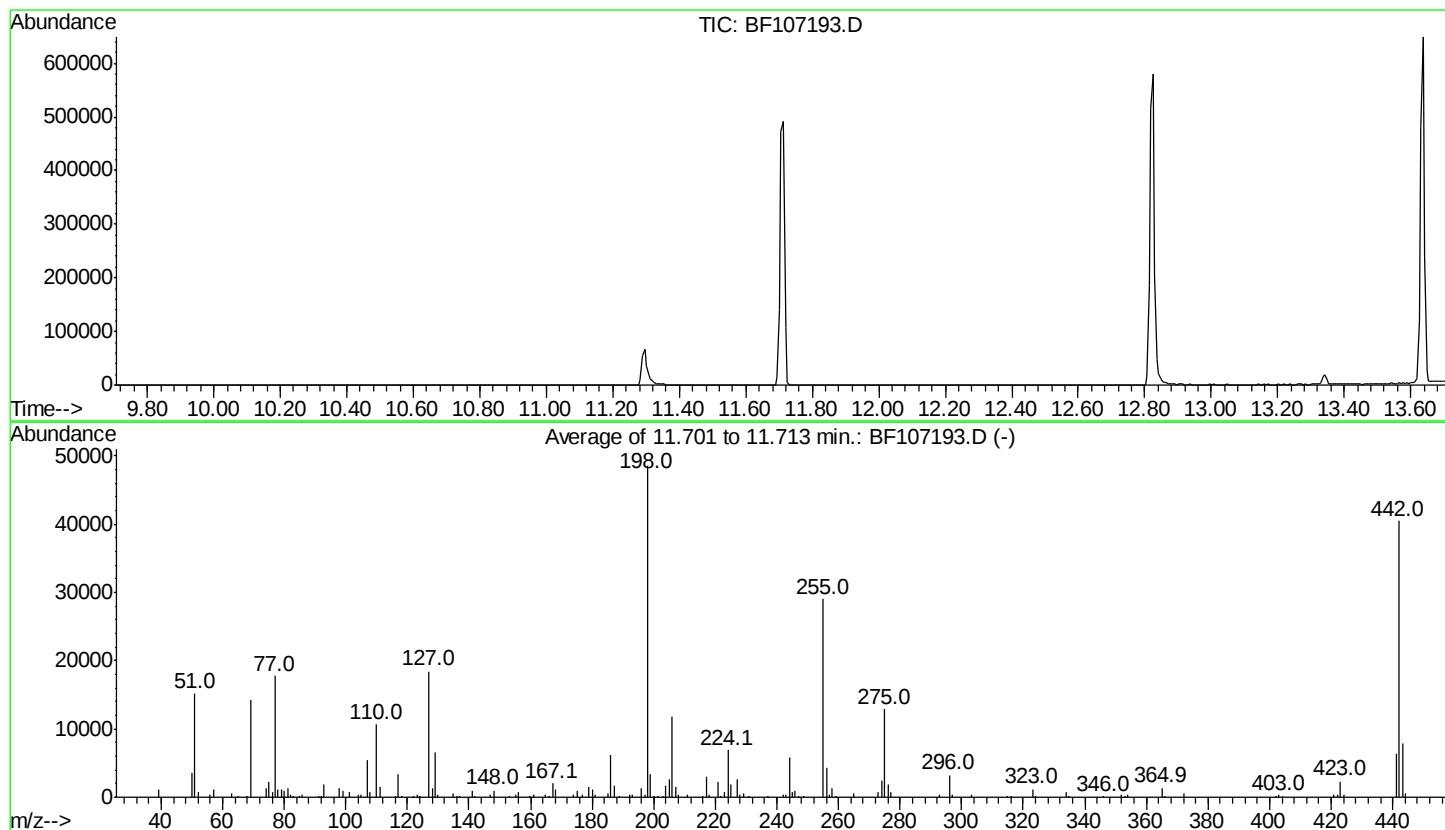

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	15118	PASS
68	69	0.00	2	0.9	123	PASS
69	198	0.00	100	29.5	14313	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	37.9	18394	PASS
197	198	0.00	2	0.6	307	PASS
198	198	100	100	100.0	48560	PASS
199	198	5	9	7.0	3423	PASS
275	198	10	60	26.6	12908	PASS
365	198	1	100	2.9	1389	PASS
441	198	0.01	100	13.1	6374	PASS
442	198	50	100	83.2	40409	PASS
443	442	15	24	19.7	7955	PASS