

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070720\
Data File : BF120803.D
Acq On : 8 Jul 2020 00:33
Operator : JU/CG
Sample : PB130002BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130002BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	567	573	576	rBV	3714361	4191759	86.79%	12.706%
2	6.475	739	746	748	rBV	3450146	4218911	87.35%	12.788%
3	6.845	805	809	812	rBV	1240676	930811	19.27%	2.821%
4	7.004	832	836	839	rBV	3977266	3547238	73.44%	10.752%
5	7.410	900	905	908	rBV	2898111	2809469	58.17%	8.516%
6	8.128	1023	1027	1030	rBV	1494602	1177476	24.38%	3.569%
7	9.210	1206	1211	1214	rBV	4894320	4650464	96.29%	14.096%
8	9.881	1322	1325	1329	rBV	1461980	1282527	26.55%	3.887%
9	10.669	1455	1459	1462	rBV	2569042	2304786	47.72%	6.986%
10	11.369	1574	1578	1581	rBV	1565789	1299972	26.92%	3.940%
11	12.963	1843	1849	1852	rBV	4363059	4829796	100.00%	14.639%
12	14.004	2022	2026	2034	rBV	1211423	995314	20.61%	3.017%
13	15.463	2269	2274	2280	rBV	659230	753033	15.59%	2.283%


Sum of corrected areas: 32991556

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070720\
Data File : BF120803.D
Acq On : 8 Jul 2020 00:33
Operator : JU/CG
Sample : PB130002BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130002BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

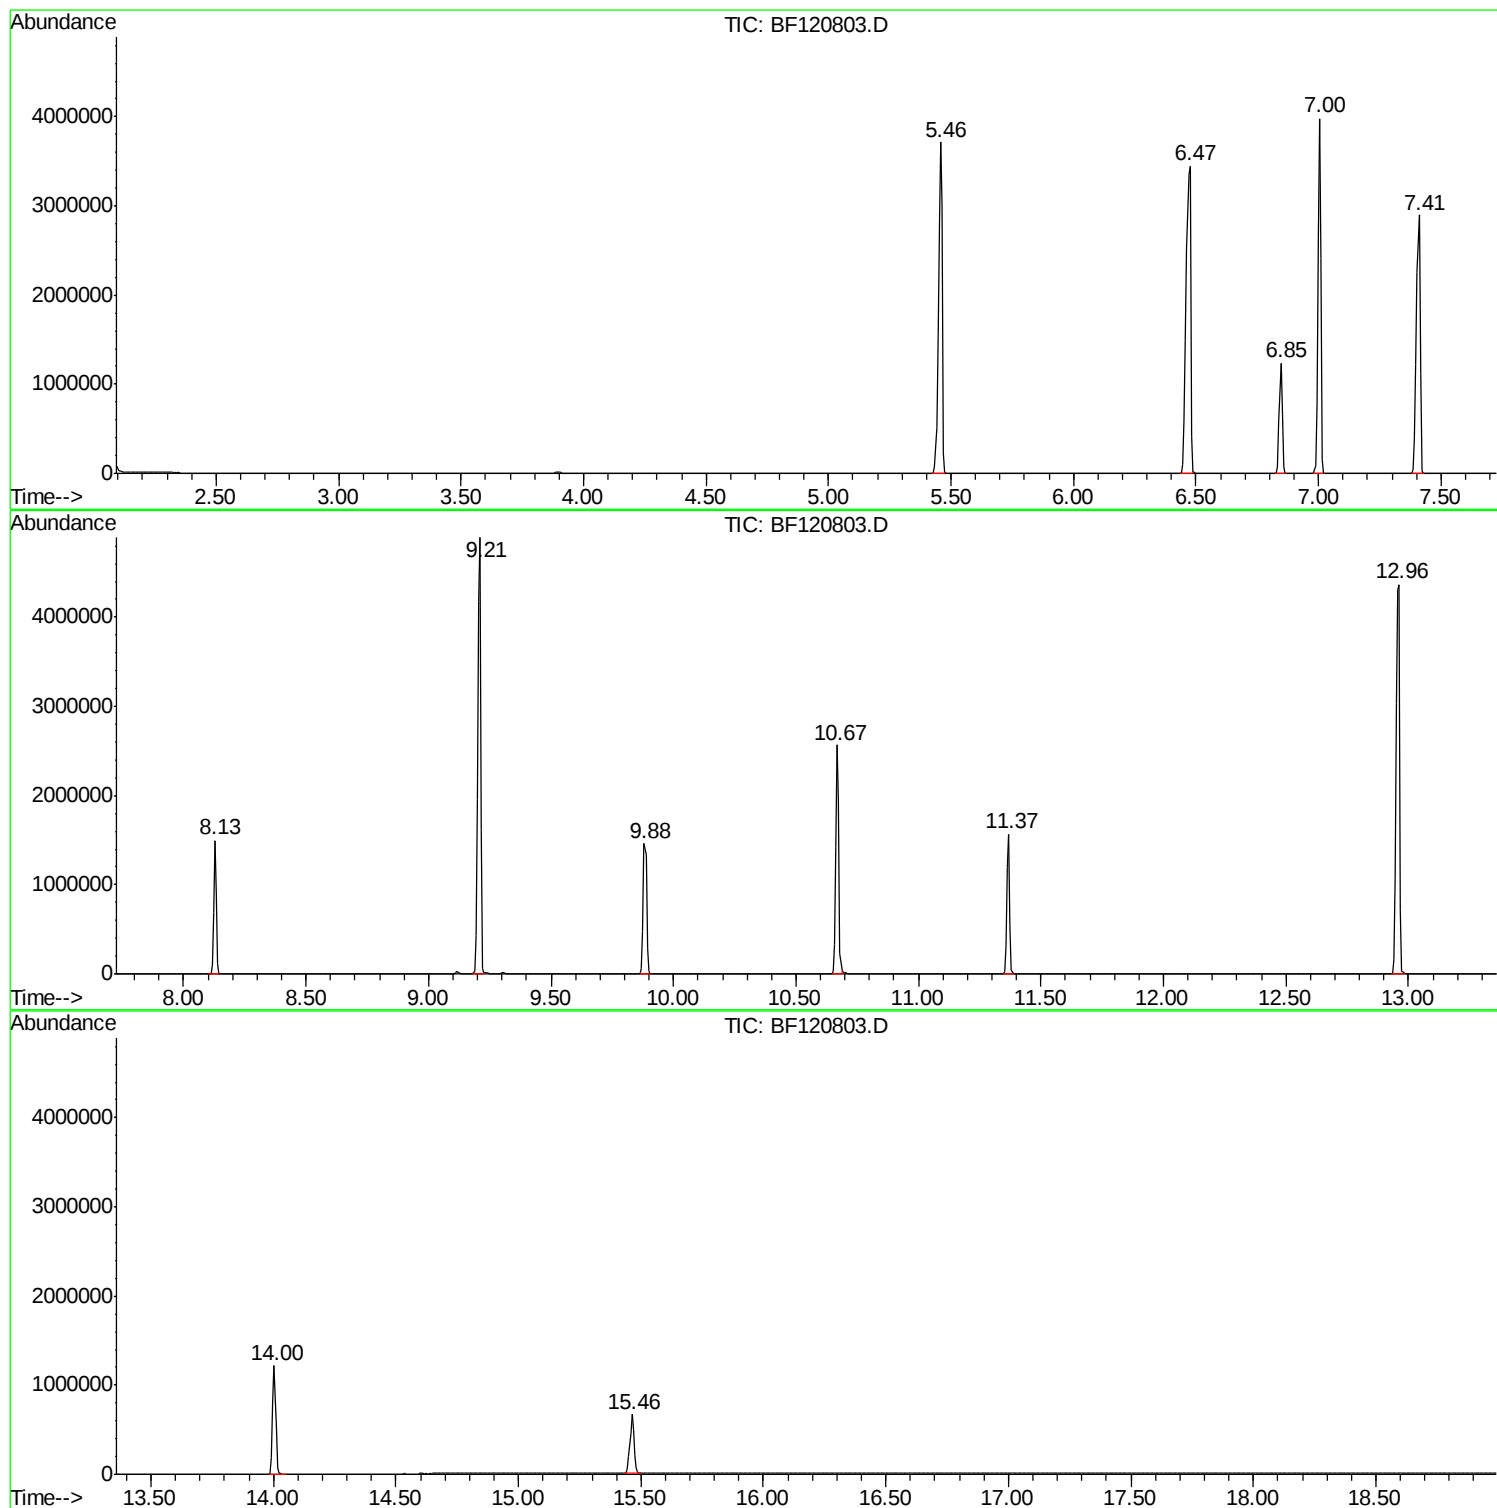

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070720\
Data File : BF120803.D
Acq On : 8 Jul 2020 00:33
Operator : JU/CG
Sample : PB130002BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130002BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF070720\
Data File : BF120803.D
Acq On : 8 Jul 2020 00:33
Operator : JU/CG
Sample : PB130002BL
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130002BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc