


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070720\
 Data File : BF120774.D
 Acq On : 7 Jul 2020 8:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 02 18:51:52 2020

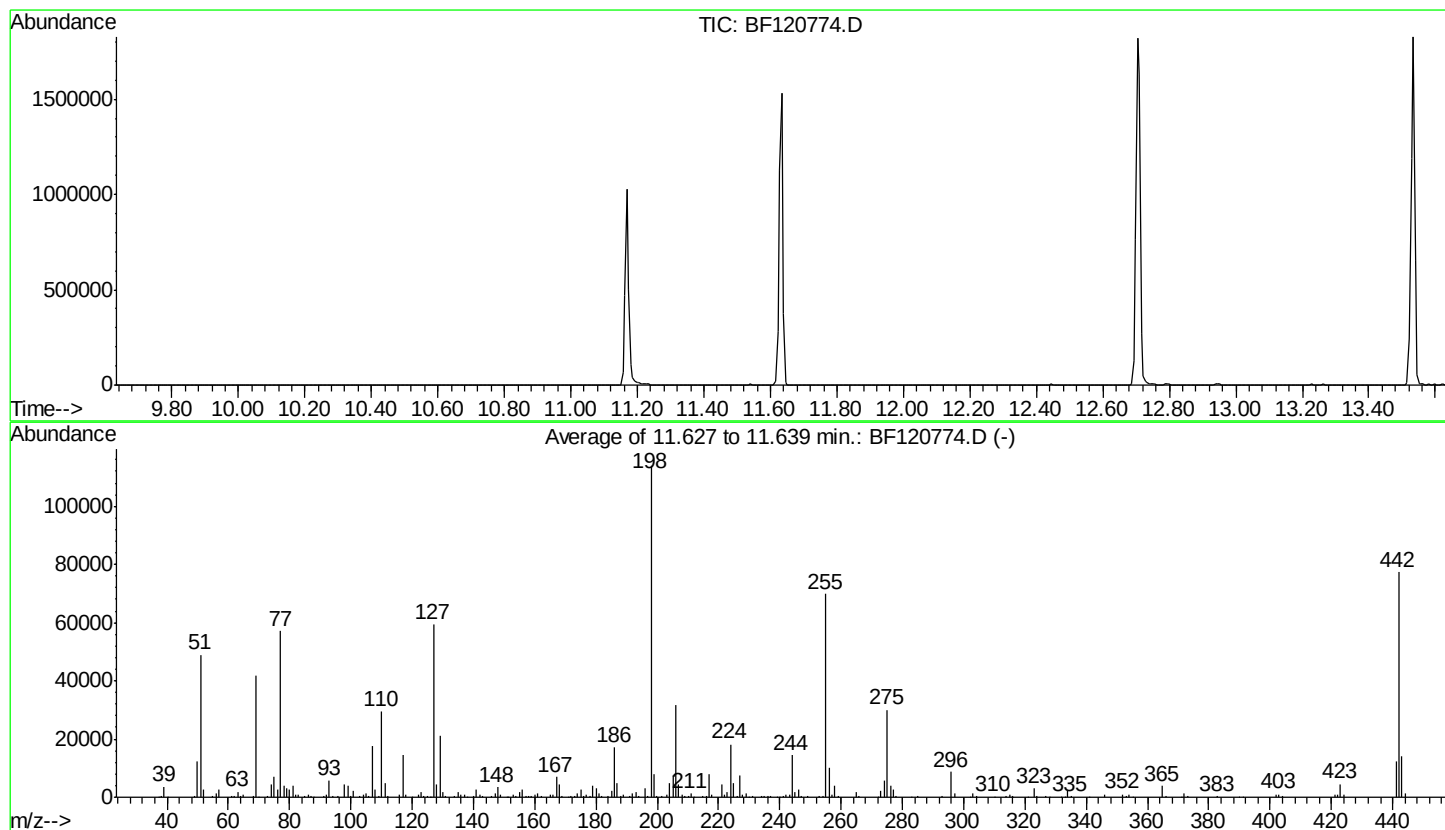

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	49027	PASS
68	69	0.00	2	1.6	666	PASS
69	198	0.00	100	36.8	41929	PASS
70	69	0.00	2	0.5	218	PASS
127	198	10	80	51.9	59192	PASS
197	198	0.00	2	0.5	614	PASS
198	198	100	100	100.0	113954	PASS
199	198	5	9	6.8	7763	PASS
275	198	10	60	26.4	30068	PASS
365	198	1	100	3.3	3777	PASS
441	198	0.01	100	10.9	12366	PASS
442	198	50	100	67.8	77277	PASS
443	442	15	24	18.2	14053	PASS