


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF070720\  
 Data File : BF120799.D  
 Acq On : 7 Jul 2020 22:13  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF070220.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Jul 02 18:51:52 2020

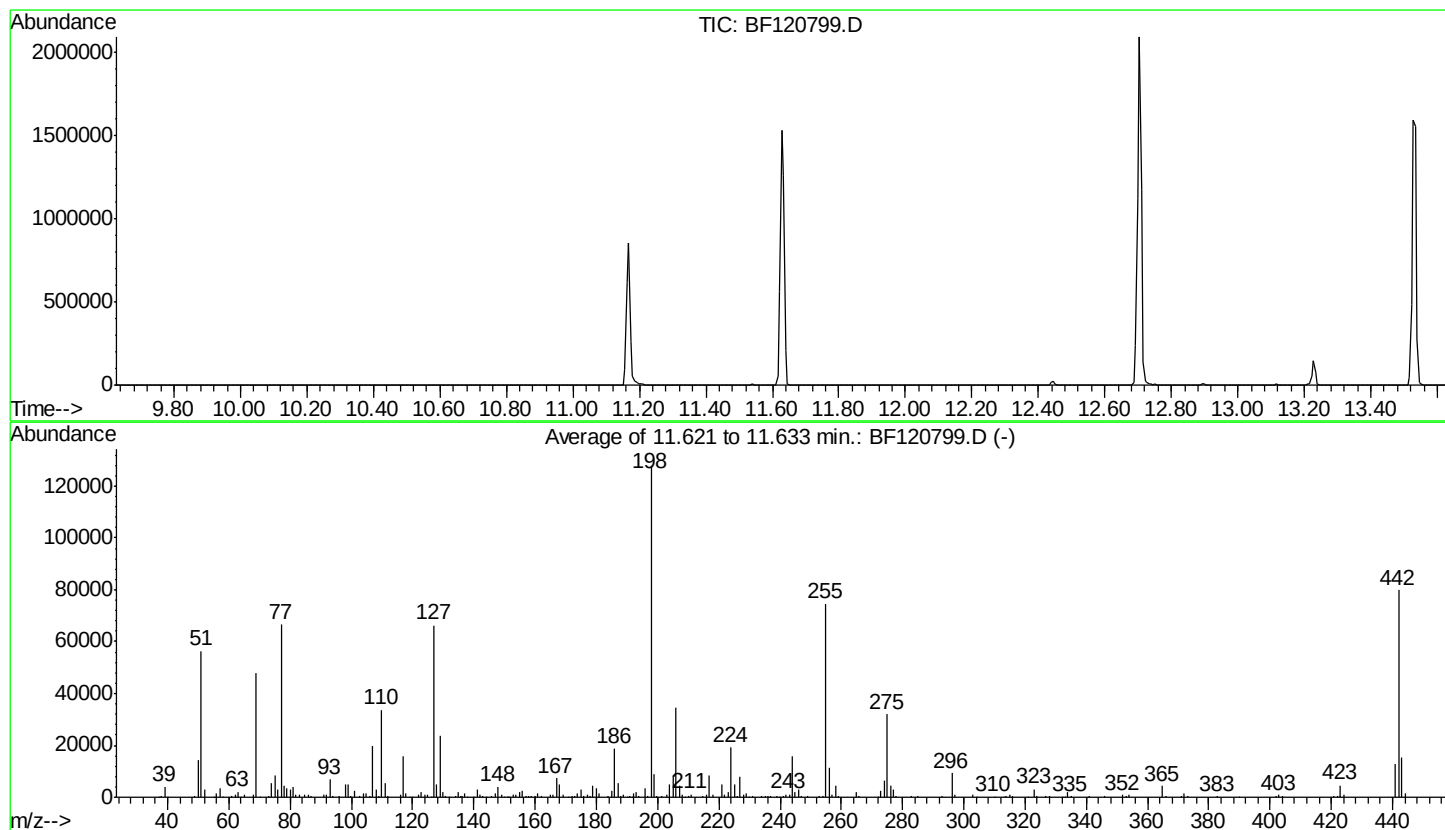

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1617

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 44.2      | 56530   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 865     | PASS             |
| 69          | 198          | 0.00         | 100          | 37.6      | 48093   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.2       | 112     | PASS             |
| 127         | 198          | 10           | 80           | 51.8      | 66234   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.5       | 637     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 127864  | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 8683    | PASS             |
| 275         | 198          | 10           | 60           | 25.0      | 31921   | PASS             |
| 365         | 198          | 1            | 100          | 3.4       | 4330    | PASS             |
| 441         | 198          | 0.01         | 100          | 10.0      | 12764   | PASS             |
| 442         | 198          | 50           | 100          | 62.4      | 79761   | PASS             |
| 443         | 442          | 15           | 24           | 19.1      | 15230   | PASS             |