
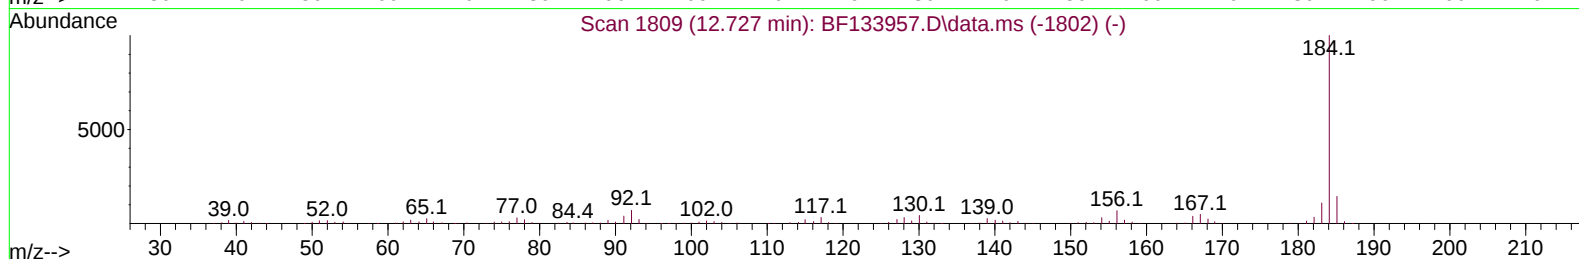
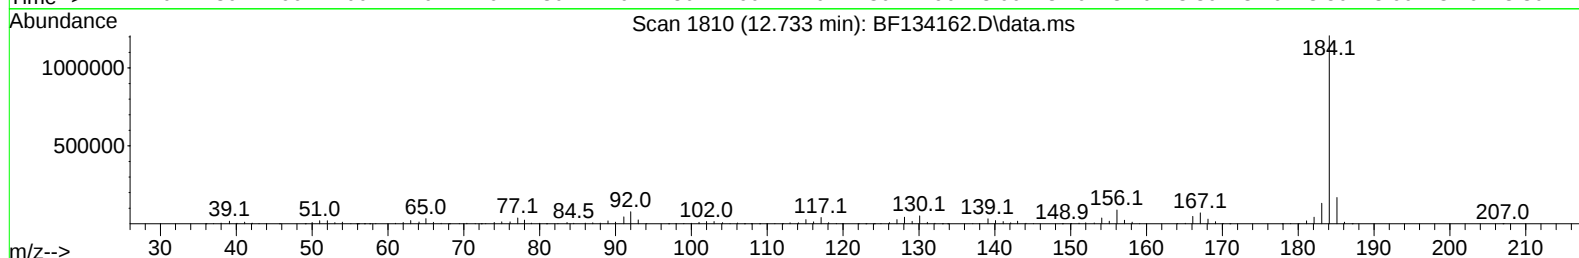


Quant Time: Jul 09 02:30:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

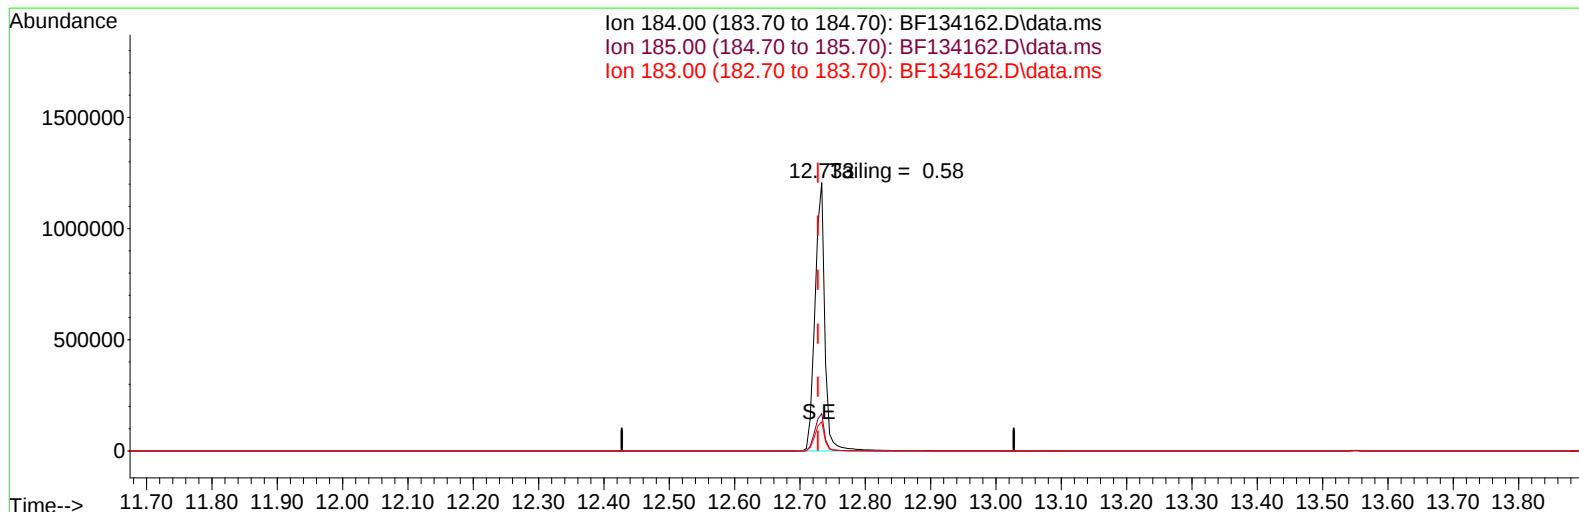

TIC: BF134162.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 98152.51 ng

```
response      1261156
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.99
183.00	11.00	10.91
0.00	0.00	0.00