
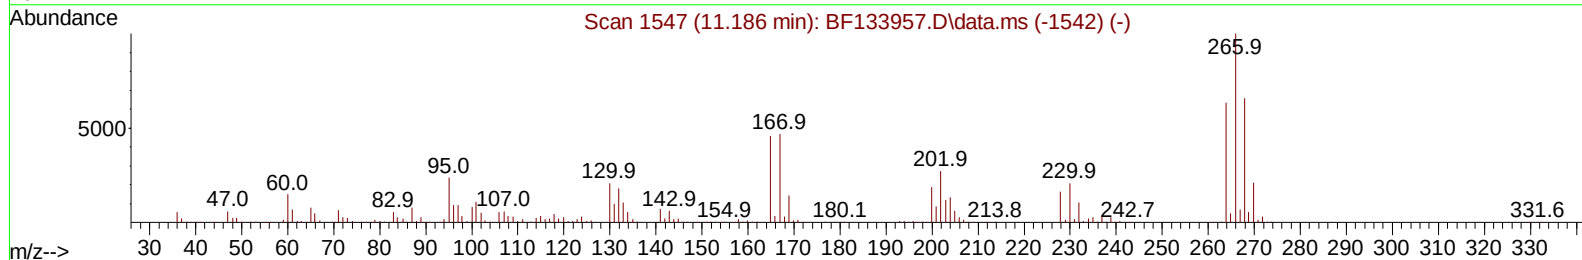
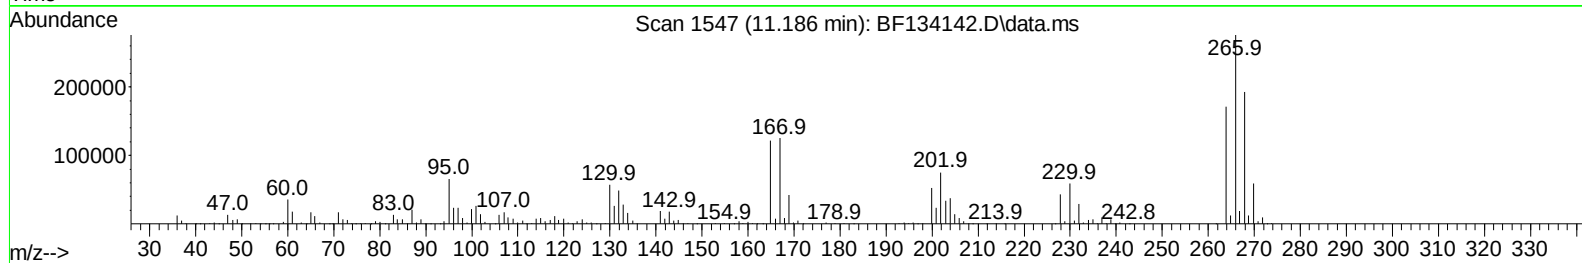


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070823\
Data File : BF134142.D
Acq On : 08 Jul 2023 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 12:56:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

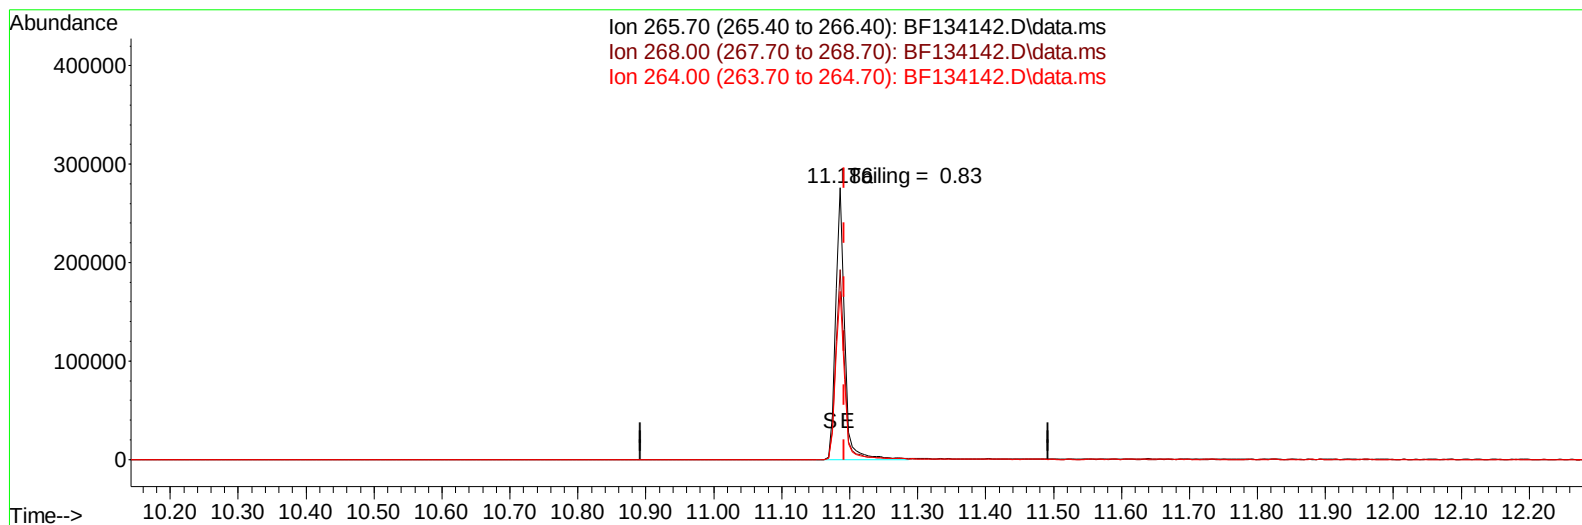

TIC: BF134142.D\data.ms

(70) Pentachlorophenol (C)




11.186min (-0.006) 27958.42 ng

response 251476

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	69.95
264.00	63.30	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070823\
Data File : BF134142.D
Acq On : 08 Jul 2023 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 08 12:56:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

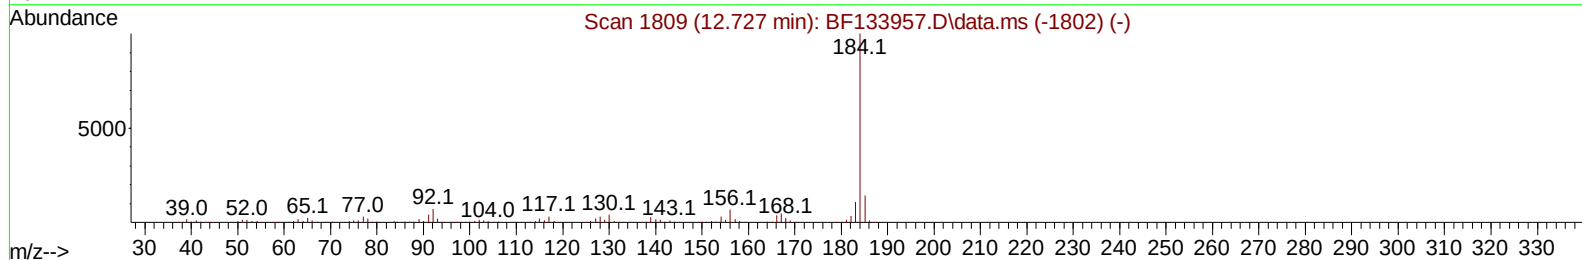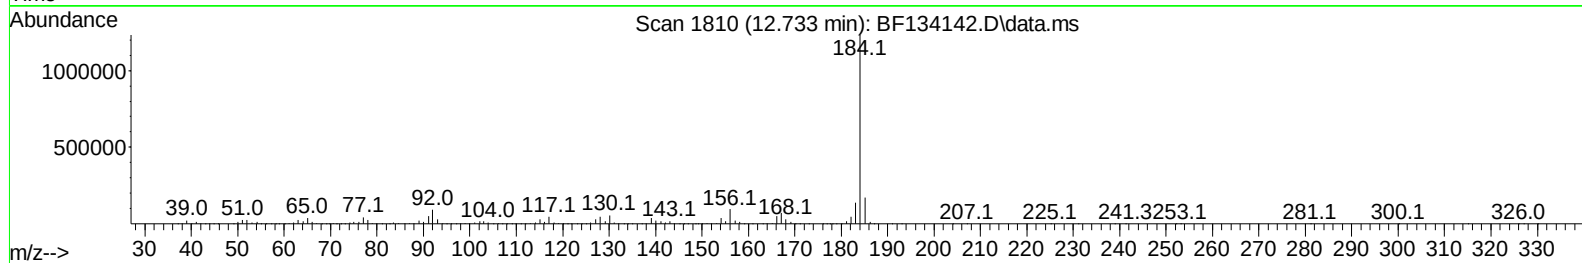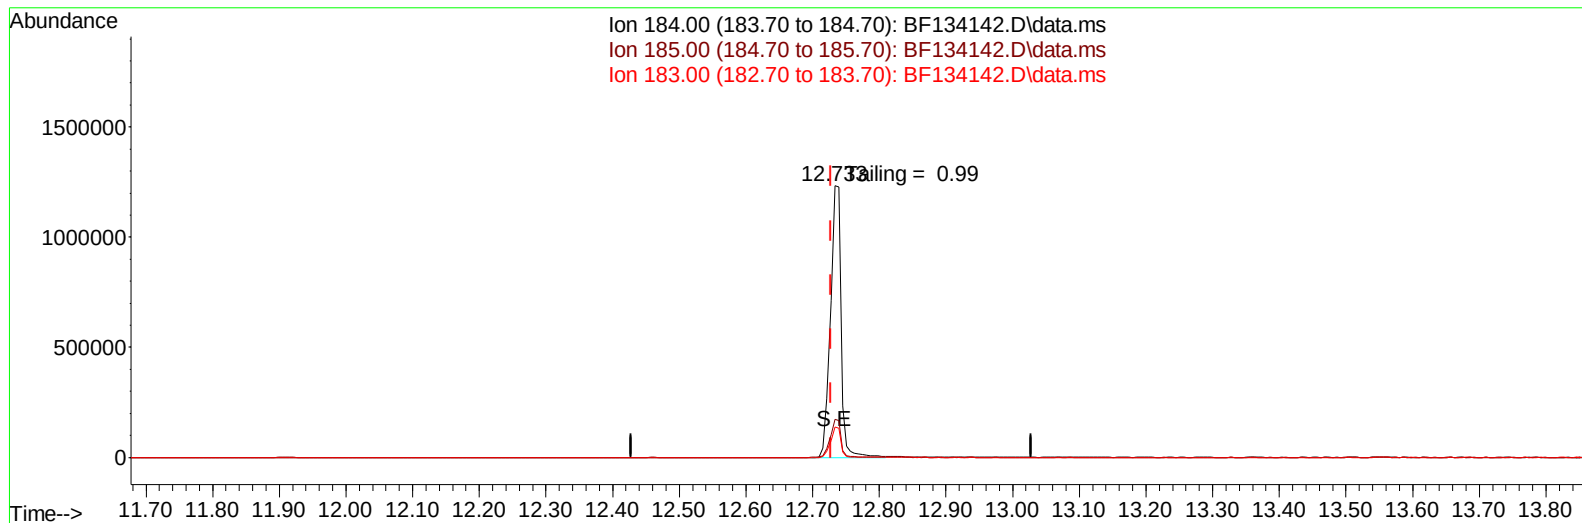

TIC: BF134142.D\data.ms

(77) Benzidine**12.733min (+ 0.006) 23885.38 ng****response 1383332**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.99
183.00	11.00	11.22
0.00	0.00	0.00