
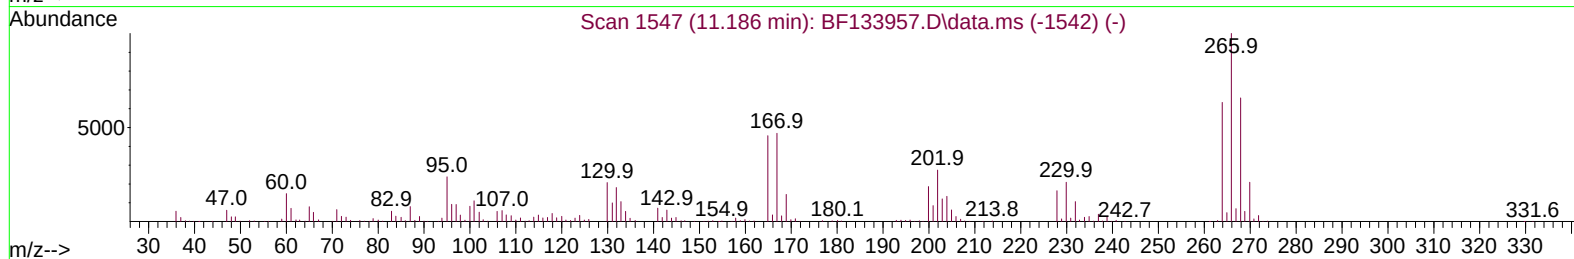
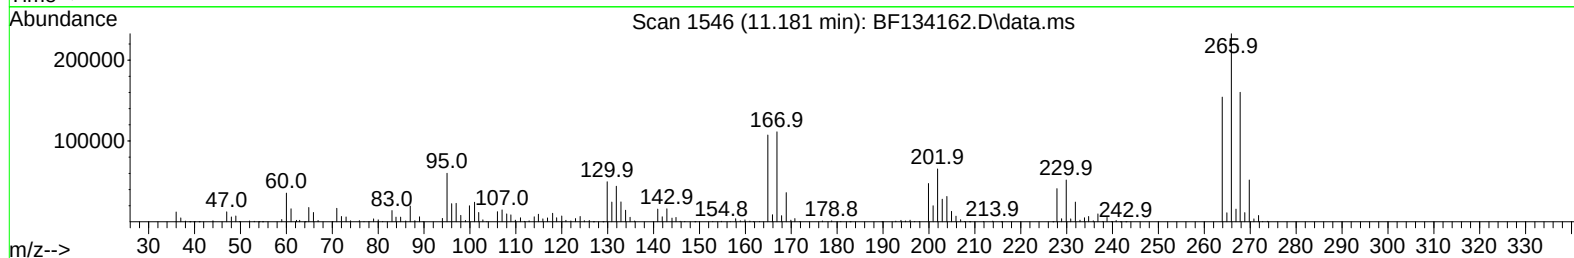


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070823\
Data File : BF134162.D
Acq On : 08 Jul 2023 23:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 09 02:30:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

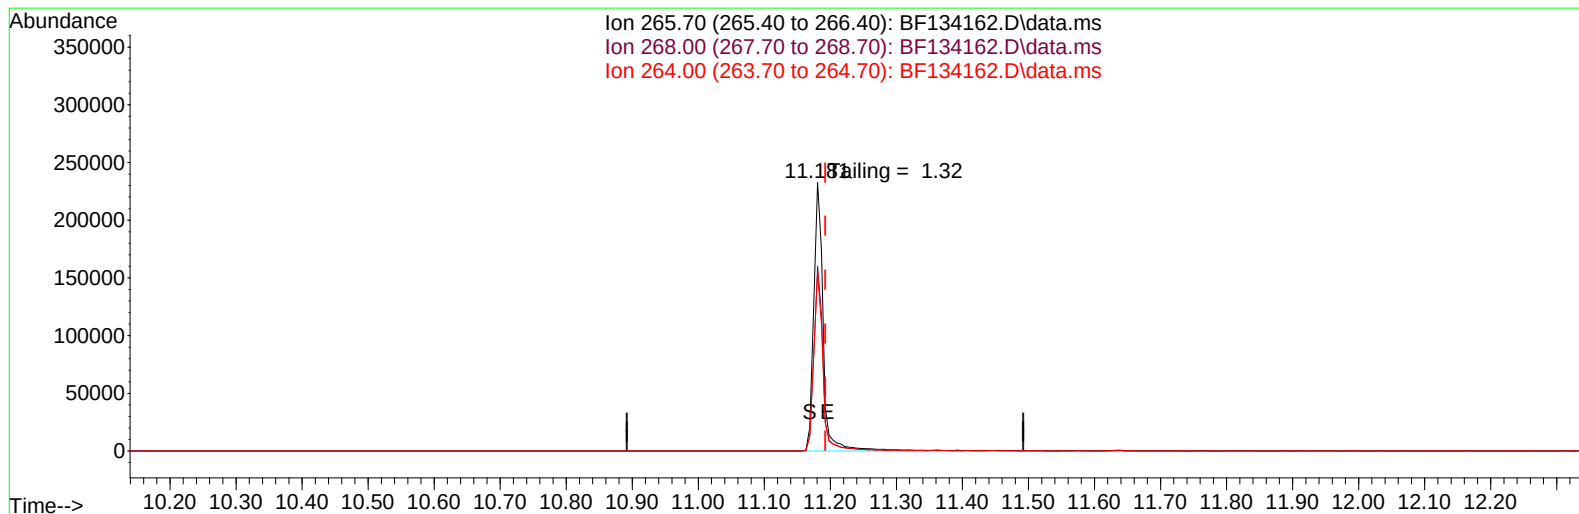

TIC: BF134162.D\data.ms




(70) Pentachlorophenol (C)

11.181min (-0.012) 131675.95 ng

response 231900

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	68.90
264.00	63.30	66.32
0.00	0.00	0.00

Quant Time: Jul 09 02:30:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

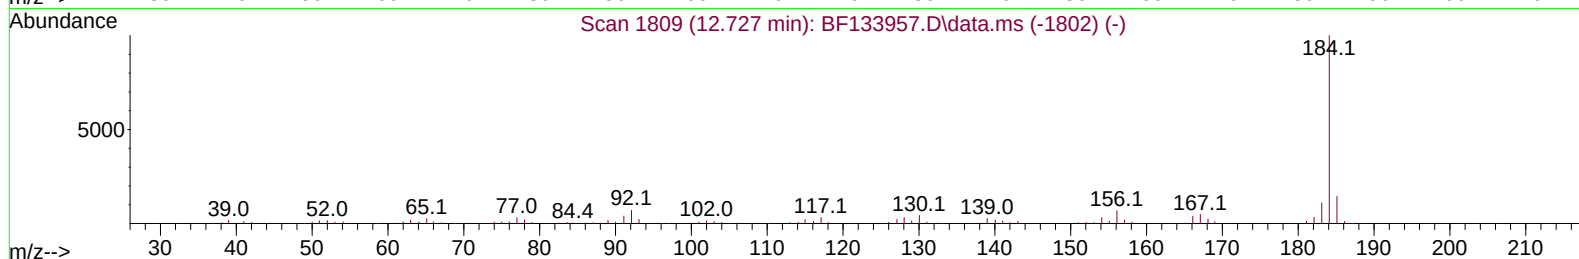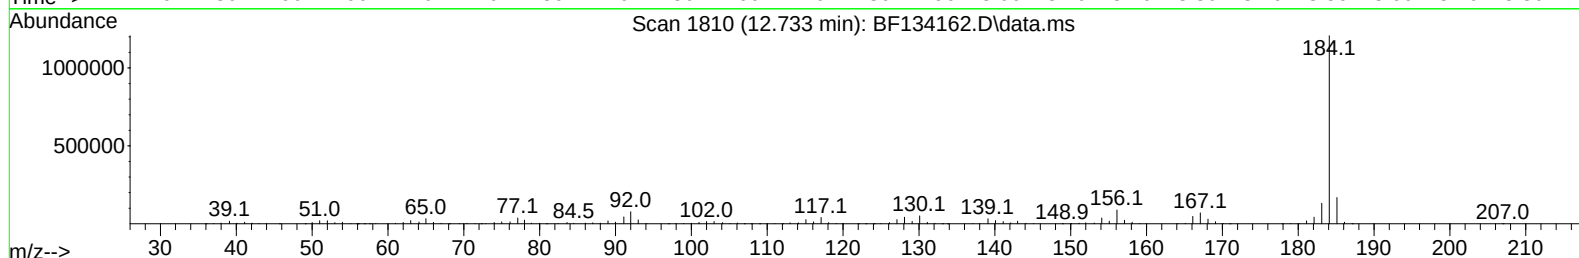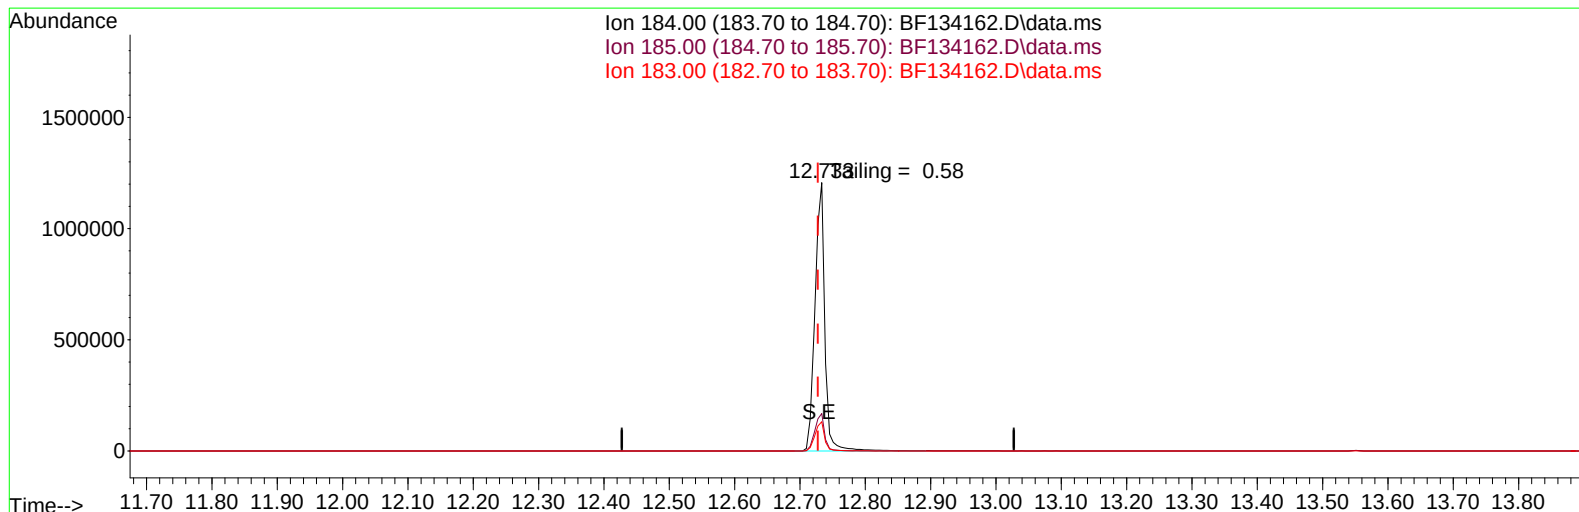

TIC: BF134162.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 98152.51 ng

```
response      1261156
```

Ion	Exp%	Act%
-----	------	------

184.00	100.00	100.00
--------	--------	--------

185.00 14.50 13.99

183.00	11.00	10.91
--------	-------	-------

0.00 0.00 0.00