

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070823\
 Data File : BF134171.D
 Acq On : 09 Jul 2023 05:02
 Operator : CG\JU
 Sample : 03507-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CP-1

Quant Time: Jul 09 05:48:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 30 18:35:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.845	152	162382	20.000	ng	0.00
21) Naphthalene-d8	8.122	136	652533	20.000	ng	-0.01
39) Acenaphthene-d10	9.880	164	321920	20.000	ng	-0.01
64) Phenanthrene-d10	11.374	188	623953	20.000	ng	-0.01
76) Chrysene-d12	14.033	240	409771	20.000	ng	#-0.02
86) Perylene-d12	15.539	264	359229	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.498	112	1072566	110.490	ng	0.01
7) Phenol-d6	6.480	99	1316790	110.301	ng	-0.01
23) Nitrobenzene-d5	7.410	82	998636	82.497	ng	-0.01
42) 2,4,6-Tribromophenol	10.680	330	511798	126.801	ng	0.00
45) 2-Fluorobiphenyl	9.204	172	1727804	78.033	ng	0.00
79) Terphenyl-d14	12.980	244	2201307	86.459	ng	0.00


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070823\
Data File : BF134171.D
Acq On : 09 Jul 2023 05:02
Operator : CG\JU
Sample : 03507-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CP-1

Quant Time: Jul 09 05:48:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration




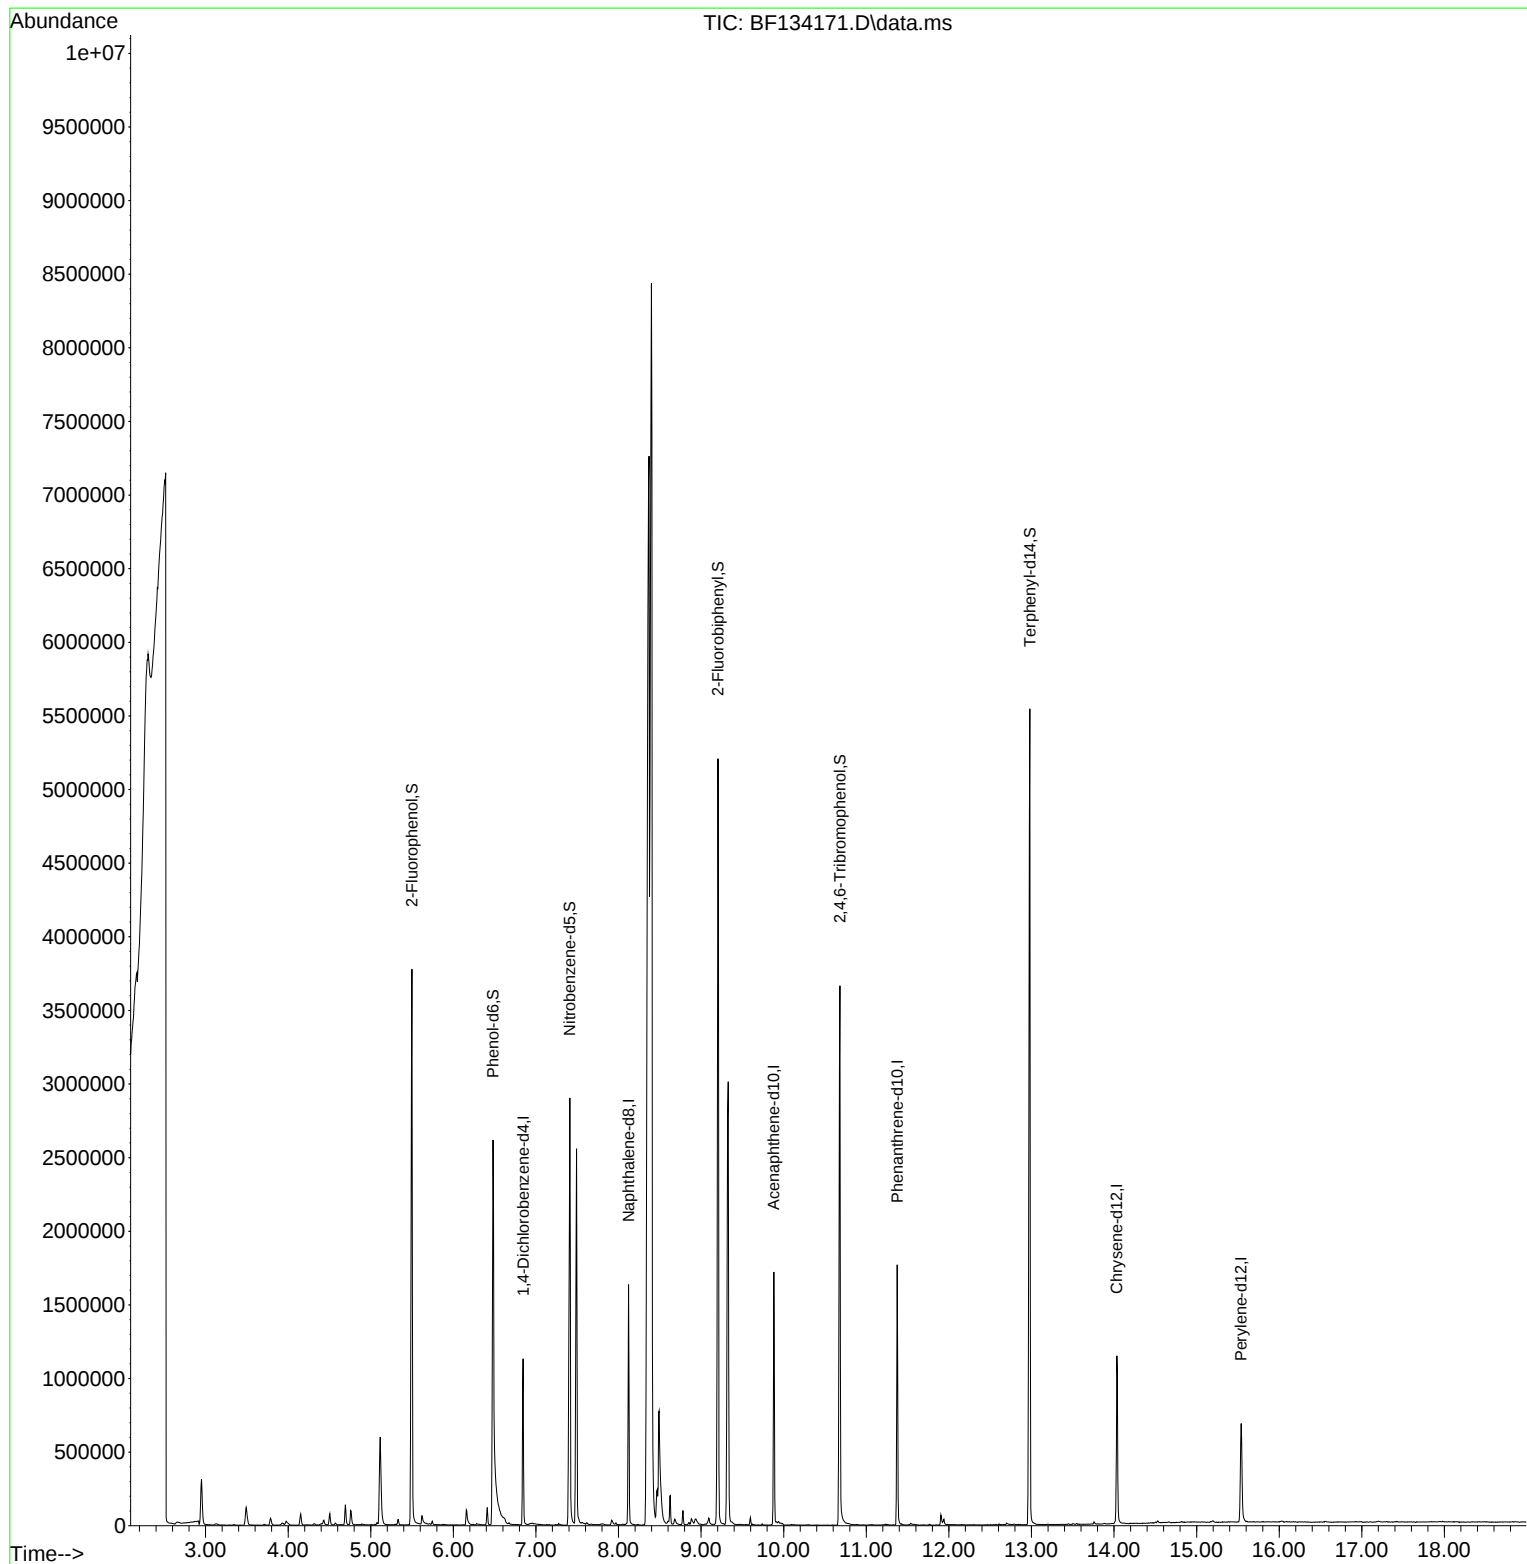




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.845 min Scan# 80
Delta R.T. -0.006 min
Lab File: BF134171.D
Acq: 09 Jul 2023 05:02




Instrument :
BNA_F
ClientSampleId :
CP-1

Tgt Ion:152 Resp: 162382
Ion Ratio Lower Upper
152 100
150 160.6 124.5 186.7
115 60.2 50.2 75.2

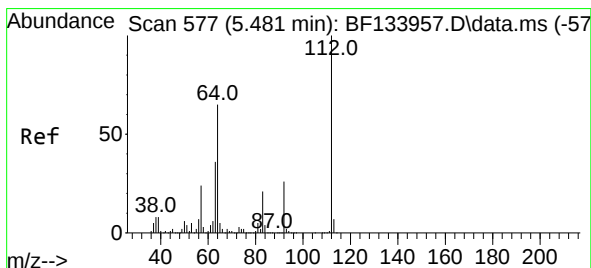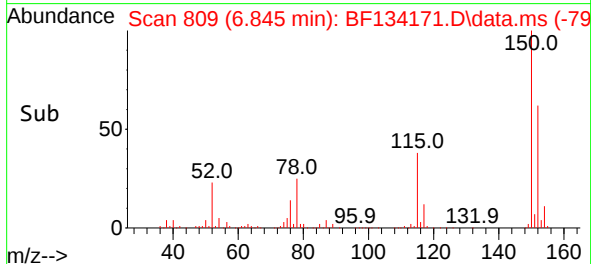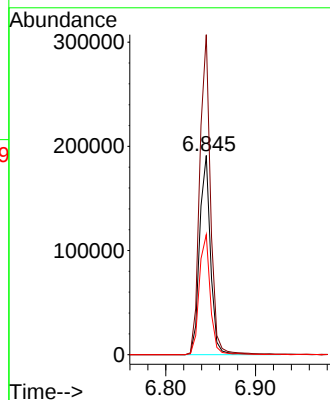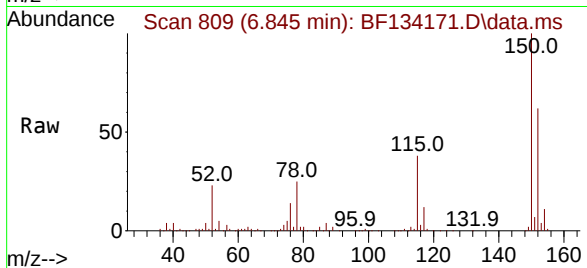

#5
2-Fluorophenol
Concen: 110.490 ng
RT: 5.498 min Scan# 580
Delta R.T. 0.011 min
Lab File: BF134171.D
Acq: 09 Jul 2023 05:02

Tgt Ion:112 Resp: 1072566
Ion Ratio Lower Upper
112 100
64 63.3 52.1 78.1
63 36.0 28.6 42.8


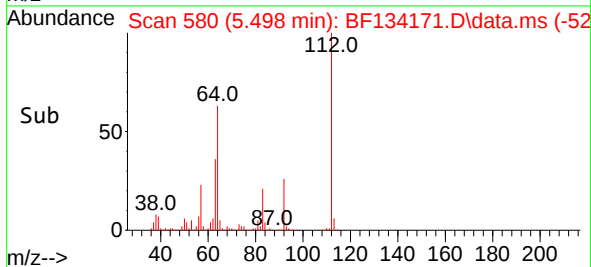
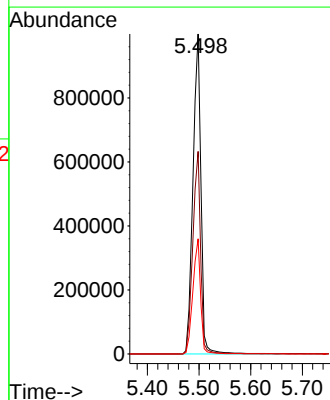
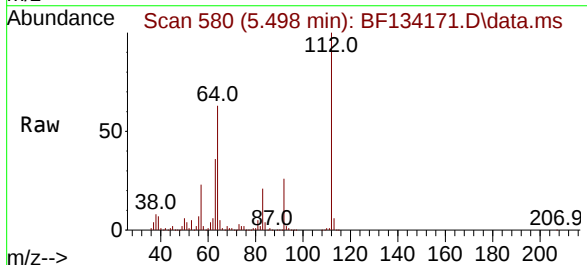




#7
Phenol-d6
Concen: 110.301 ng
RT: 6.480 min Scan# 749
Delta R.T. -0.012 min
Lab File: BF134171.D
Acq: 09 Jul 2023 05:02




Instrument :
BNA_F
ClientSampleId :
CP-1


Tgt Ion: 99 Resp: 1316790
Ion Ratio Lower Upper
99 100
42 24.8 19.8 29.6
71 41.8 31.9 47.9

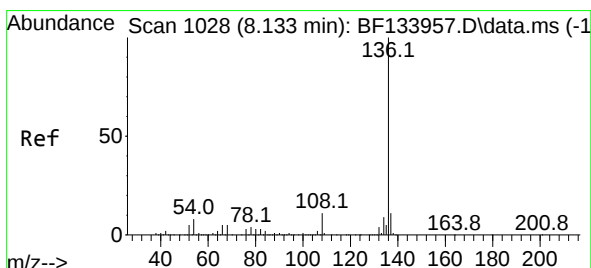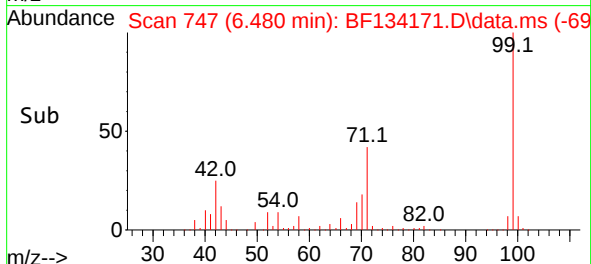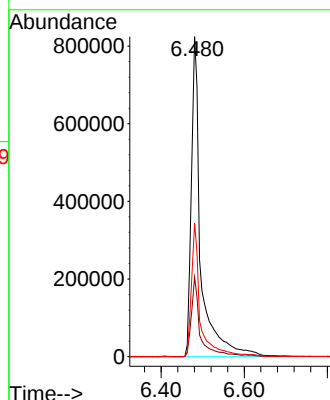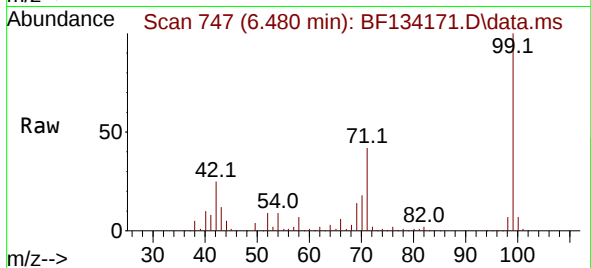

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.122 min Scan# 1026
Delta R.T. -0.012 min
Lab File: BF134171.D
Acq: 09 Jul 2023 05:02

Tgt Ion:136 Resp: 652533
Ion Ratio Lower Upper
136 100
137 11.1 8.6 12.8
54 8.9 6.5 9.7
68 5.4 4.2 6.2

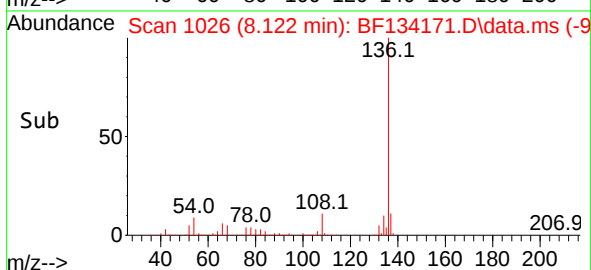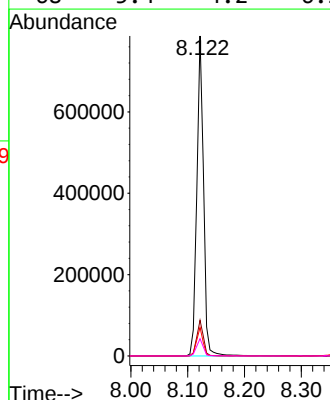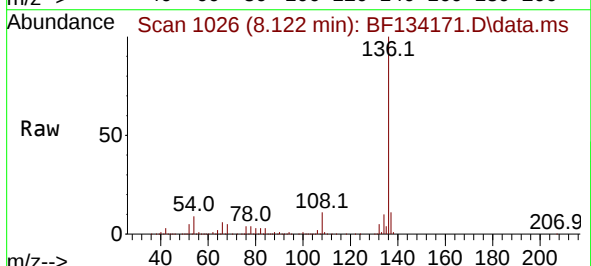

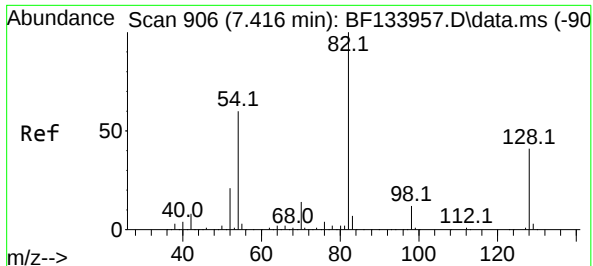

#23

Nitrobenzene-d5

Concen: 82.497 ng

RT: 7.410 min Scan# 906

Delta R.T. -0.012 min

Lab File: BF134171.D

Acq: 09 Jul 2023 05:02

Instrument :

BNA_F

ClientSampleId :

CP-1





Tgt Ion: 82 Resp: 998636

Ion Ratio Lower Upper

82 100

128 41.5 32.5 48.7

54 58.7 48.2 72.2

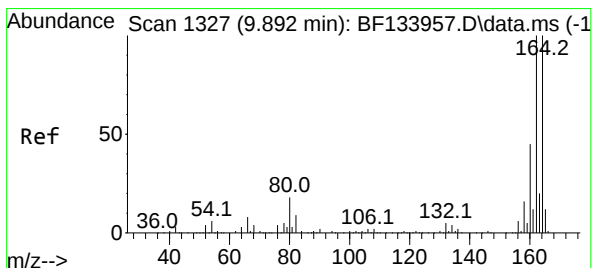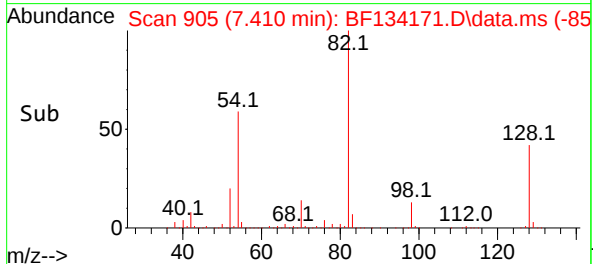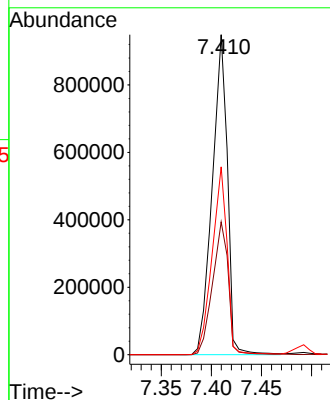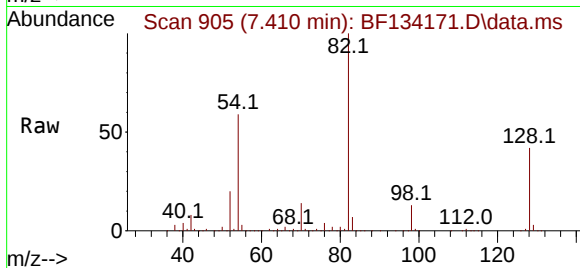

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.880 min Scan# 1325

Delta R.T. -0.012 min

Lab File: BF134171.D

Acq: 09 Jul 2023 05:02




Tgt Ion:164 Resp: 321920

Ion Ratio Lower Upper

164 100

162 101.2 80.0 120.0

160 46.2 35.9 53.9

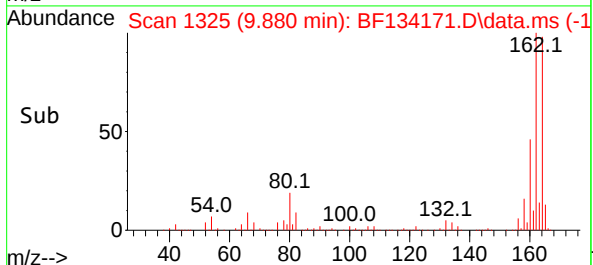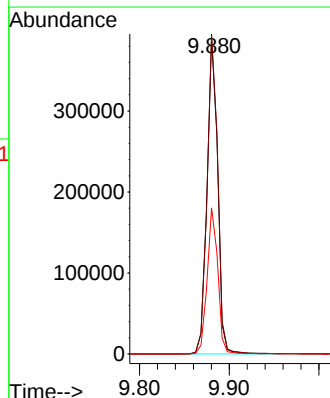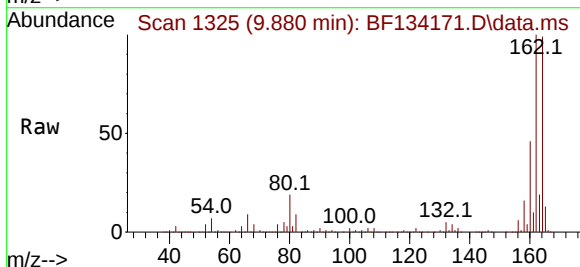



#42

2,4,6-Tribromophenol

Concen: 126.801 ng

RT: 10.680 min Scan# 1461

Delta R.T. -0.006 min

Lab File: BF134171.D

Acq: 09 Jul 2023 05:02

Instrument :

BNA_F

ClientSampleId :

CP-1





Tgt Ion:330 Resp: 511798

Ion Ratio Lower Upper

330 100

332 96.3 77.0 115.6

141 30.0 26.3 39.5

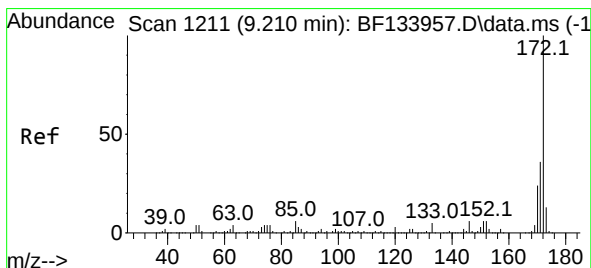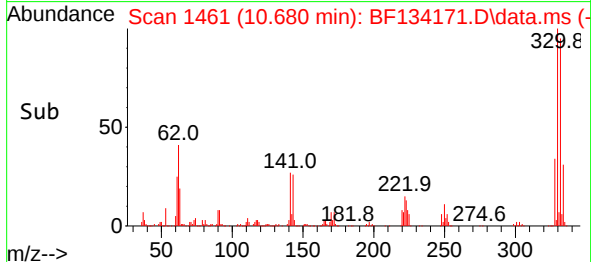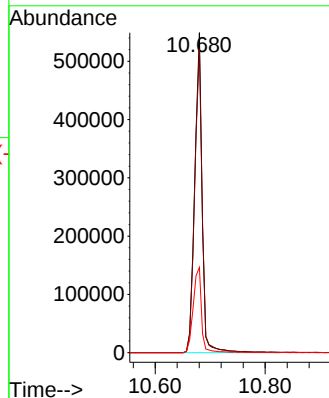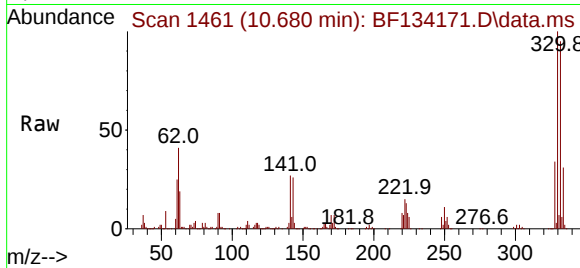

#45

2-Fluorobiphenyl

Concen: 78.033 ng

RT: 9.204 min Scan# 1210

Delta R.T. -0.006 min

Lab File: BF134171.D

Acq: 09 Jul 2023 05:02




Tgt Ion:172 Resp: 1727804

Ion Ratio Lower Upper

172 100

171 35.4 28.6 43.0

170 24.1 19.4 29.0


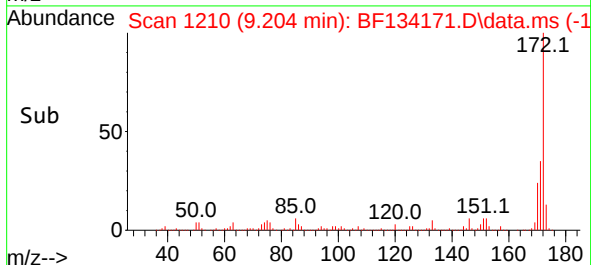
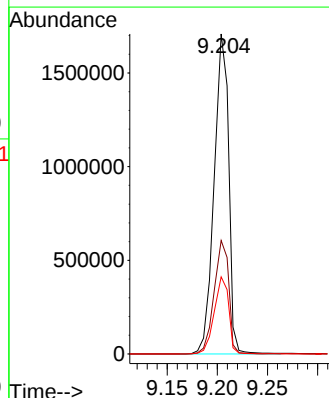
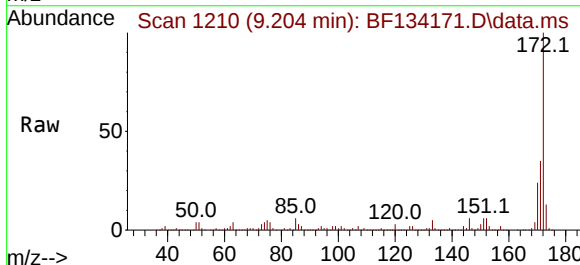




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.374 min Scan# 1
Delta R.T. -0.012 min
Lab File: BF134171.D
Acq: 09 Jul 2023 05:02




Instrument :
BNA_F
ClientSampleId :
CP-1

Tgt Ion:188 Resp: 623953
Ion Ratio Lower Upper
188 100
94 8.8 6.4 9.6
80 9.6 7.3 10.9

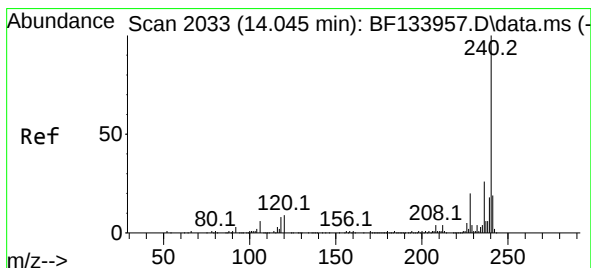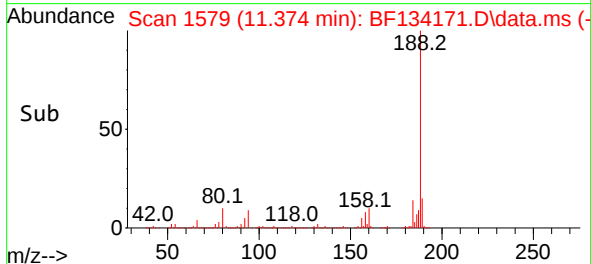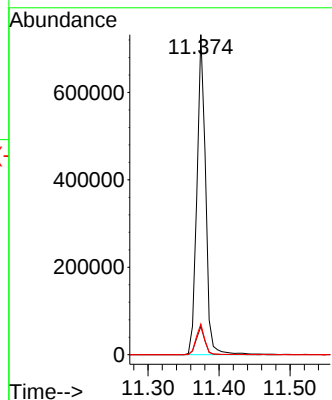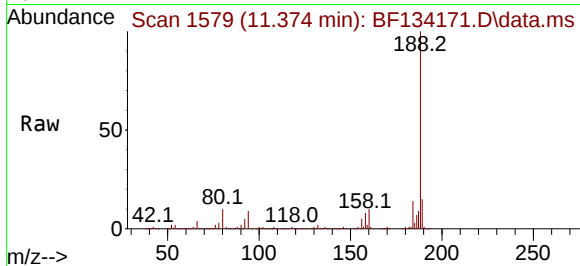

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.033 min Scan# 2031
Delta R.T. -0.018 min
Lab File: BF134171.D
Acq: 09 Jul 2023 05:02

Tgt Ion:240 Resp: 409771
Ion Ratio Lower Upper
240 100
120 11.3 7.4 11.0#
236 25.8 21.0 31.6


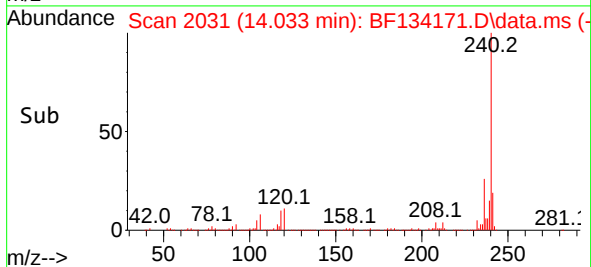
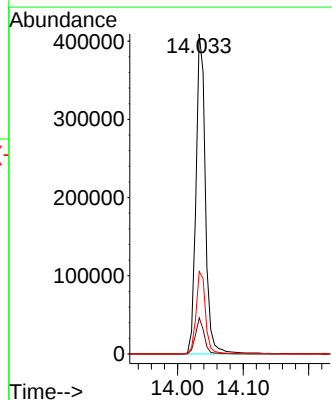
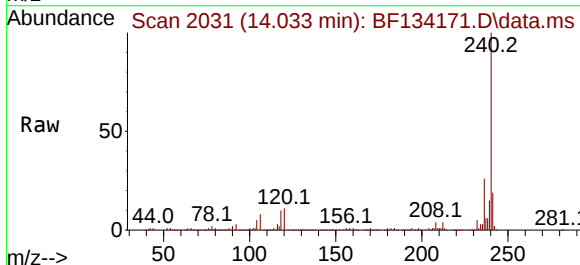




#79
 Terphenyl-d14
 Concen: 86.459 ng
 RT: 12.980 min Scan# 11
 Delta R.T. -0.006 min
 Lab File: BF134171.D
 Acq: 09 Jul 2023 05:02

Instrument :
 BNA_F
 ClientSampleId :
 CP-1

Tgt Ion:244 Resp: 2201307
 Ion Ratio Lower Upper
 244 100
 212 6.7 6.0 9.0
 122 8.6 8.3 12.5

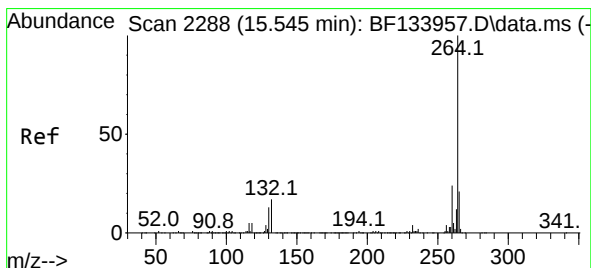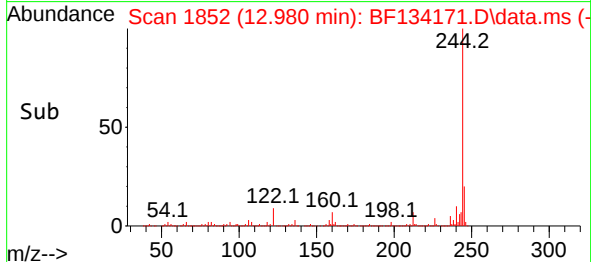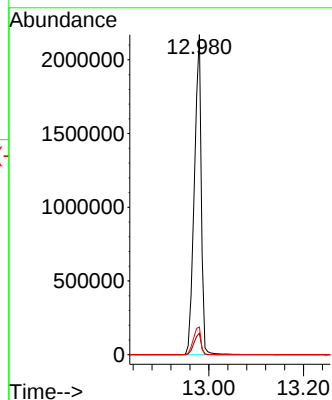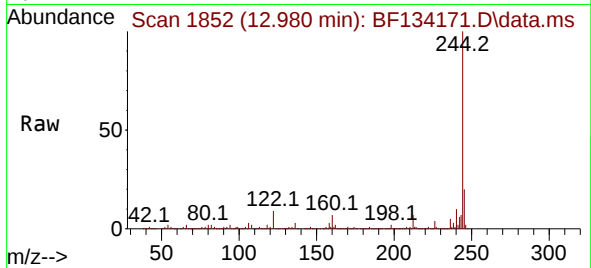

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.539 min Scan# 2287
 Delta R.T. -0.012 min
 Lab File: BF134171.D
 Acq: 09 Jul 2023 05:02

Tgt Ion:264 Resp: 359229
 Ion Ratio Lower Upper
 264 100
 260 23.1 19.5 29.3
 265 21.7 16.6 25.0

