


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070823\
Data File : BF134142.D
Acq On : 08 Jul 2023 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 30 18:35:29 2023

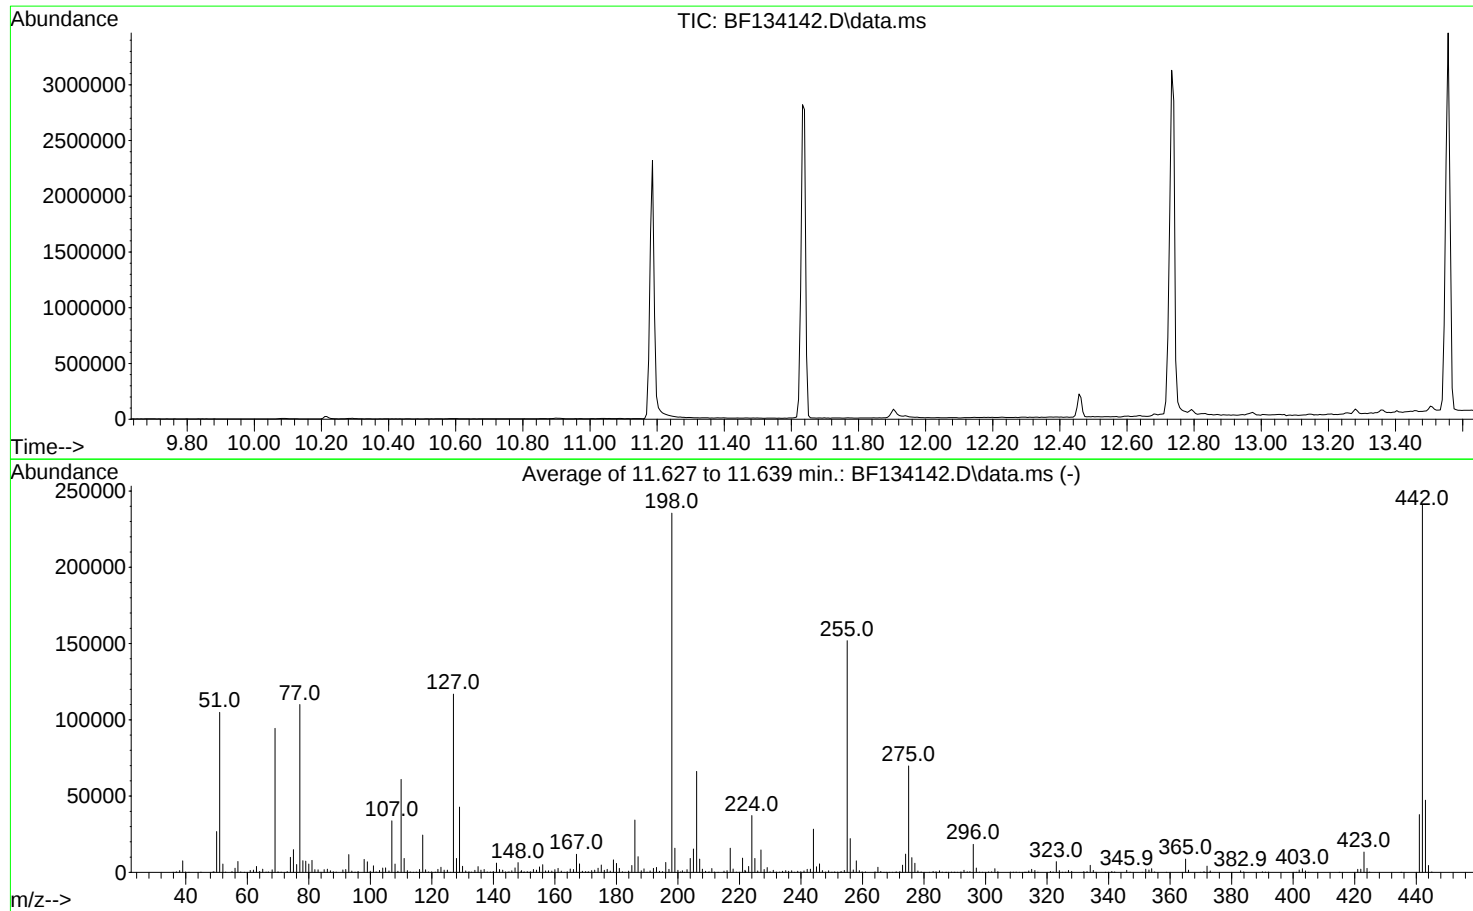




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	104896	PASS
68	69	0.00	2	1.7	1635	PASS
69	198	0.00	100	40.1	94367	PASS
70	69	0.00	2	0.3	268	PASS
127	198	10	80	49.6	116899	PASS
197	198	0.00	2	0.8	1948	PASS
198	198	100	100	100.0	235496	PASS
199	198	5	9	6.7	15886	PASS
275	198	10	60	29.6	69757	PASS
365	198	1	100	3.7	8732	PASS
441	198	0.01	100	16.1	37877	PASS
442	442	50	100	100.0	241160	PASS
443	442	15	24	19.6	47357	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070823\
 Data File : BF134142.D
 Acq On : 08 Jul 2023 11:29
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 08 12:56:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 30 18:35:29 2023
 Response via : Initial Calibration

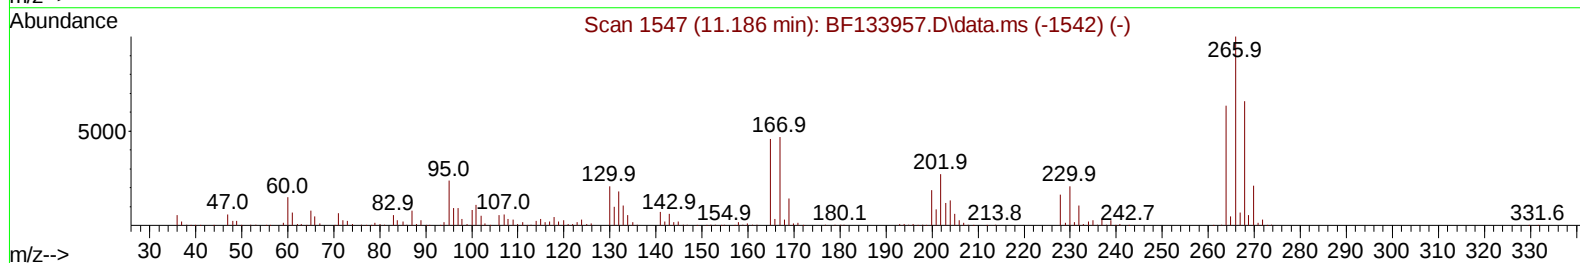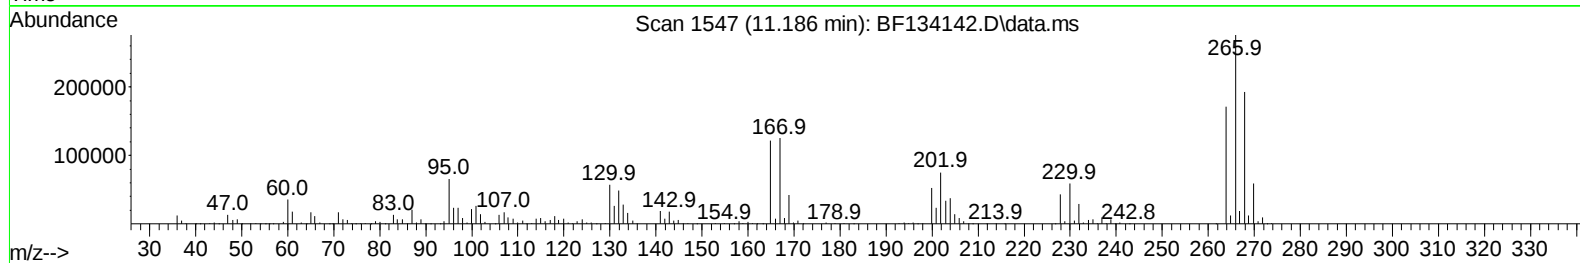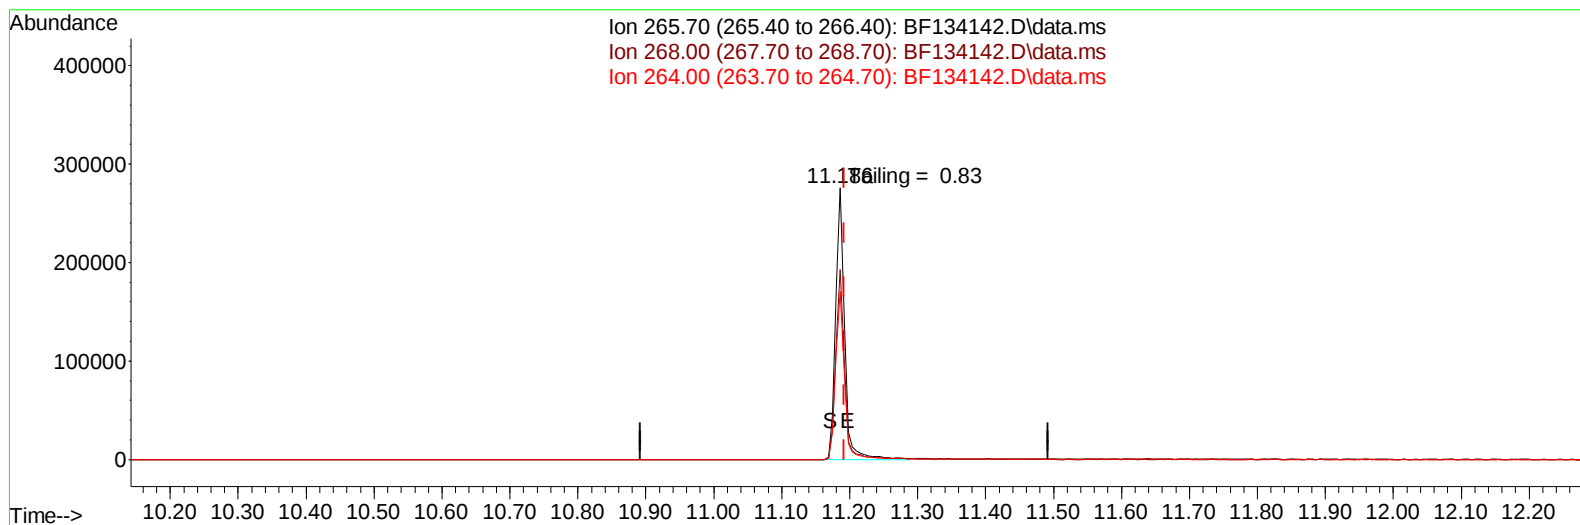

TIC: BF134142.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 27958.42 ng




response 251476

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	69.95
264.00	63.30	61.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070823\
Data File : BF134142.D
Acq On : 08 Jul 2023 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 08 12:56:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

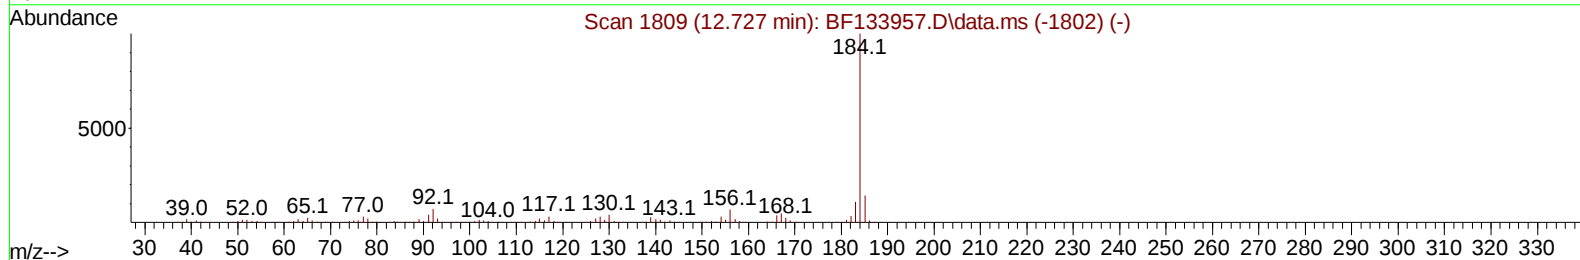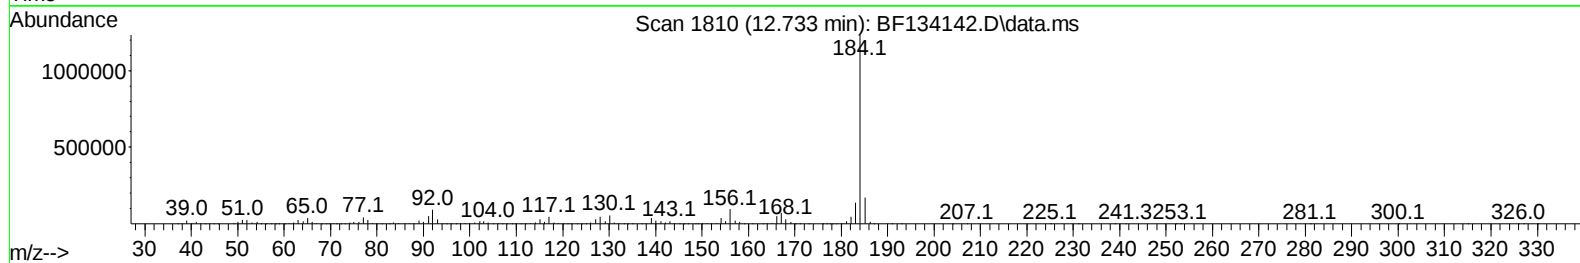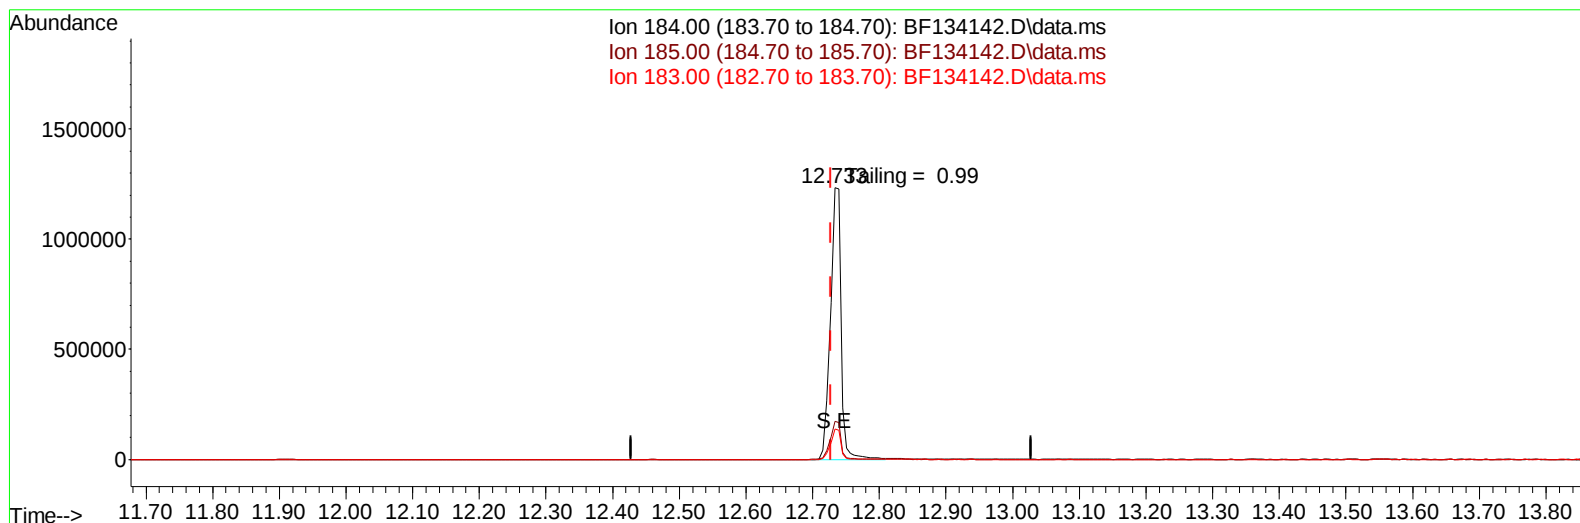

TIC: BF134142.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 23885.38 ng

response 1383332

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.99
183.00	11.00	11.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/6/2023	BNA_F	<u>BF134142.D</u>
Compound Name	Response	Retention Time
DDT	588527	13.557
DDD	8726	13.28
DDE	551	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9277	597804	1.55

Instrument :
BNA_F
ClientSampleId :
DFTPP