


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070823\
Data File : BF134162.D
Acq On : 08 Jul 2023 23:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 30 18:35:29 2023

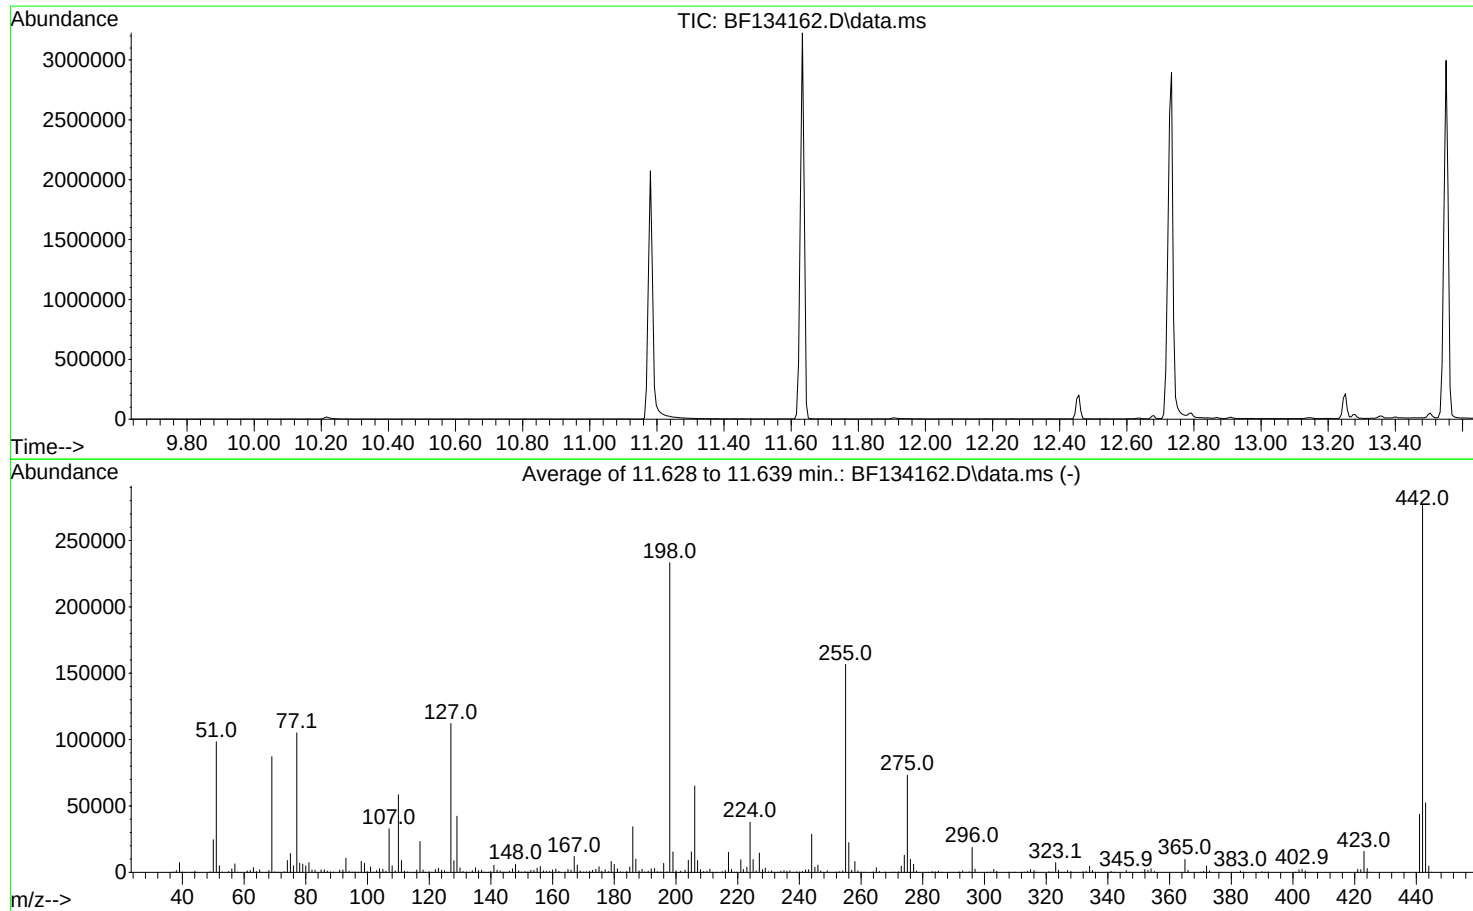




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.2	98371	PASS
68	69	0.00	2	1.7	1474	PASS
69	198	0.00	100	37.4	87125	PASS
70	69	0.00	2	0.5	460	PASS
127	198	10	80	48.1	112149	PASS
197	198	0.00	2	0.2	509	PASS
198	198	100	100	100.0	233237	PASS
199	198	5	9	6.6	15377	PASS
275	198	10	60	31.4	73205	PASS
365	198	1	100	4.2	9791	PASS
441	198	0.01	100	18.8	43757	PASS
442	442	50	100	100.0	277096	PASS
443	442	15	24	18.9	52301	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070823\
Data File : BF134162.D
Acq On : 08 Jul 2023 23:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 09 02:30:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

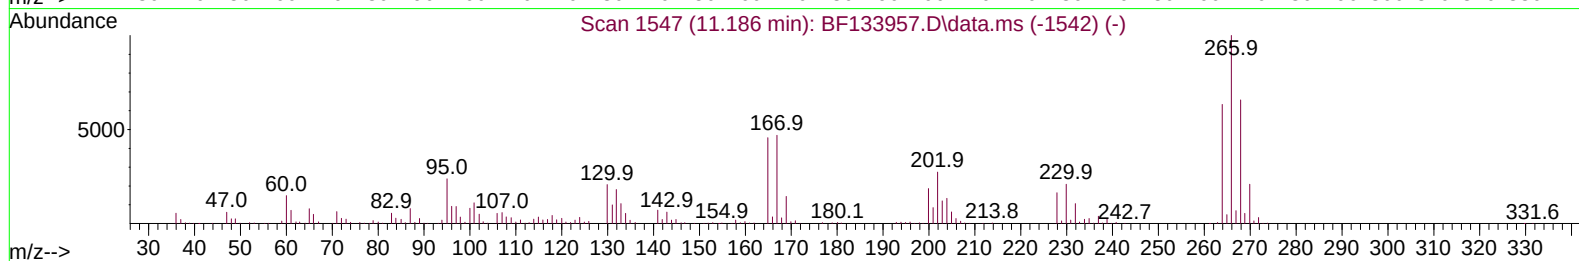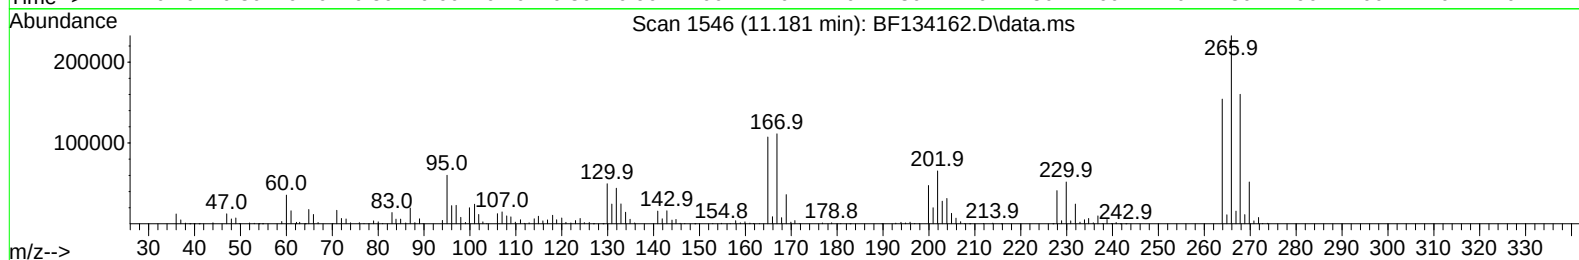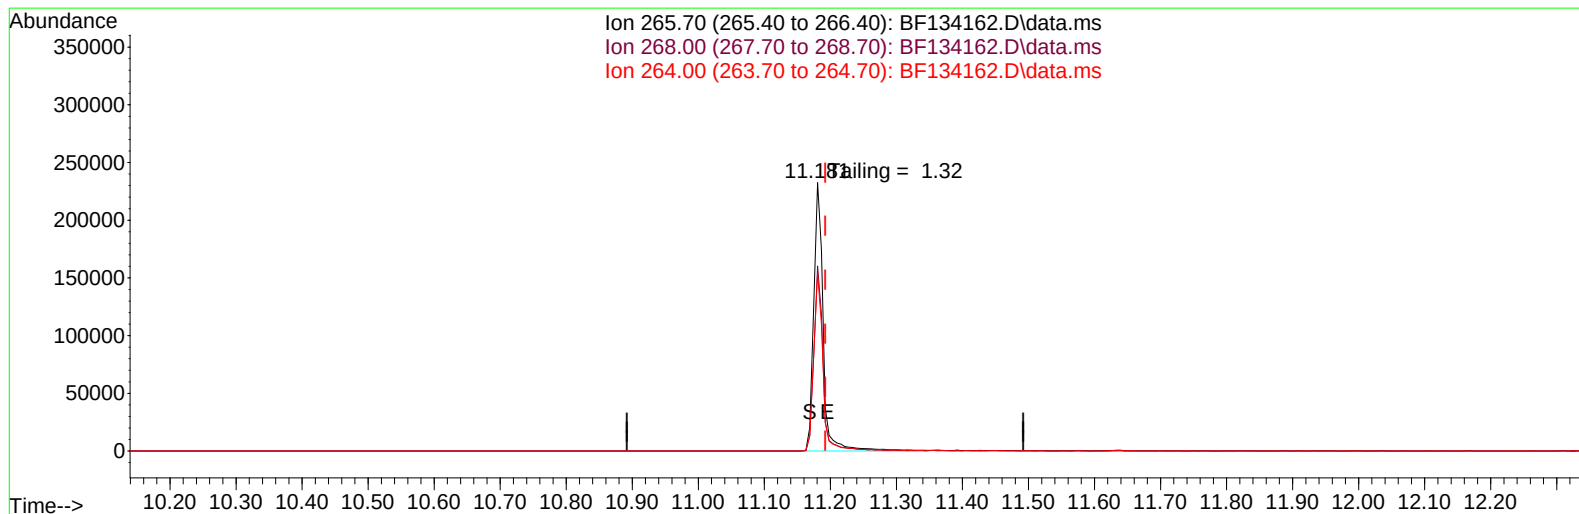

TIC: BF134162.D\data.ms

(70) Pentachlorophenol (C)

11.181min (-0.012) 131675.95 ng




response 231900

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	68.90
264.00	63.30	66.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070823\
Data File : BF134162.D
Acq On : 08 Jul 2023 23:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 09 02:30:51 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 30 18:35:29 2023
Response via : Initial Calibration

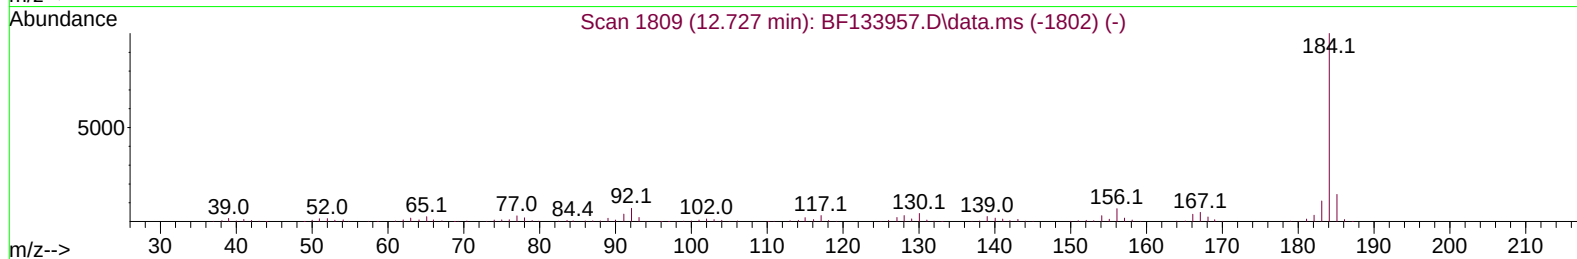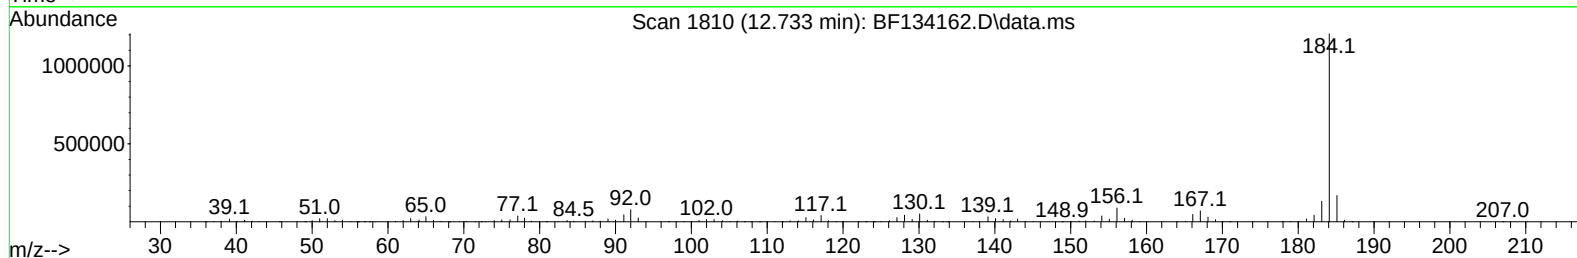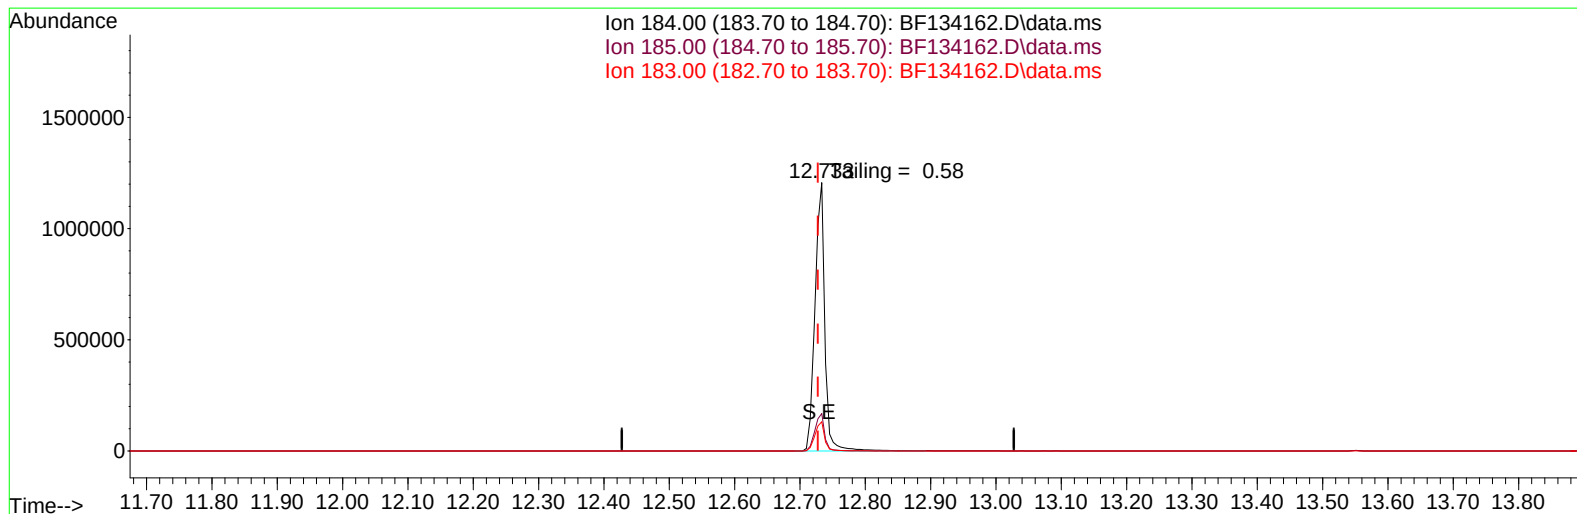

TIC: BF134162.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 98152.51 ng

response 1261156

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.99
183.00	11.00	10.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/8/2023	BNA_F	<u>BF134162.D</u>
Compound Name	Response	Retention Time
DDT	519650	13.551
DDD	42334	13.251
DDE	1763	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
44097	563747	7.82

Instrument :
BNA_F
ClientSampleId :
DFTPP