


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF070915\
 Data File : BF080401.D
 Acq On : 9 Jul 2015 14:27
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF070615.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 07 03:05:40 2015

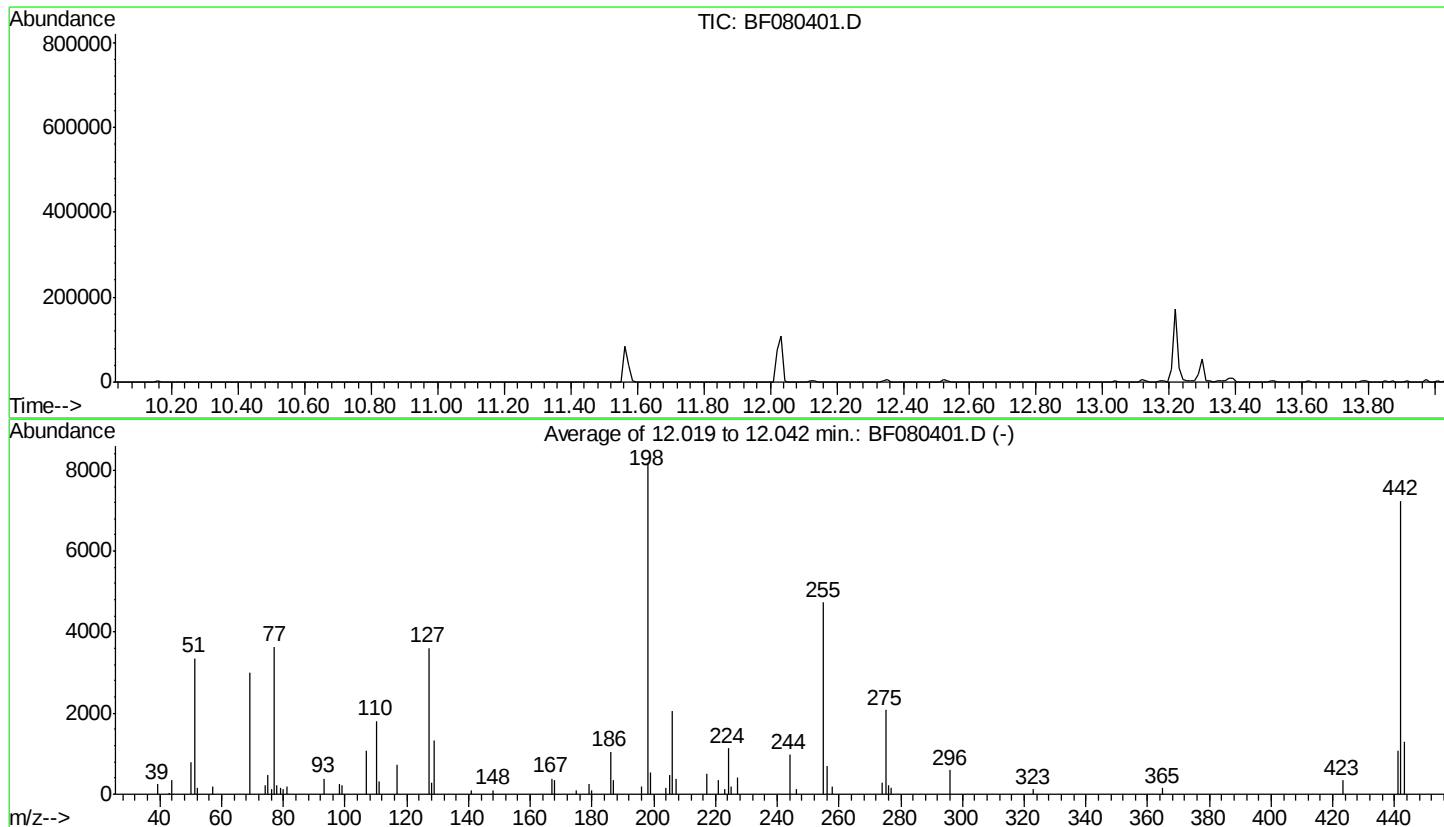

AutoFind: Scans 869, 870, 871; Background Corrected with Scan 866

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	3365	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.8	3012	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	3618	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	8186	PASS
199	198	5	9	6.7	546	PASS
275	198	10	60	25.3	2072	PASS
365	198	1	100	1.9	156	PASS
441	442	0.01	24	14.8	1069	PASS
442	198	50	100	88.5	7244	PASS
443	442	15	24	18.1	1308	PASS