


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070918\
 Data File : BF107220.D
 Acq On : 9 Jul 2018 11:23
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 29 14:38:29 2018

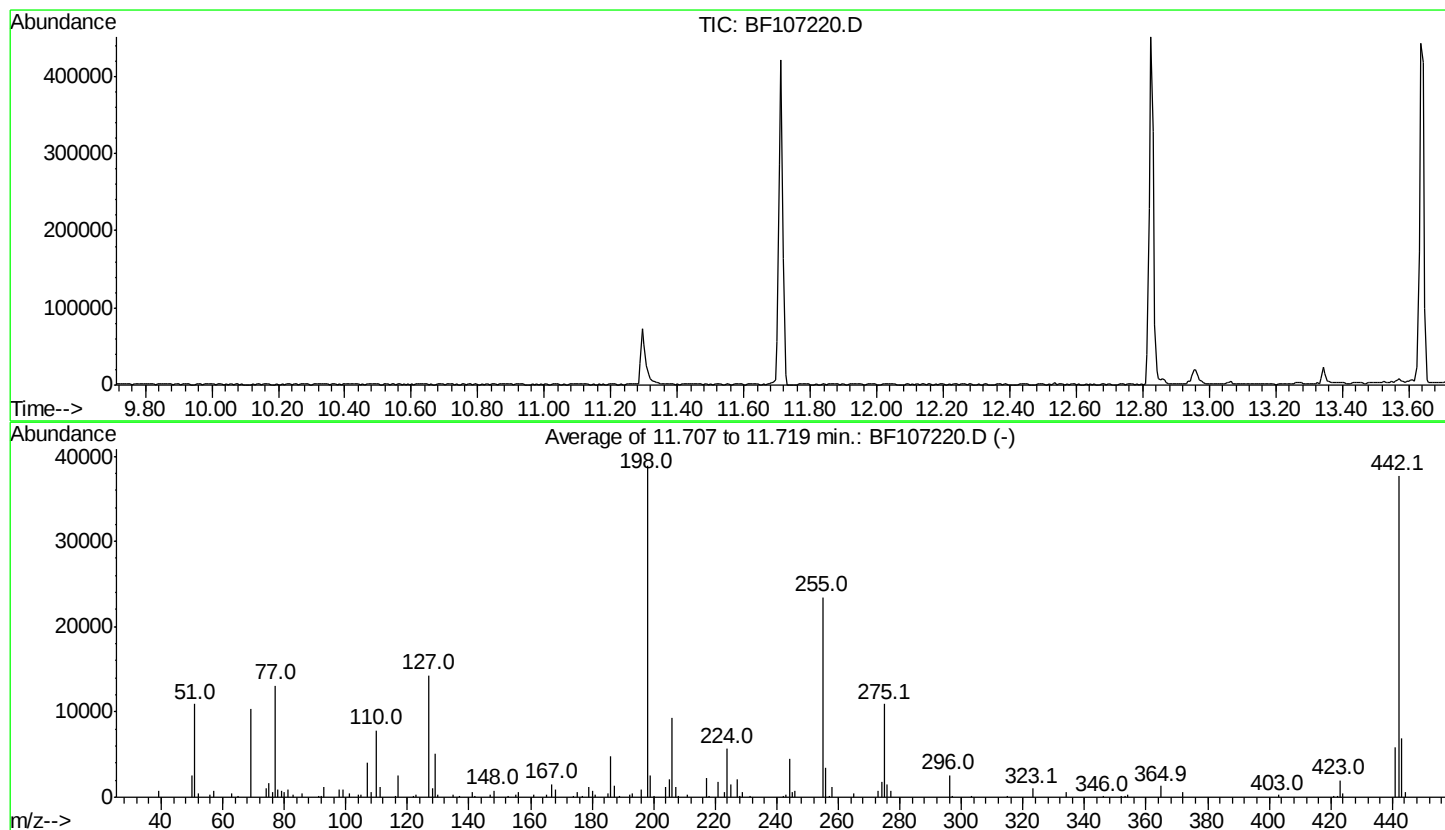

AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.1	10940	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.7	10382	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.8	14304	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38885	PASS
199	198	5	9	6.6	2565	PASS
275	198	10	60	28.1	10935	PASS
365	198	1	100	3.4	1312	PASS
441	198	0.01	100	15.0	5846	PASS
442	198	50	100	96.9	37680	PASS
443	442	15	24	18.3	6908	PASS