


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF070918\
 Data File : BF107248.D
 Acq On : 10 Jul 2018 00:28
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampled :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 29 14:38:29 2018

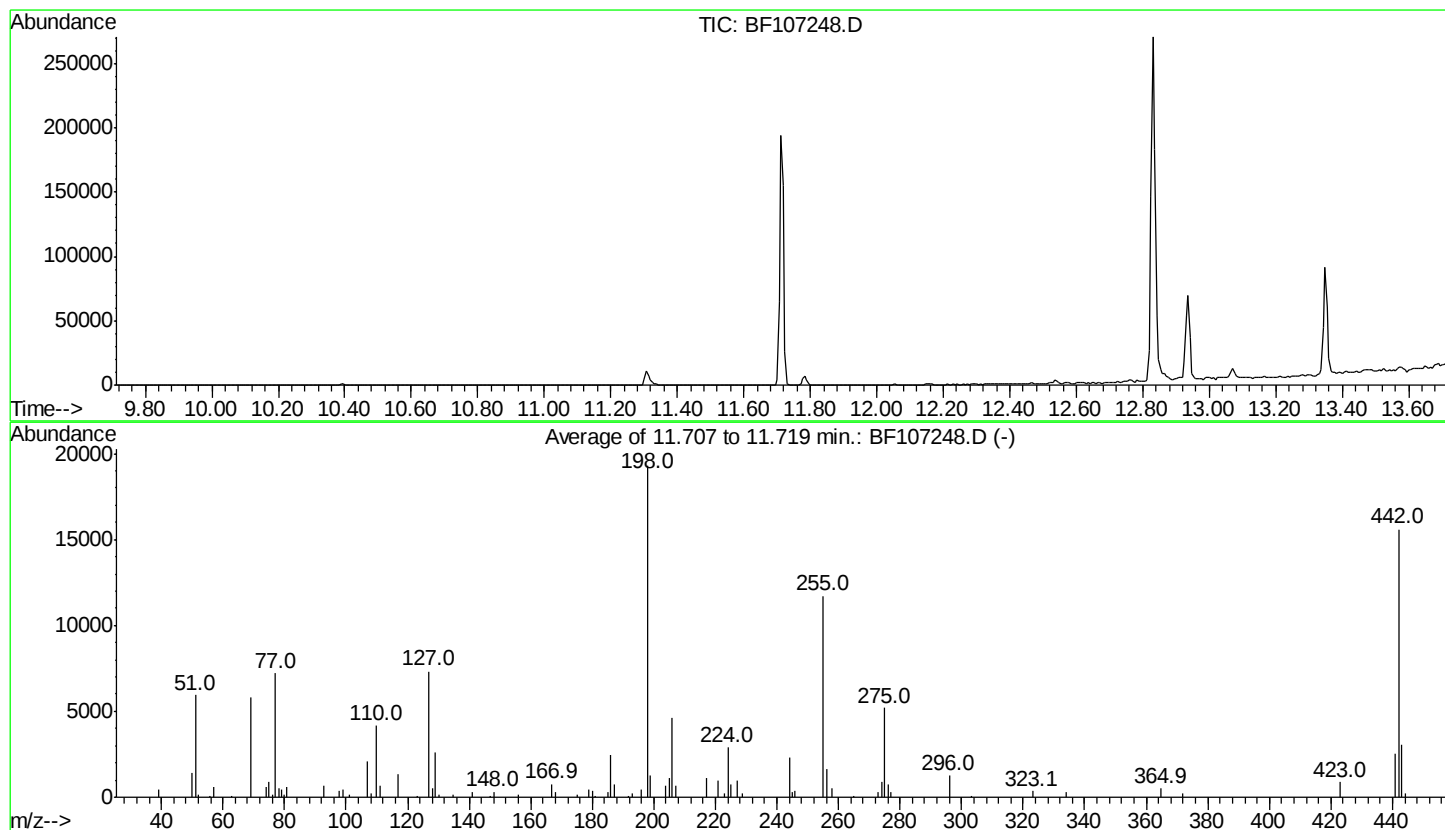

AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	5955	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.9	5778	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	38.0	7323	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19295	PASS
199	198	5	9	6.7	1295	PASS
275	198	10	60	26.9	5199	PASS
365	198	1	100	2.6	498	PASS
441	198	0.01	100	13.2	2544	PASS
442	198	50	100	80.8	15582	PASS
443	442	15	24	19.6	3049	PASS