

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071018\
 Data File : BF107293.D
 Acq On : 11 Jul 2018 1:25
 Operator : JU/SJ
 Sample : J3907-02
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 S-2

Quant Time: Jul 11 02:27:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 29 14:38:29 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	25922	20.00	ng	-0.02
21) Naphthalene-d8	8.22	136	90159	20.00	ng	-0.02
38) Acenaphthene-d10	9.98	164	43570	20.00	ng	-0.02
63) Phenanthrene-d10	11.48	188	91024	20.00	ng	-0.02
75) Chrysene-d12	14.14	240	74526	20.00	ng	-0.03
86) Perylene-d12	15.67	264	55163	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.58	112	201828	131.84	ng	-0.02
7) Phenol-d6	6.58	99	236932	123.94	ng	-0.03
23) Nitrobenzene-d5	7.50	82	132929	81.94	ng	-0.04
41) 2,4,6-Tribromophenol	10.78	330	67033	132.74	ng	-0.02
44) 2-Fluorobiphenyl	9.30	172	251534	100.39	ng	-0.03
78) Terphenyl-d14	13.06	244	333561	108.42	ng	-0.02
Target Compounds						
10) Phenol	6.60	94	5334	2.445	ng	Qvalue # 50
49) Dimethylphthalate	9.69	163	56494	17.288	ng	99
83) Bis(2-ethylhexyl)phthalate	14.07	149	8173	3.164	ng	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF071018\
Data File : BF107293.D
Acq On : 11 Jul 2018 1:25
Operator : JU/SJ
Sample : J3907-02
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
S-2

Quant Time: Jul 11 02:27:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF061918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 29 14:38:29 2018
Response via : Initial Calibration

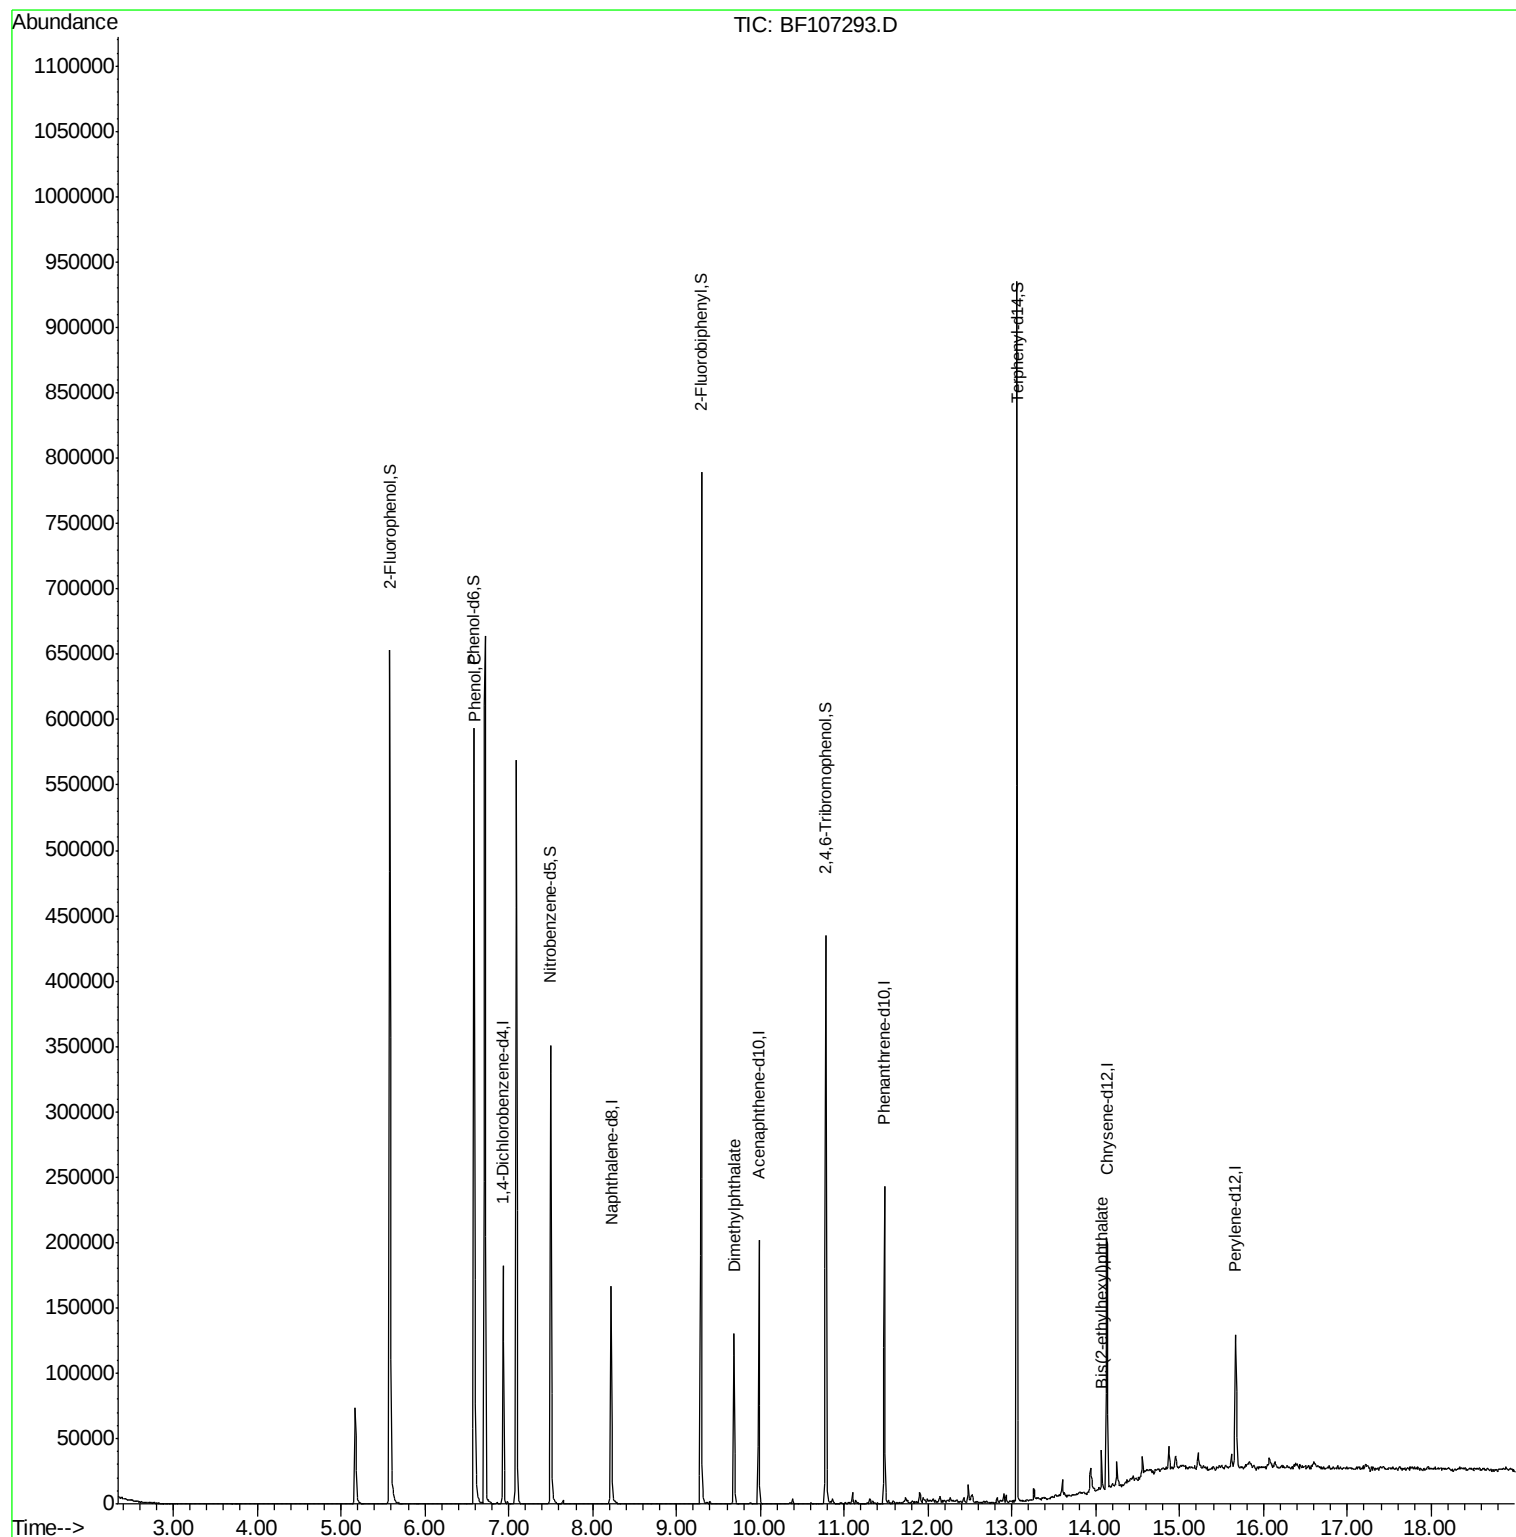

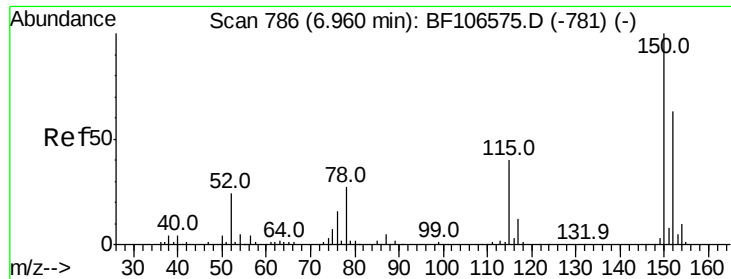


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.94 min Scan# 782
Delta R.T. -0.02 min
Lab File: BF107293.D
Acq: 11 Jul 2018 1:25

Instrument :
BNA_F
ClientSampleId :
S-2

Tot Ion:152 Resp: 25922
Ion Ratio Lower Upper
152 100
150 159.8 124.6 186.8
115 59.3 50.1 75.1

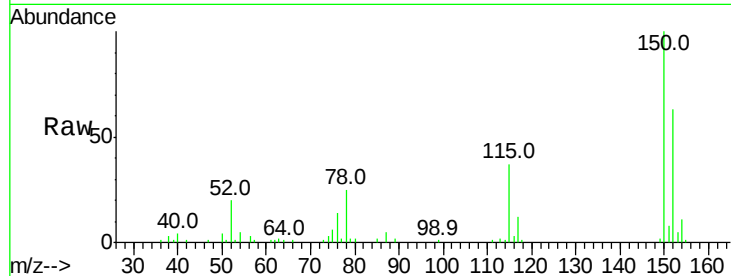


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

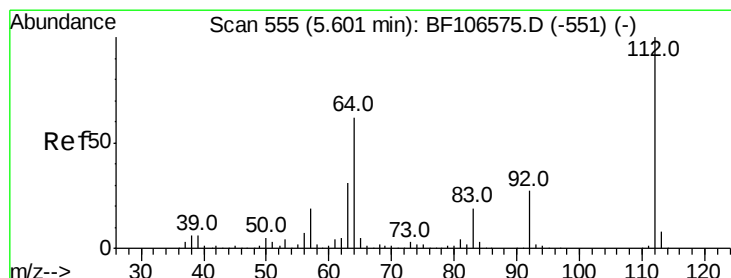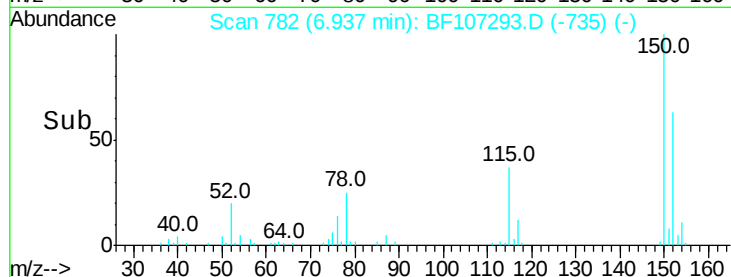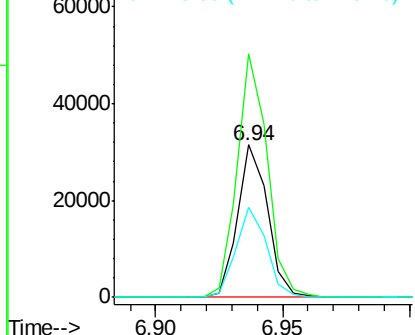



#5


2-Fluorophenol
Concen: 131.841 ng
RT: 5.58 min Scan# 552
Delta R.T. -0.02 min
Lab File: BF107293.D
Acq: 11 Jul 2018 1:25

Tgt Ion:112 Resp: 201828
Ion Ratio Lower Upper
112 100
64 58.8 47.9 71.9
63 27.9 23.7 35.5

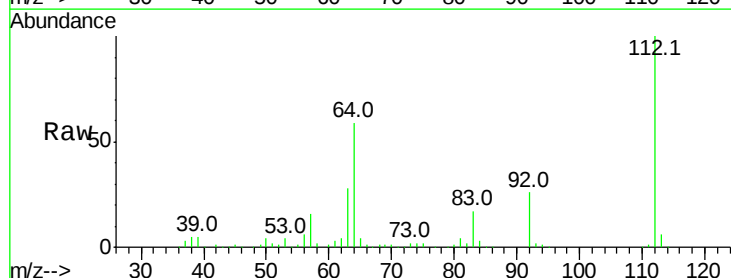

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

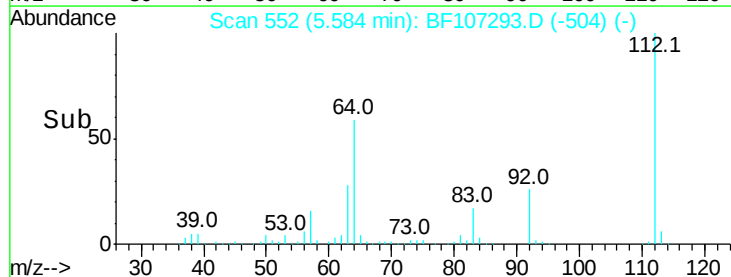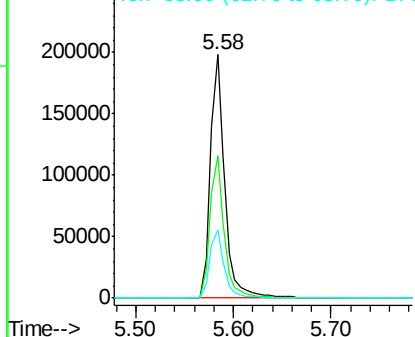

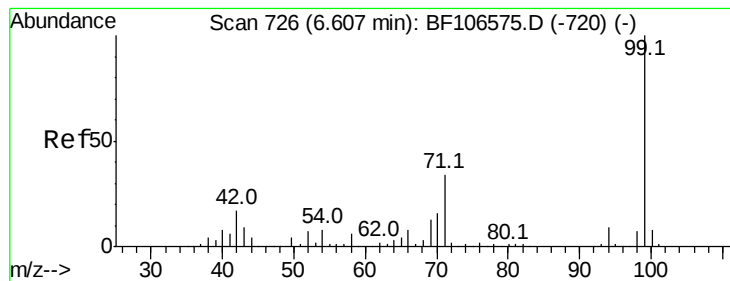

#7

Phenol-d6

Concen: 123.936 ng

RT: 6.58 min Scan# 722

Delta R.T. -0.03 min

Lab File: BF107293.D

Acq: 11 Jul 2018 1:25

Instrument :

BNA_F

ClientSampled :

S-2


Tot Ion: 99 Resp: 236932

Ion Ratio Lower Upper




99 100

42 16.3 14.5 21.7

71 33.5 25.4 38.0

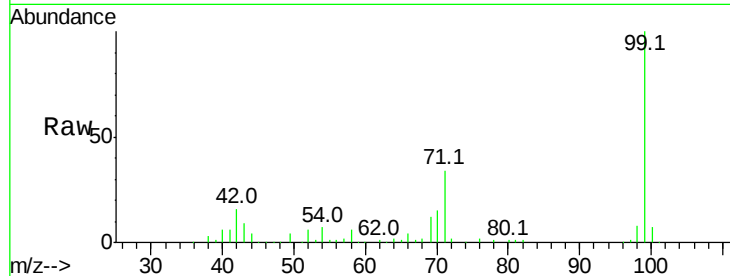

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

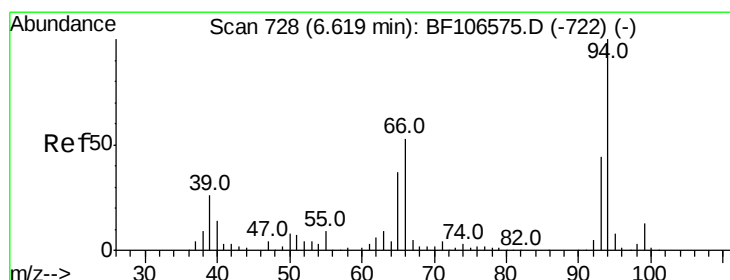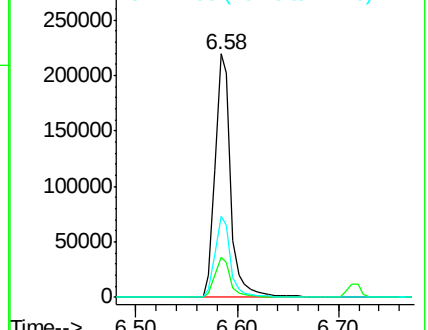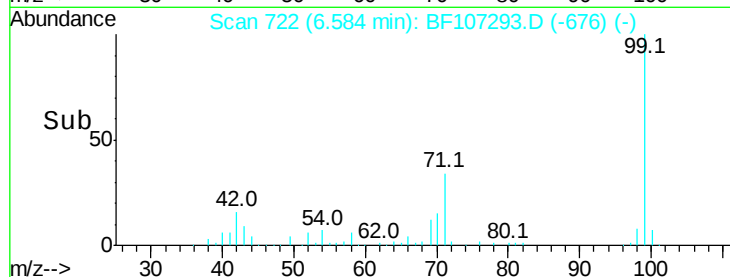

#10

Phenol

Concen: 2.445 ng

RT: 6.60 min Scan# 724

Delta R.T. -0.03 min

Lab File: BF107293.D

Acq: 11 Jul 2018 1:25


Tgt Ion: 94 Resp: 5334

Ion Ratio Lower Upper



94 100


65 40.3 7.9 47.9

66 77.2 16.2 56.2#

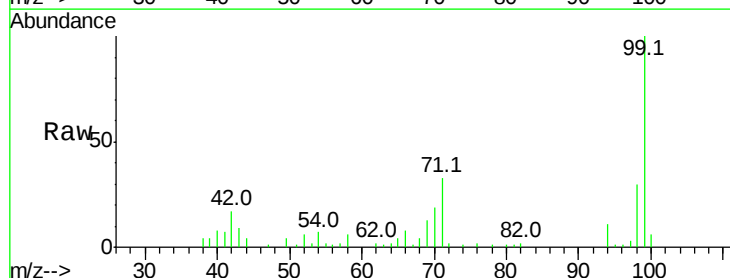

Abundance Ion 94.00 (93.70 to 94.70): BF1
Ion 65.00 (64.70 to 65.70): BF1
Ion 66.00 (65.70 to 66.70): BF1

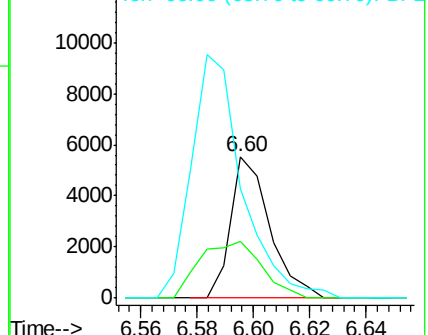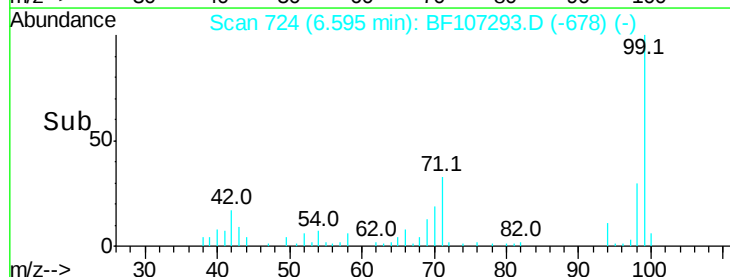


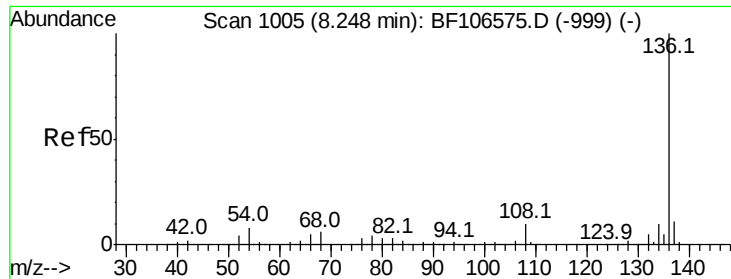




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.22 min Scan# 1001
Delta R.T. -0.02 min
Lab File: BF107293.D
Acq: 11 Jul 2018 1:25

Instrument :
BNA_F
ClientSampled :
S-2

Tot Ion:	136	Resp:	90159
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.9	13.3
54	7.8	6.6	9.8
68	6.0	5.0	7.4

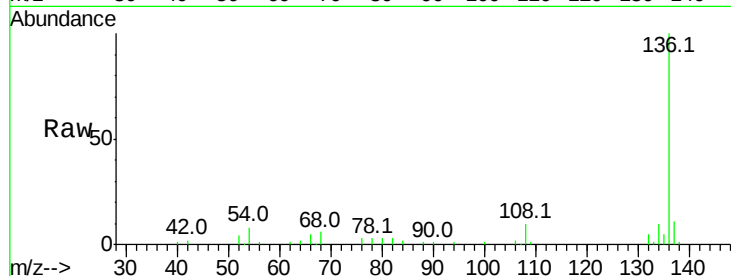


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

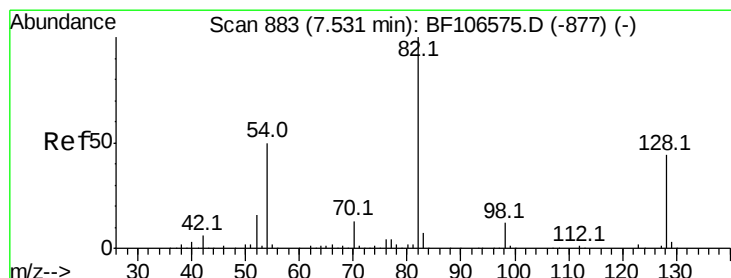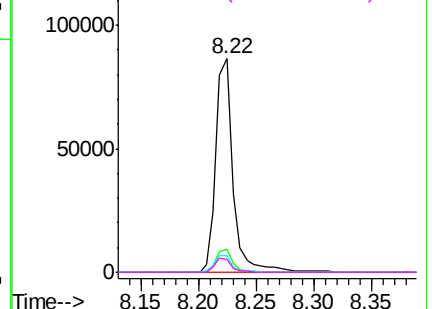
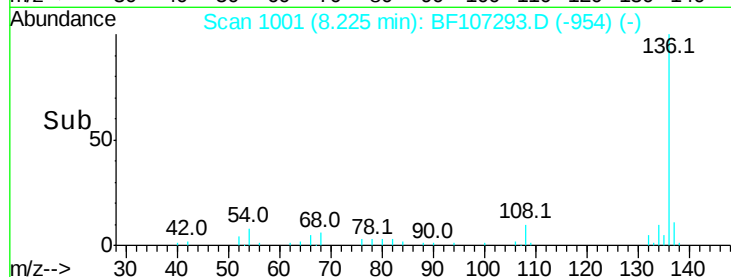



#23
Nitrobenzene-d5
Concen: 81.937 ng
RT: 7.50 min Scan# 878
Delta R.T. -0.04 min
Lab File: BF107293.D
Acq: 11 Jul 2018 1:25

Tgt Ion:	82	Resp:	132929
Ion	Ratio	Lower	Upper
82	100		
128	43.6	36.1	54.1
54	49.1	41.4	62.2

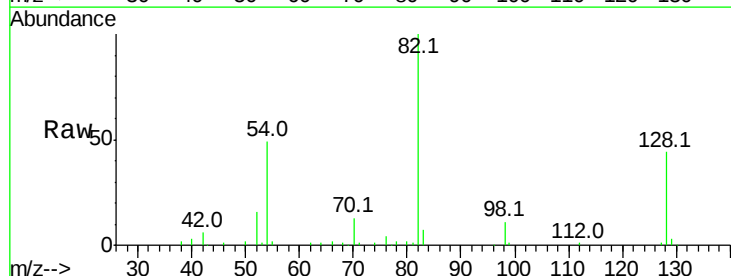

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1



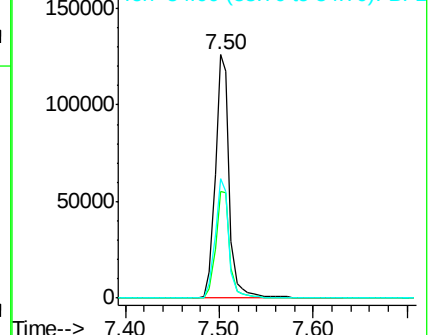
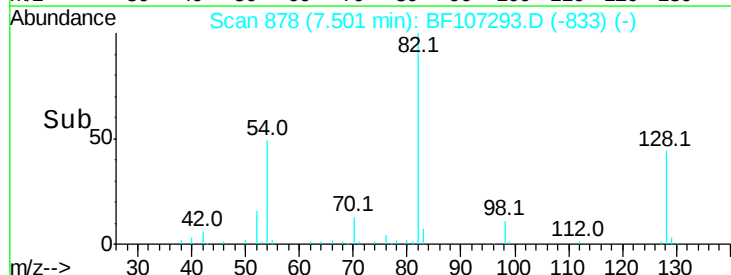


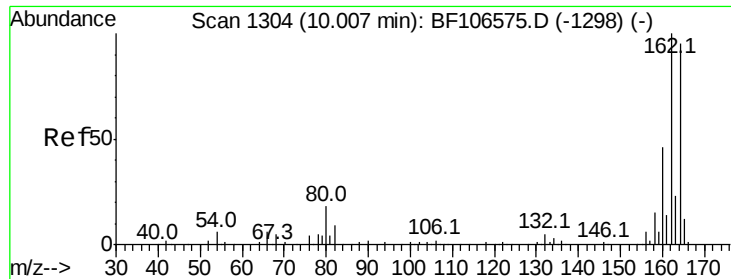

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.98 min Scan# 1300
Delta R.T. -0.02 min
Lab File: BF107293.D
Acq: 11 Jul 2018 1:25




Instrument :
BNA_F
ClientSampleId :
S-2


Tot Ion:164 Resp: 43570
Ion Ratio Lower Upper
164 100
162 96.6 86.1 129.1
160 43.1 38.3 57.5

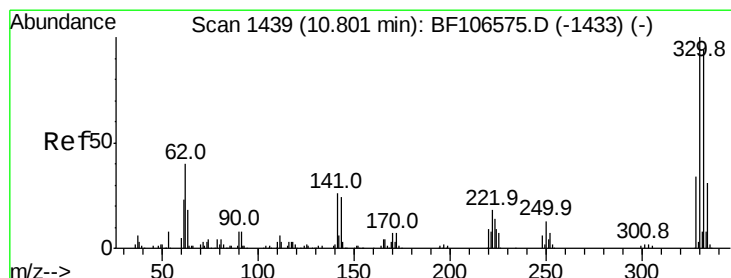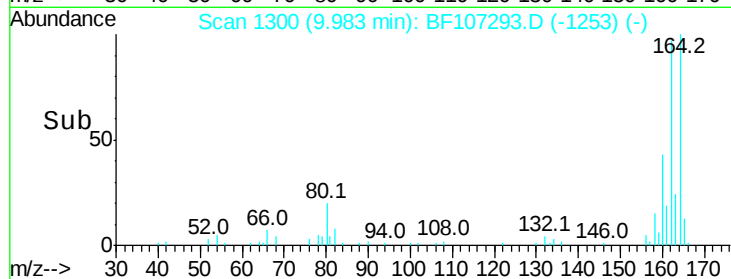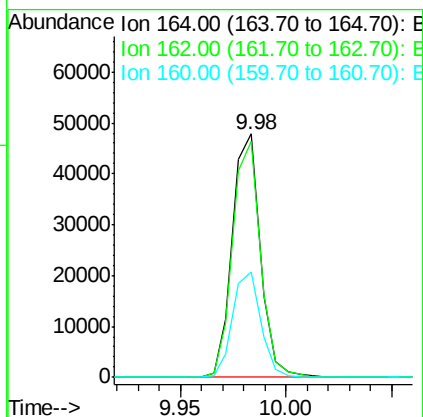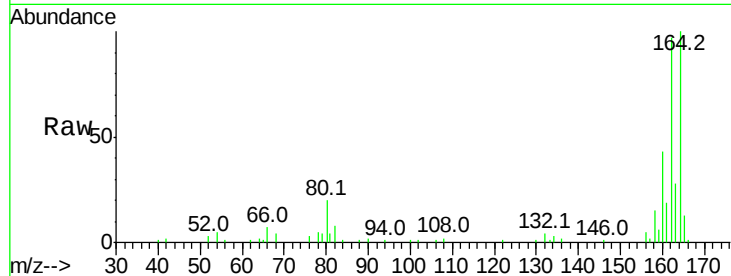

#41
2,4,6-Tribromophenol
Concen: 132.742 ng
RT: 10.78 min Scan# 1436
Delta R.T. -0.02 min
Lab File: BF107293.D
Acq: 11 Jul 2018 1:25

Tgt Ion:330 Resp: 67033
Ion Ratio Lower Upper
330 100
332 95.5 77.0 115.6
141 23.0 29.9 44.9#


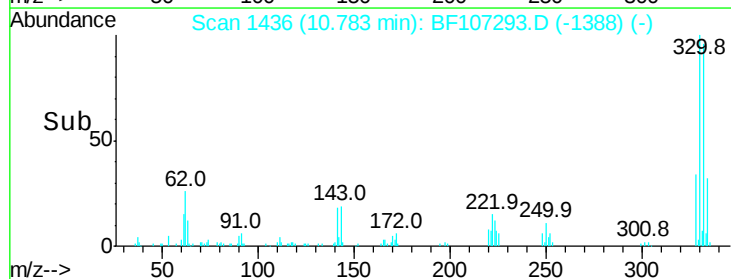
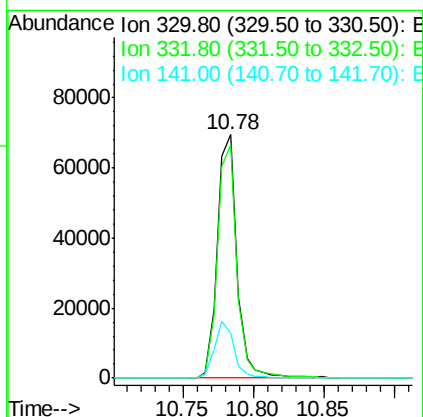
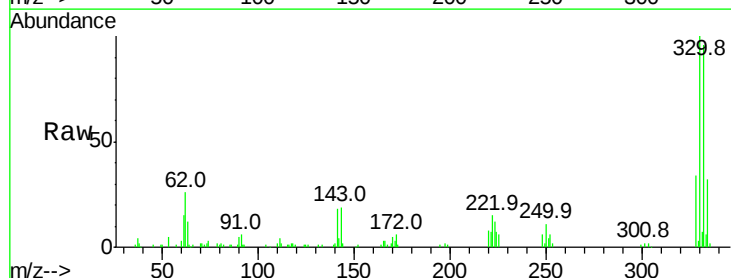


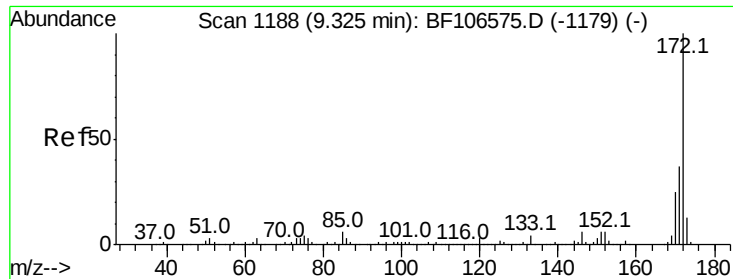

#44
2-Fluorobiphenyl
Concen: 100.387 ng
RT: 9.30 min Scan# 1183
Delta R.T. -0.03 min
Lab File: BF107293.D
Acq: 11 Jul 2018 1:25




Instrument :
BNA_F
ClientSampleId :
S-2


Tot Ion	Ratio	Lower	Upper
172	100		
171	34.6	29.7	44.5
170	23.1	19.6	29.4

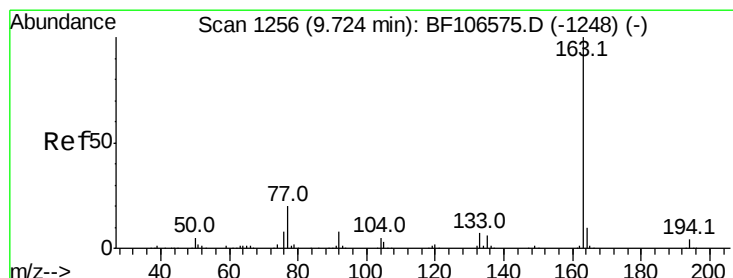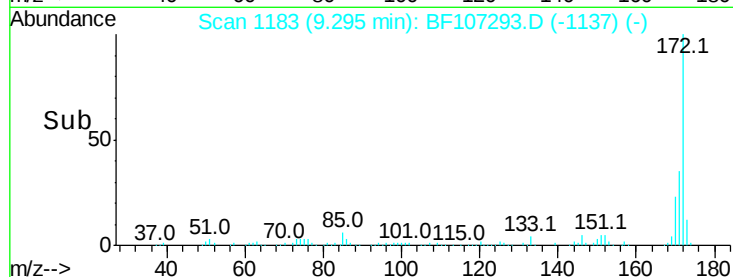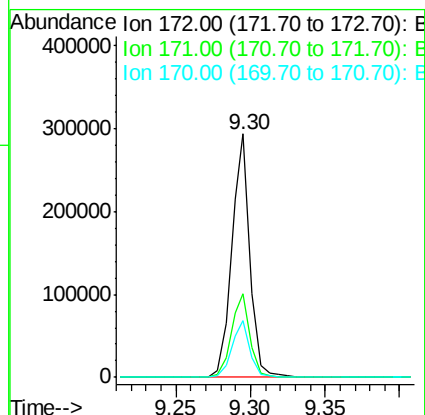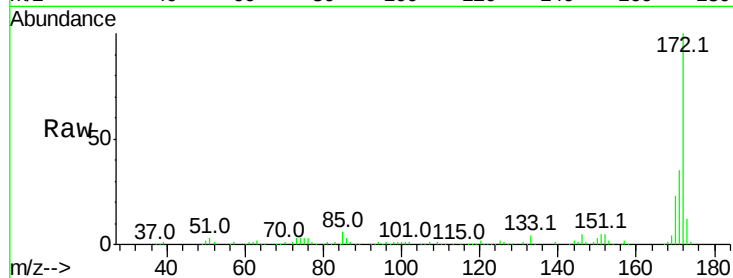

#49
Dimethylphthalate
Concen: 17.288 ng
RT: 9.69 min Scan# 1250
Delta R.T. -0.04 min
Lab File: BF107293.D
Acq: 11 Jul 2018 1:25

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	2.7	4.1
164	10.5	8.2	12.2

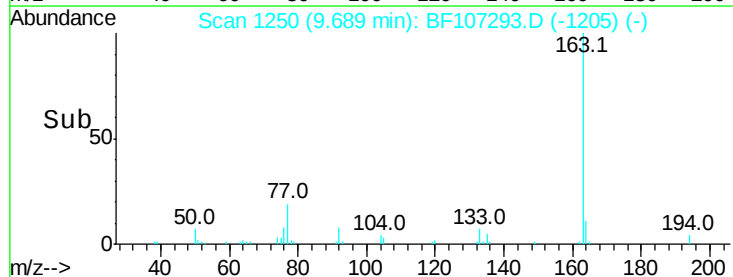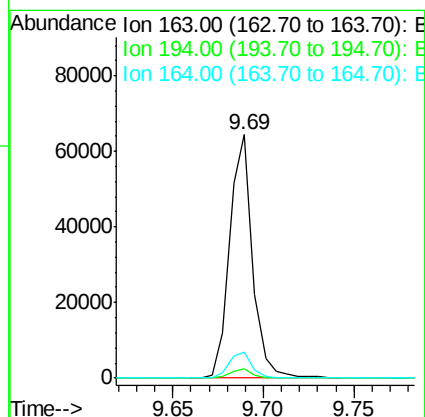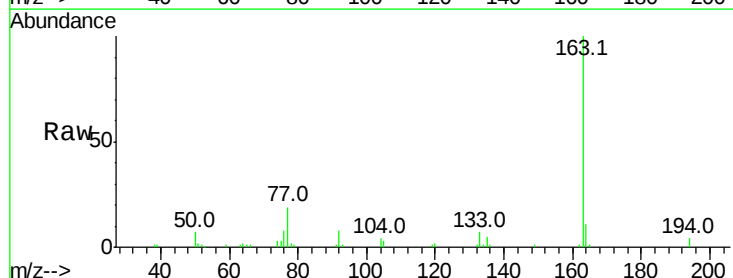

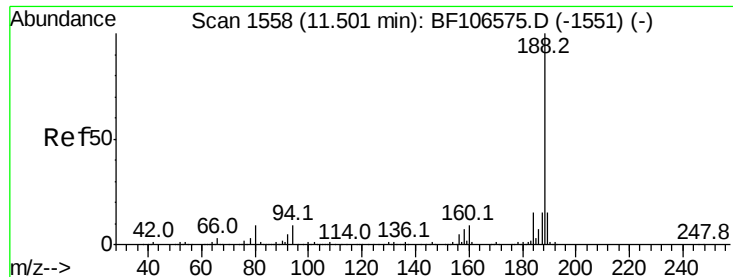

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.48 min Scan# 1554

Delta R.T. -0.02 min

Lab File: BF107293.D

Acq: 11 Jul 2018 1:25

Instrument :

BNA_F

ClientSampled :

S-2


Tot Ion:188 Resp: 91024

Ion Ratio Lower Upper

188 100

94 9.0 8.5 12.7




80 9.5 9.2 13.8

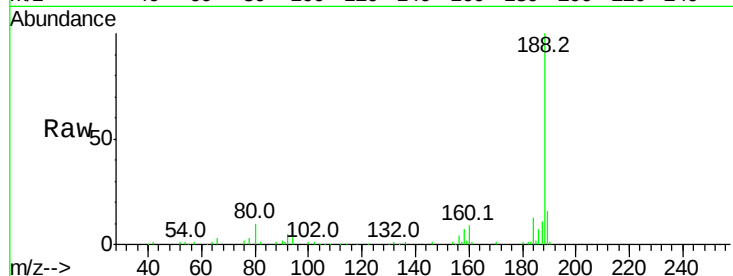

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

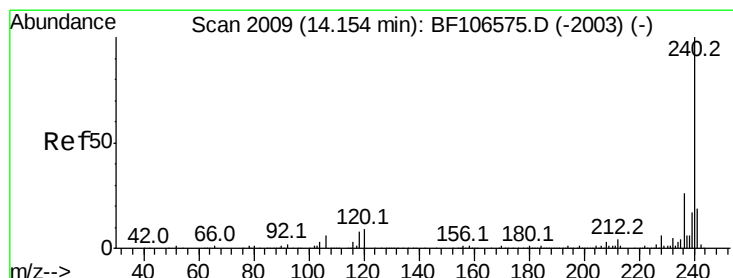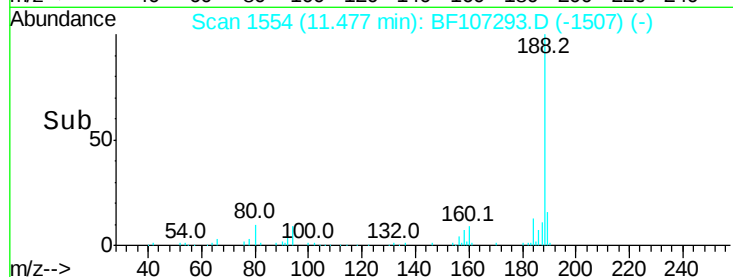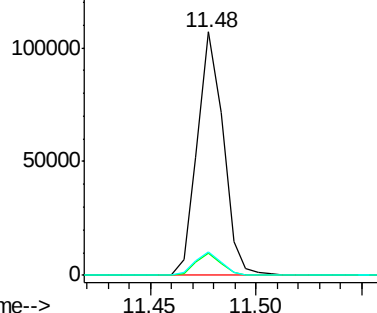

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.14 min Scan# 2006

Delta R.T. -0.03 min

Lab File: BF107293.D

Acq: 11 Jul 2018 1:25


Tgt Ion:240 Resp: 74526

Ion Ratio Lower Upper

240 100

120 8.1 9.5 14.3#



236 25.7 20.7 31.1

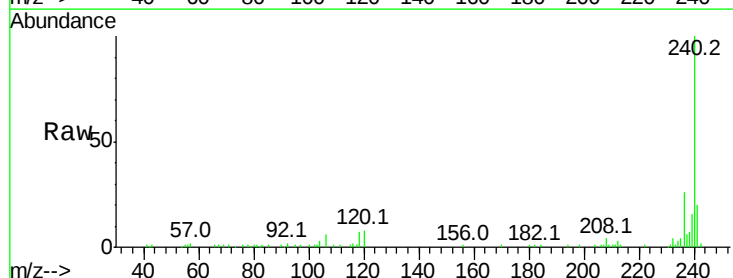


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



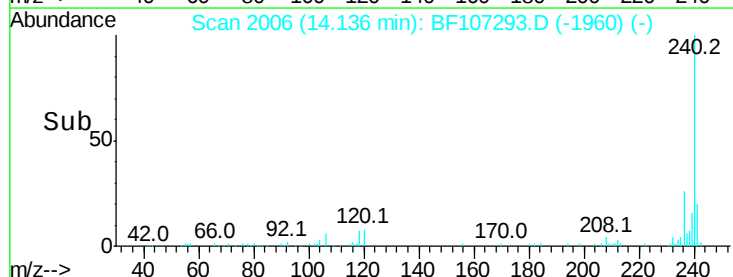
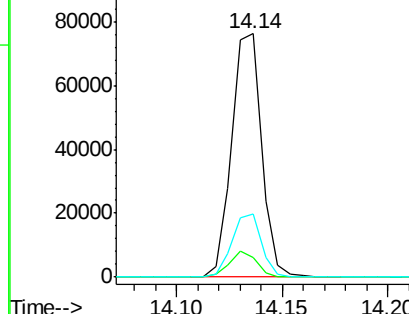


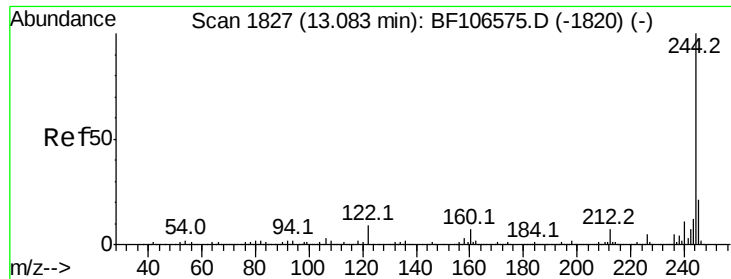

#78
 Terphenyl-d14
 Concen: 108.416 ng
 RT: 13.06 min Scan# 1823
 Delta R.T. -0.02 min
 Lab File: BF107293.D
 Acq: 11 Jul 2018 1:25




Instrument :
 BNA_F
 ClientSampleId :
 S-2


Tot Ion:244 Resp: 333561
 Ion Ratio Lower Upper
 244 100
 212 6.4 5.4 8.0
 122 9.0 11.0 16.4#

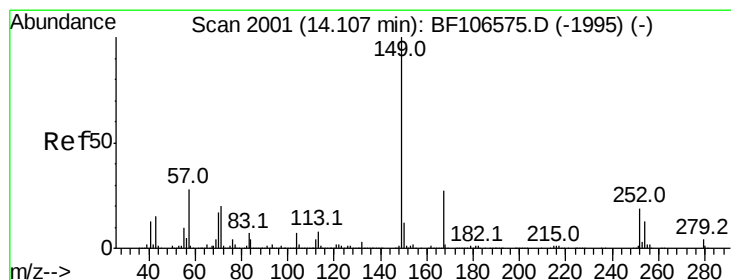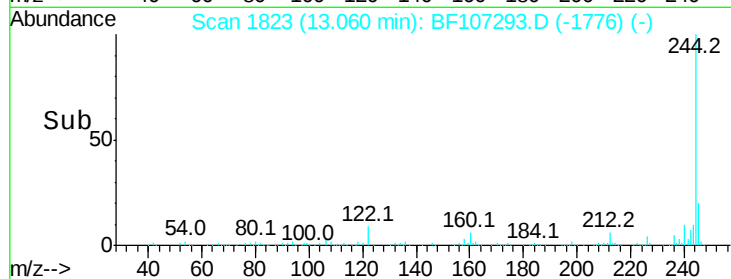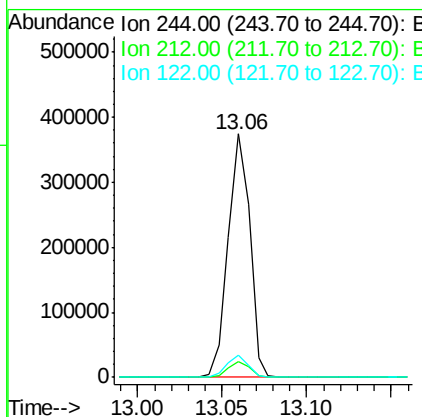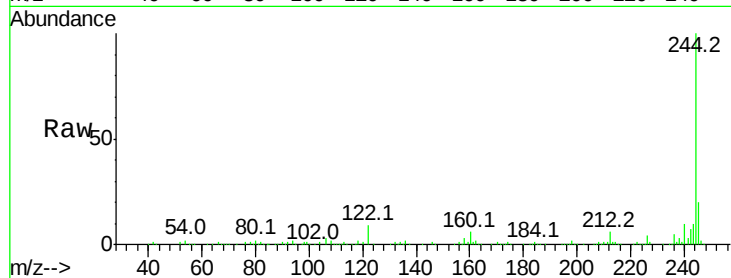

#83
 Bis(2-ethylhexyl)phthalate
 Concen: 3.164 ng
 RT: 14.07 min Scan# 1995
 Delta R.T. -0.04 min
 Lab File: BF107293.D
 Acq: 11 Jul 2018 1:25

Tgt Ion:149 Resp: 8173
 Ion Ratio Lower Upper
 149 100
 167 29.0 21.3 31.9
 279 3.9 3.0 4.4

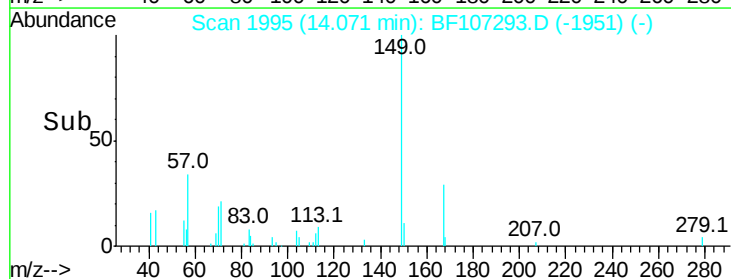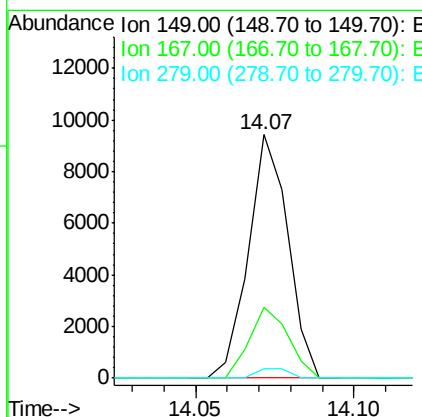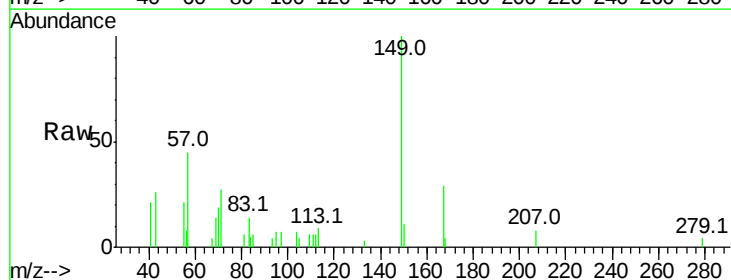


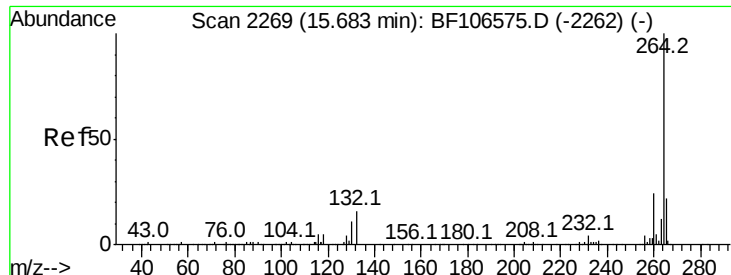

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.67 min Scan# 2266
 Delta R.T. -0.05 min
 Lab File: BF107293.D
 Acq: 11 Jul 2018 1:25

Instrument :
 BNA_F
 ClientSampleId :
 S-2

Tot Ion:264 Resp: 55163
 Ion Ratio Lower Upper
 264 100
 260 23.3 19.2 28.8
 265 22.0 17.5 26.3

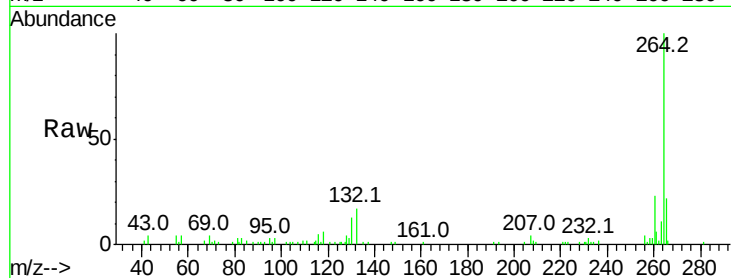

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

