


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071018\
 Data File : BF107261.D
 Acq On : 10 Jul 2018 10:01
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jun 29 14:38:29 2018

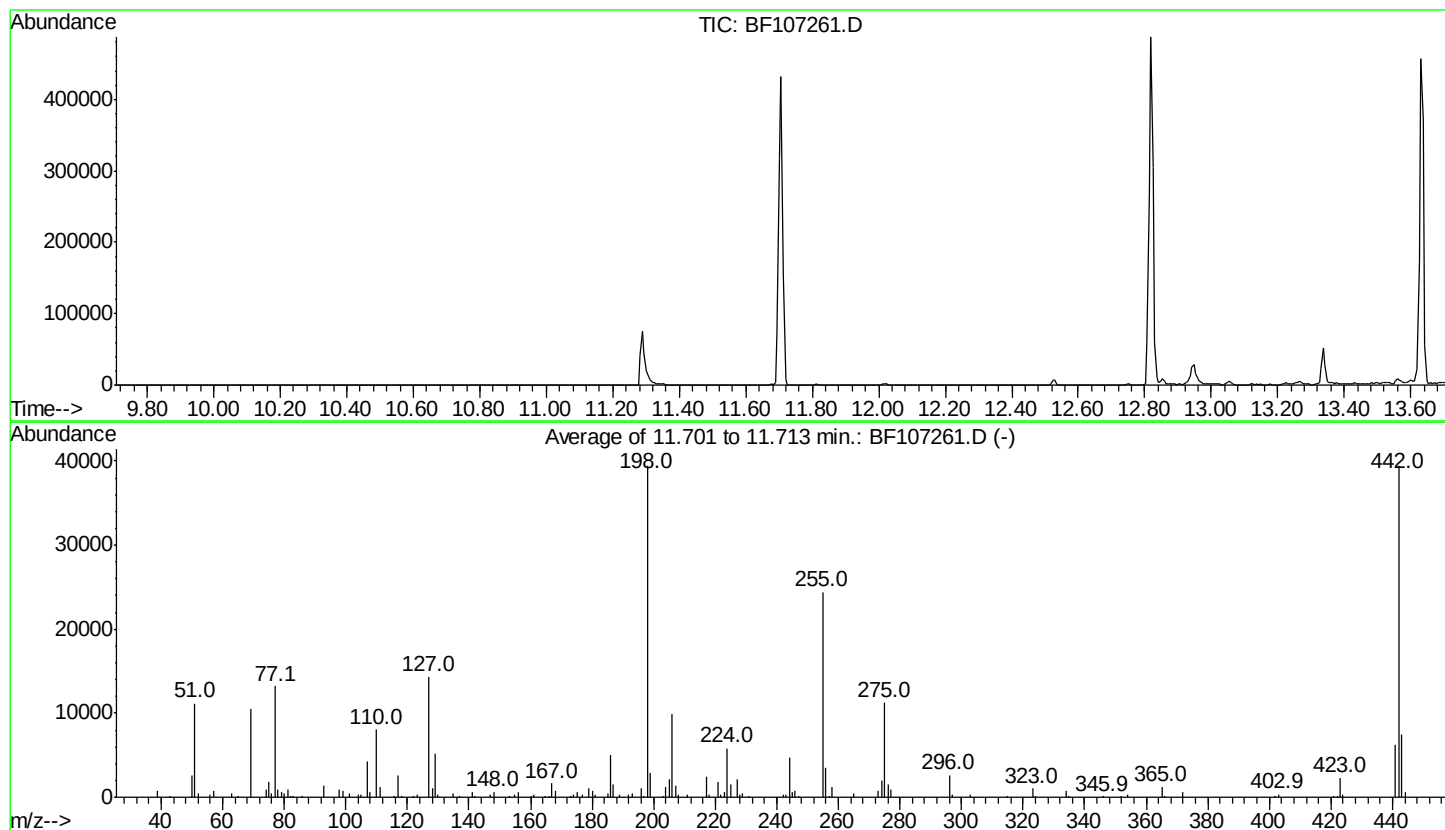

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1587

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	11146	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.7	10525	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.4	14375	PASS
197	198	0.00	2	0.3	108	PASS
198	198	100	100	100.0	39453	PASS
199	198	5	9	7.2	2836	PASS
275	198	10	60	28.4	11217	PASS
365	198	1	100	3.3	1297	PASS
441	198	0.01	100	15.9	6276	PASS
442	198	50	100	100.0	39442	PASS
443	442	15	24	18.8	7433	PASS