


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF071018\
Data File : BF107288.D
Acq On : 10 Jul 2018 23:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF061918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jun 29 14:38:29 2018

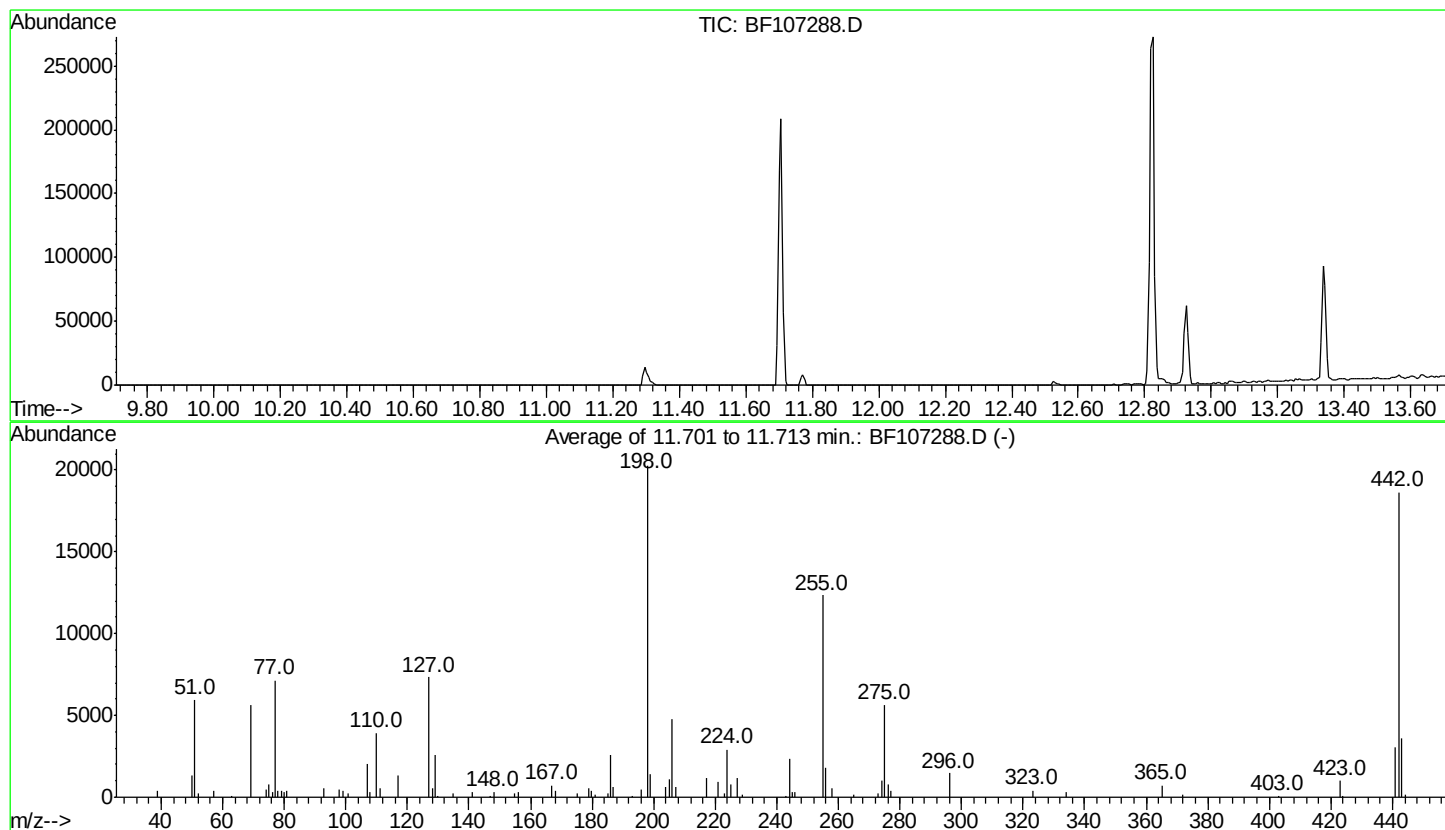

AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	5975	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	27.7	5621	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	36.1	7324	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20266	PASS
199	198	5	9	7.0	1411	PASS
275	198	10	60	27.9	5651	PASS
365	198	1	100	3.5	716	PASS
441	198	0.01	100	14.9	3025	PASS
442	198	50	100	92.0	18641	PASS
443	442	15	24	19.2	3587	PASS