
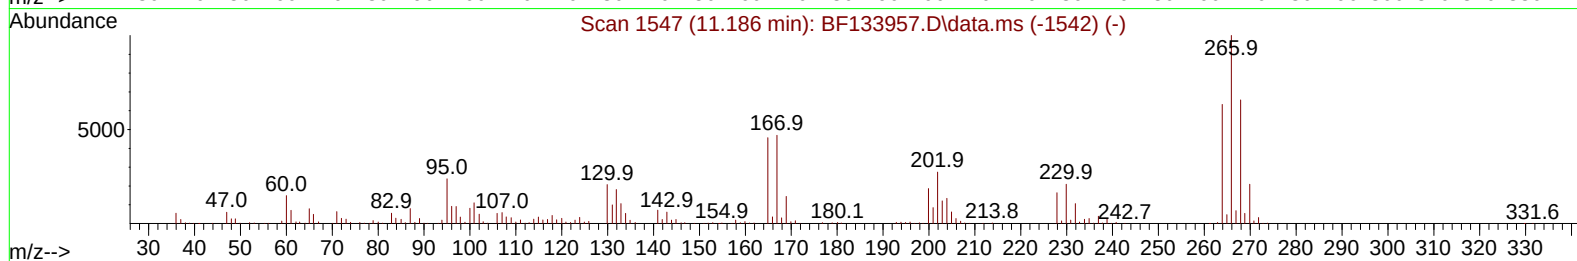
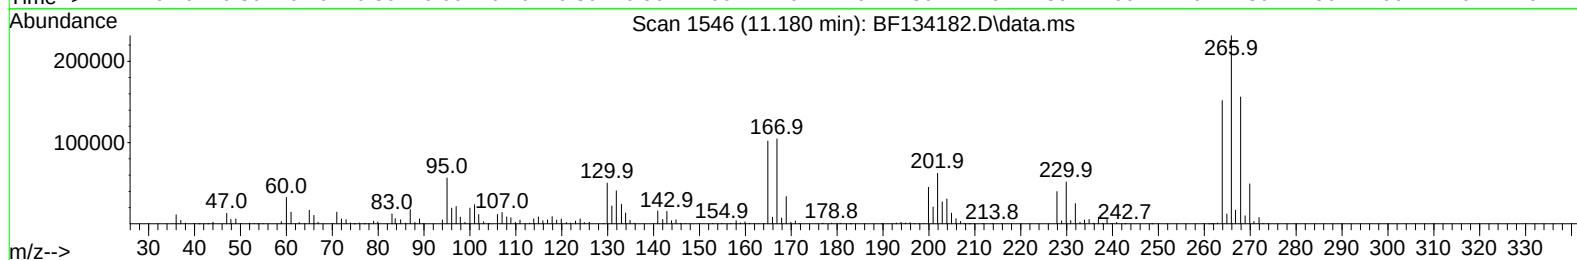


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF071023\  
Data File : BF134182.D  
Acq On : 10 Jul 2023 12:16  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 16:37:53 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF062623.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jun 30 18:35:29 2023  
Response via : Initial Calibration

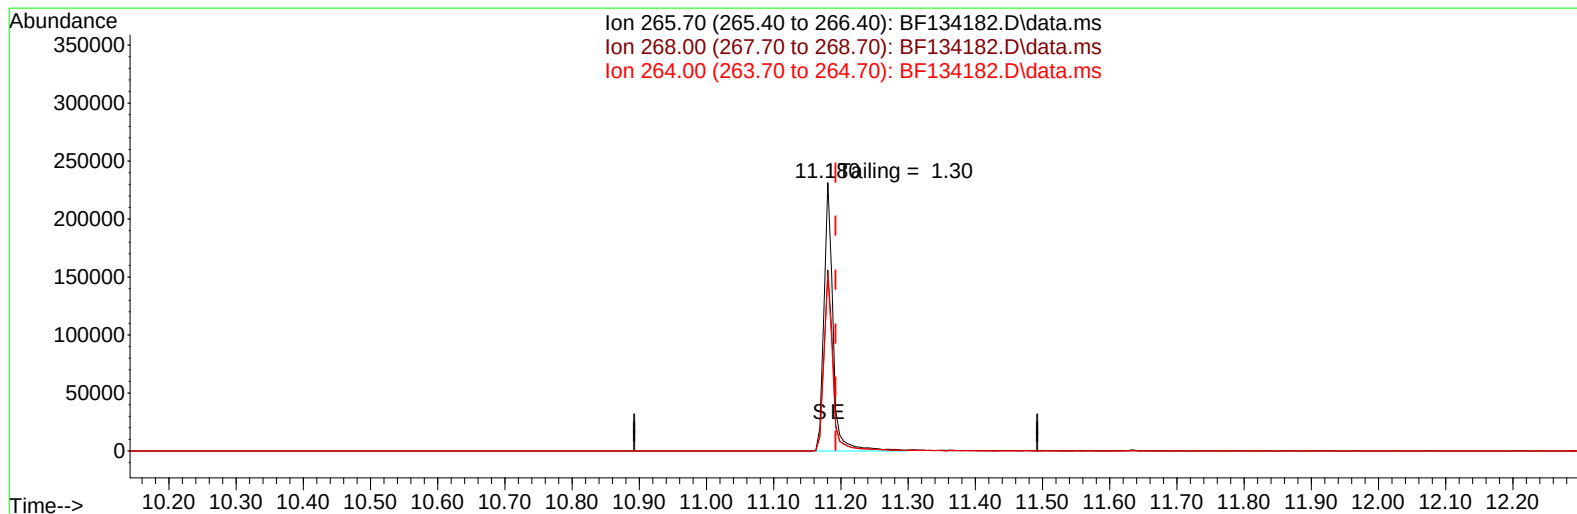

TIC: BF134182.D\data.ms

**(70) Pentachlorophenol (C)**




**11.180min (-0.012) 28675.39 ng**

**response 218646**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.80  | 67.42  |
| 264.00 | 63.30  | 65.57  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF071023\  
Data File : BF134182.D  
Acq On : 10 Jul 2023 12:16  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 10 16:37:53 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF062623.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jun 30 18:35:29 2023  
Response via : Initial Calibration

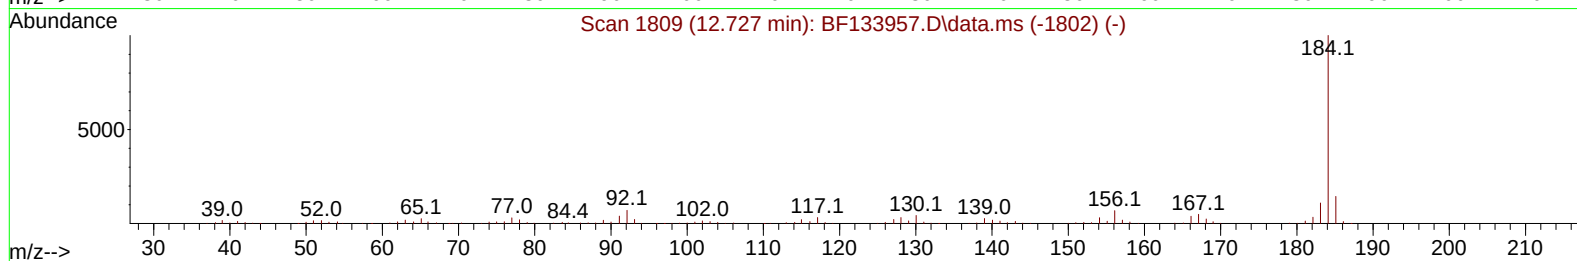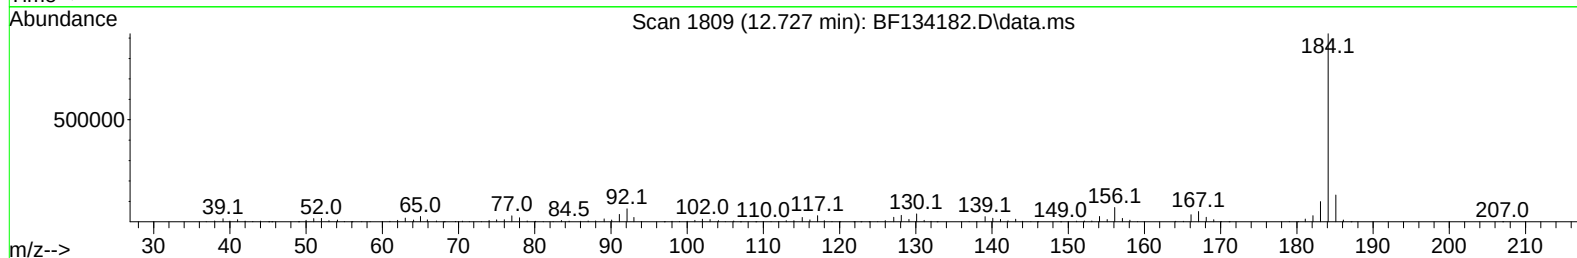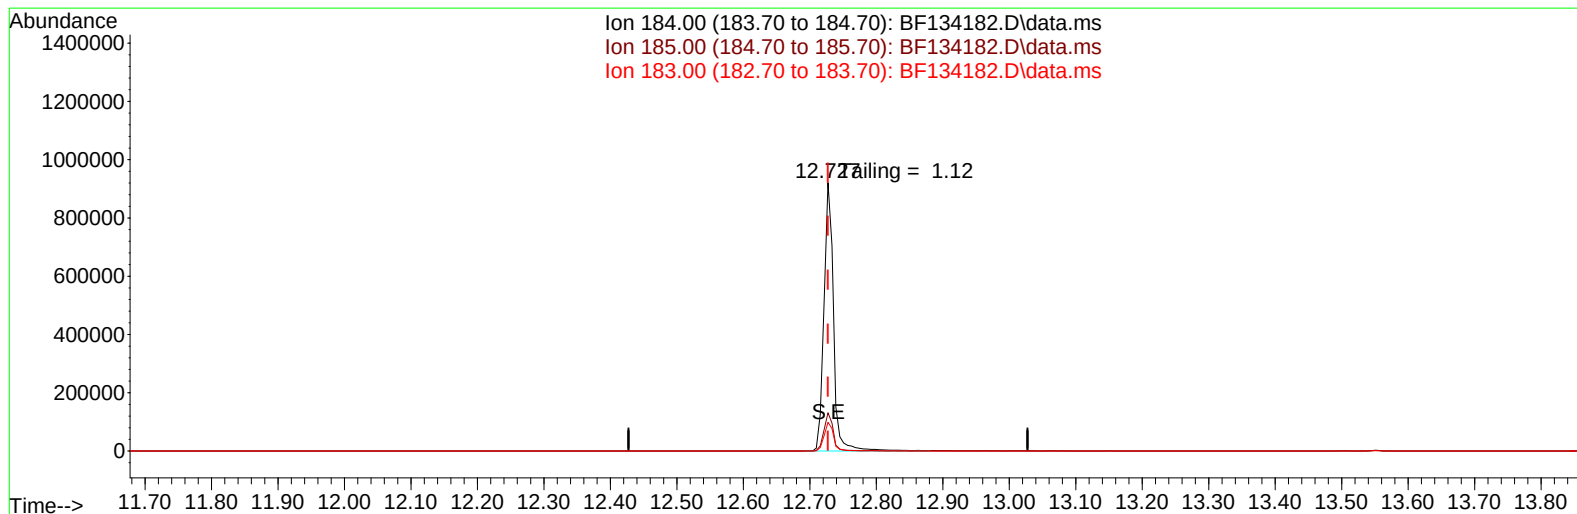

TIC: BF134182.D\data.ms

**(77) Benzidine**

12.727min (-0.000) 0.00 ng

response 924359

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.50  | 14.26  |
| 183.00 | 11.00  | 10.72  |
| 0.00   | 0.00   | 0.00   |